

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120219\
 Data File : VW014207.D
 Acq On : 02 Dec 2019 16:47
 Operator : SY/VA
 Sample : K6063-21
 Misc : 5.10G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 03 10:07:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 03 10:03:32 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	280230	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	287023	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	161801	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	76371	17.08	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	68.32%
7) Chloroethane-d5	2.89	69	68391	18.87	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.48%
10) 1,1-Dichloroethene-d2	4.01	63	124158	13.53	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	54.12%
20) 2-Butanone-d5	7.07	46	71210	54.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	109.64%
24) Chloroform-d	7.64	84	199547	23.16	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	92.64%
26) 1,2-Dichloroethane-d4	8.30	65	111949	25.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.36%
29) Benzene-d6	8.27	84	399548	19.62	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	78.48%
33) 1,2-Dichloropropane-d6	9.27	67	128453	21.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	86.12%
37) Toluene-d8	10.32	98	366464	18.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	75.92%
38) trans-1,3-Dichloropropene-	10.57	79	52815	20.67	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.68%
39) 2-Hexanone-d5	10.92	63	58617	51.82	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	103.64%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	117501	26.08	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.32%
61) 1,2-Dichlorobenzene-d4	13.85	152	143775	22.12	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	88.48%


Target Compounds					Ovalue
42) cis-1,3-Dichloropropene	10.03	75	2995	0.374 ug/L	# 68


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW120219\
Data File : VW014207.D
Acq On : 02 Dec 2019 16:47
Operator : SY/VA
Sample : K6063-21
Misc : 5.10G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 03 10:07:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM111119S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 03 10:03:32 2019
Response via : Initial Calibration

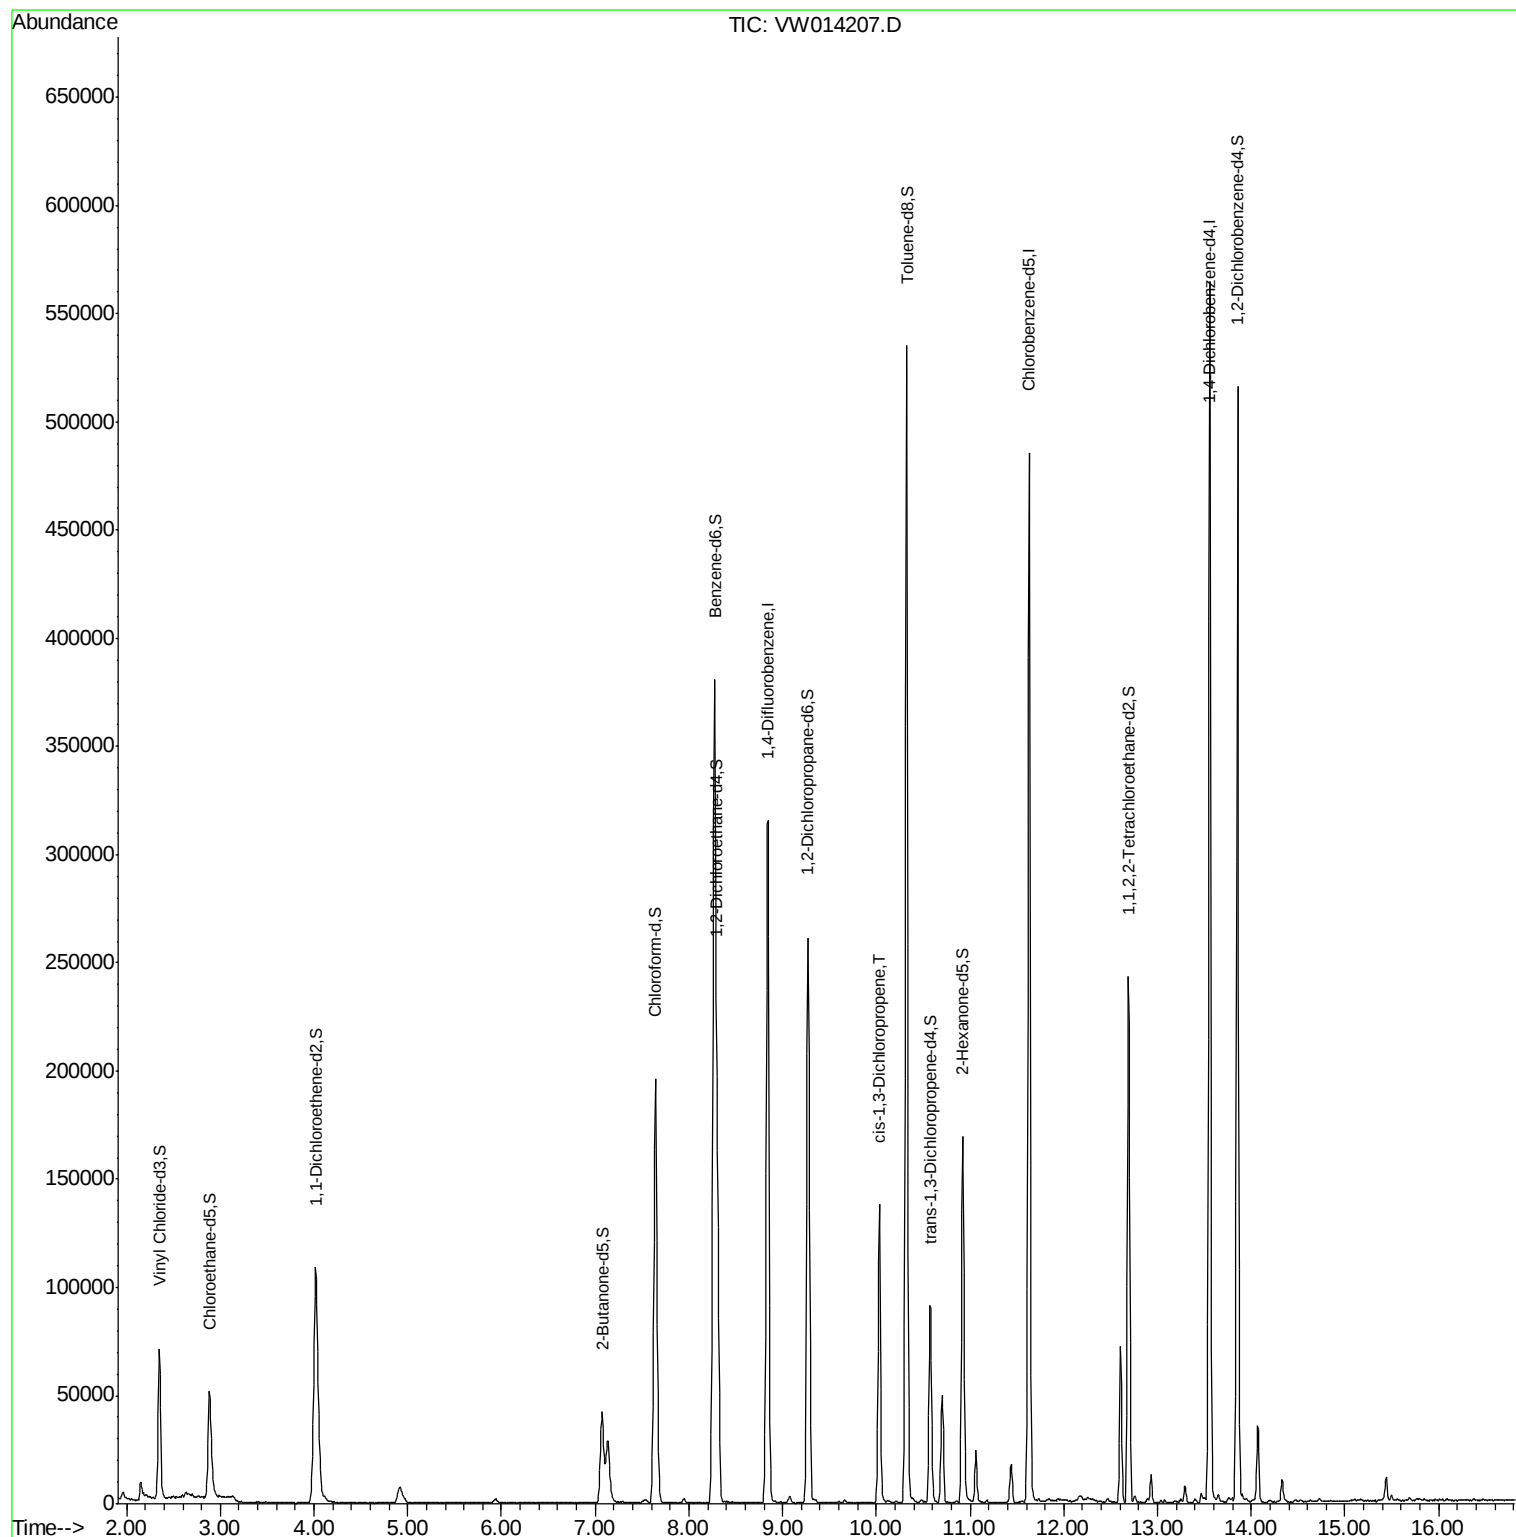

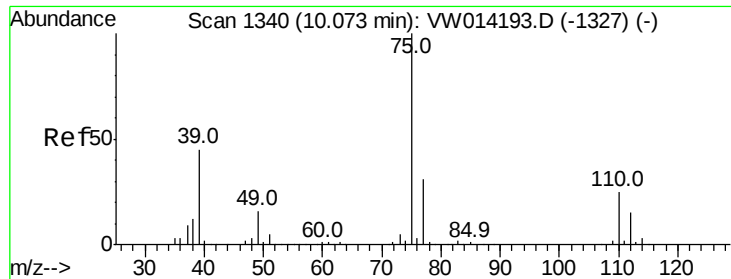

#42
 cis-1,3-Dichloropropene
 Concen: 0.374 ug/L
 RT: 10.03 min Scan# 1333
 Delta R.T. -0.04 min
 Lab File: VW014207.D
 Acq: 02 Dec 2019 16:47

Instrument :
 MSVOA_W
 ClientSampleId :

Tot Ion: 75 Resp: 2995
 Ion Ratio Lower Upper
 75 100
 77 49.6 22.1 41.1#

