

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021018.D
 Acq On : 02 Dec 2021 02:40
 Operator : SY/VA
 Sample : M4881-06
 Misc : 4.62g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9E2

Manual IntegrationsAPPROVED

Quant Time: Dec 02 07:29:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/03/2021
 Supervised By :Amit Patel 12/07/2021

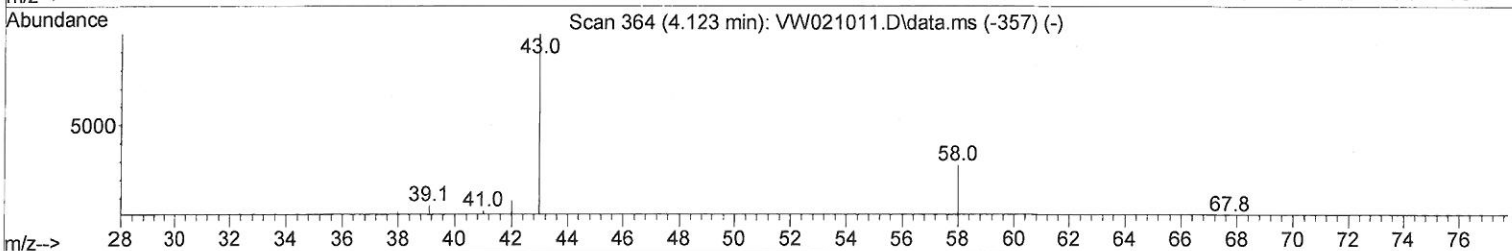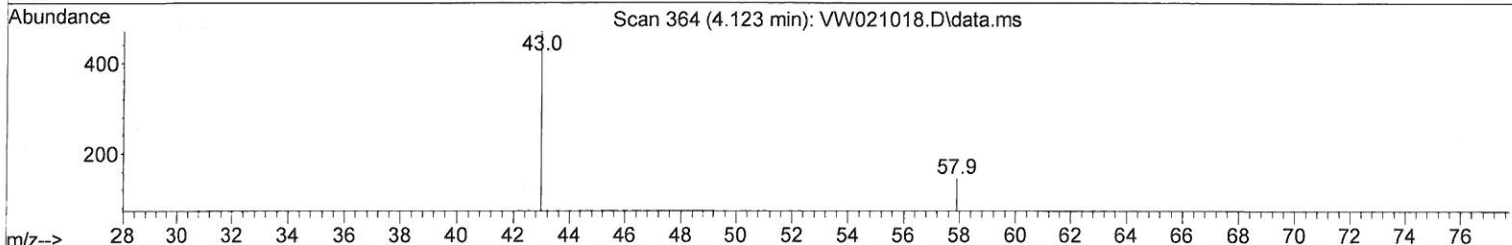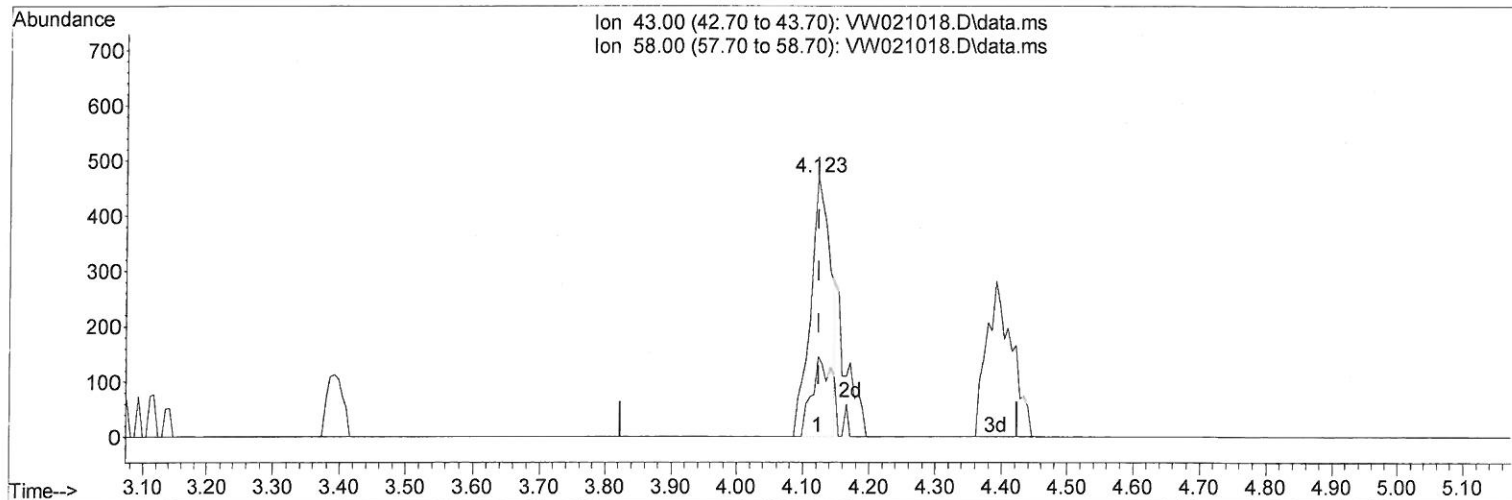

TIC: VW021018.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 4.59 ug/L

response 1003

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	8.97
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021018.D
 Acq On : 02 Dec 2021 02:40
 Operator : SY/VA
 Sample : M4881-06
 Misc : 4.62g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9E2

Manual IntegrationsAPPROVED

Quant Time: Dec 02 07:29:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/03/2021
 Supervised By :Amit Patel 12/07/2021

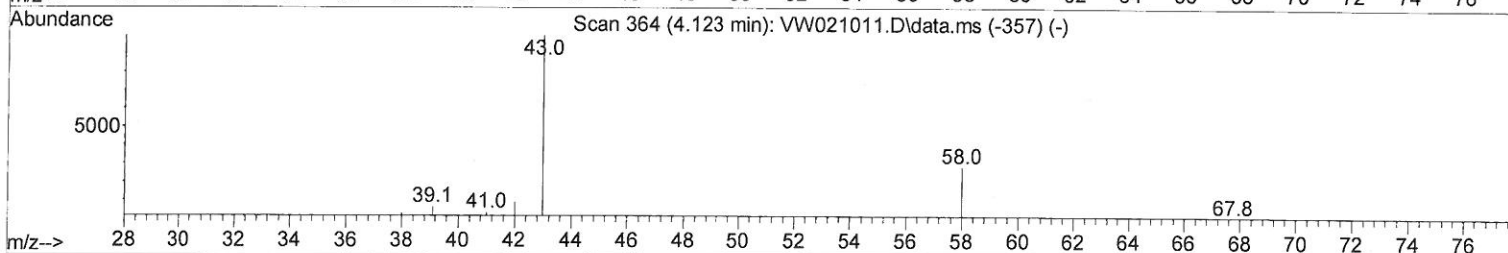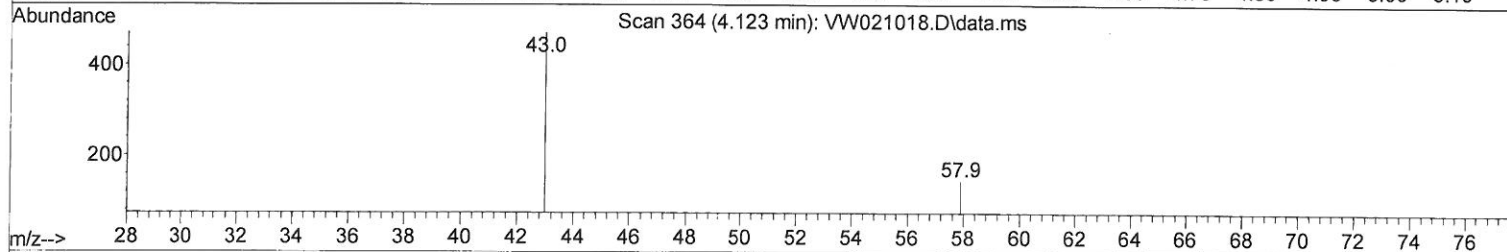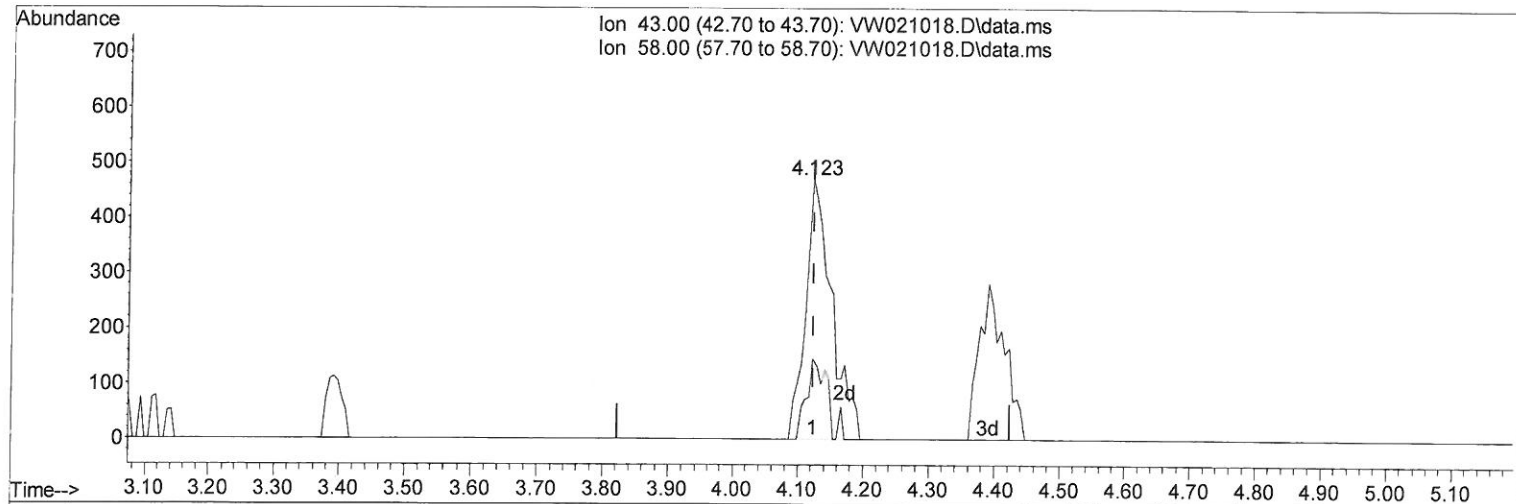

TIC: VW021018.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 5.95 ug/L m

response 1301

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	6.92
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021018.D
 Acq On : 02 Dec 2021 02:40
 Operator : SY/VA
 Sample : M4881-06
 Misc : 4.62g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9E2

Manual IntegrationsAPPROVED

Quant Time: Dec 02 07:29:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/03/2021
 Supervised By :Amit Patel 12/07/2021

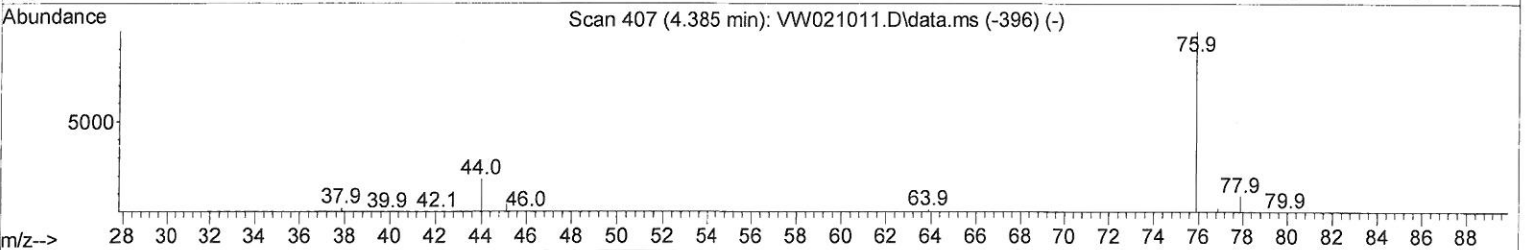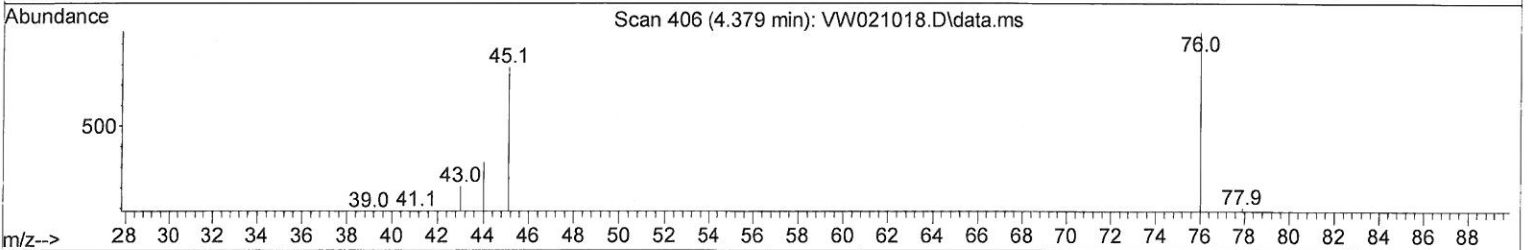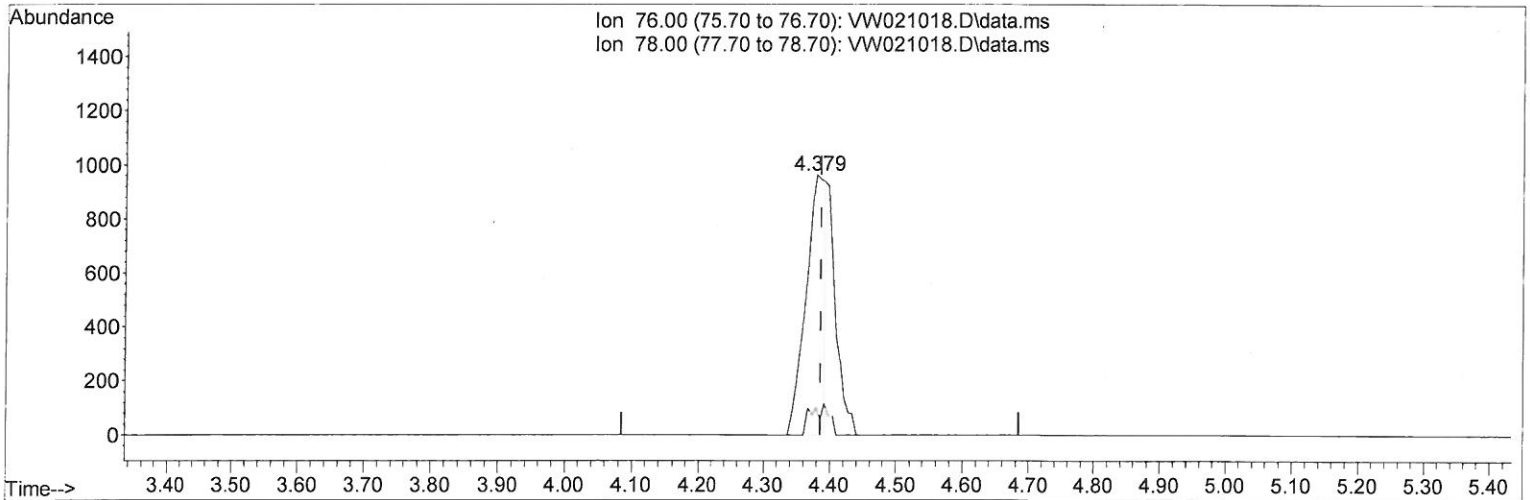

TIC: VW021018.D\data.ms

(14) Carbon disulfide (T)

4.379min (-0.006) 0.68 ug/L

response 1947

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	8.90	10.60
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021018.D
 Acq On : 02 Dec 2021 02:40
 Operator : SY/VA
 Sample : M4881-06
 Misc : 4.62g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9E2

Manual IntegrationsAPPROVED

Quant Time: Dec 02 07:29:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/03/2021
 Supervised By :Amit Patel 12/07/2021

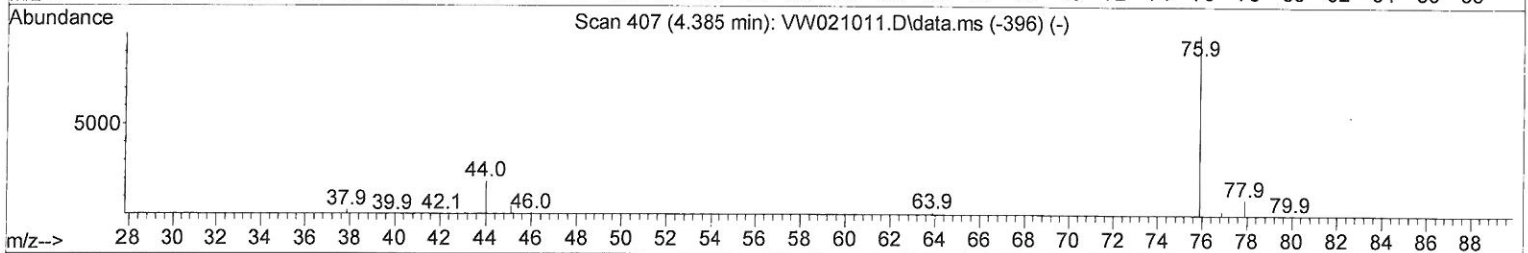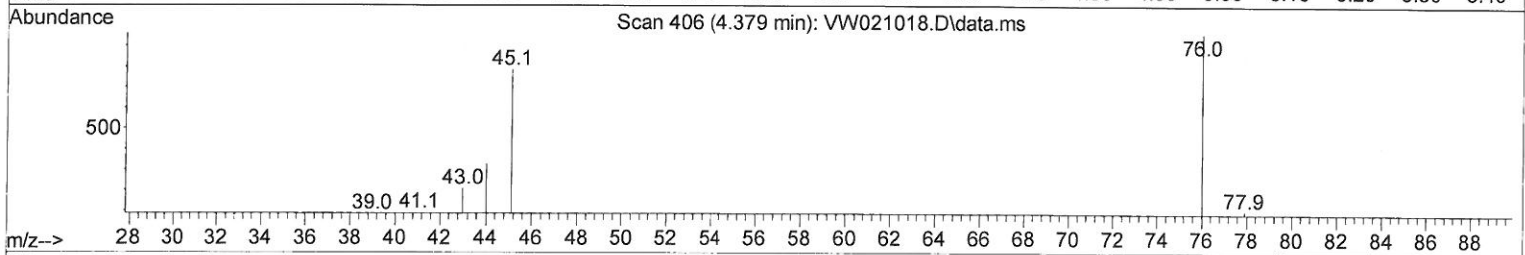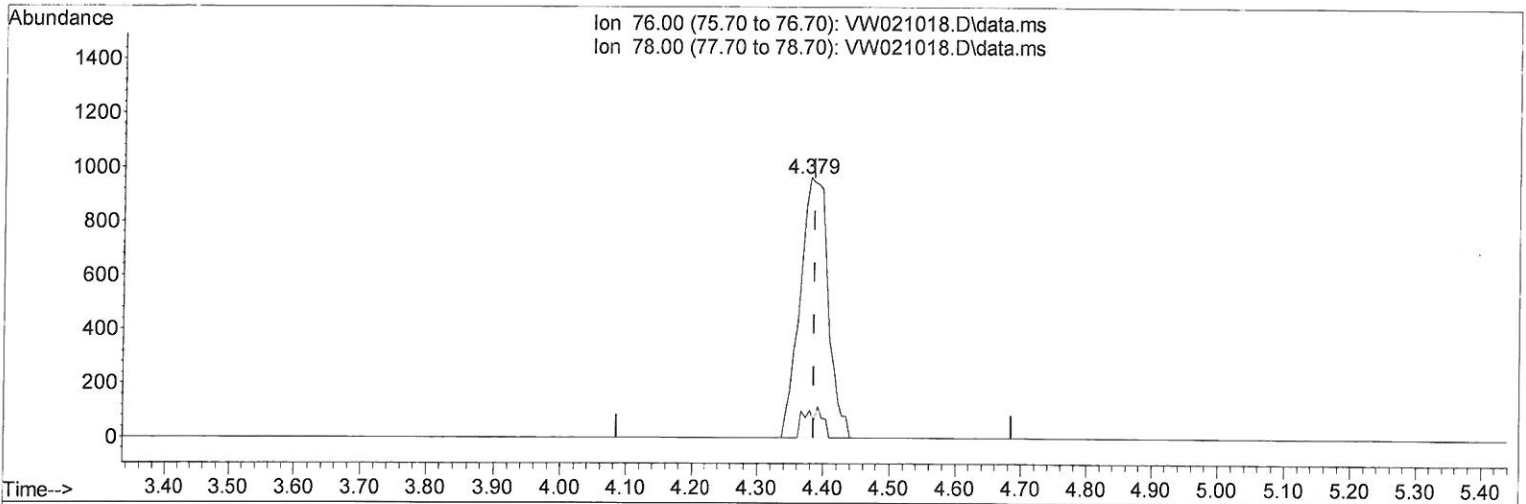

TIC: VW021018.D\data.ms

(14) Carbon disulfide (T)

4.379min (-0.006) 0.99 ug/L m

response 2841

Ion	Exp%	Act%
76.00	100.00	100.00
78.00	8.90	10.60
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021018.D
 Acq On : 02 Dec 2021 02:40
 Operator : SY/VA
 Sample : M4881-06
 Misc : 4.62g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9E2

Manual IntegrationsAPPROVED

Quant Time: Dec 02 07:29:58 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/03/2021
 Supervised By :Amit Patel 12/07/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	84535	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	70910	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	27885	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	13975	14.252	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	57.000%	
7) Chloroethane-d5	2.891	69	11202	17.713	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	70.840%	
11) 1,1-Dichloroethene-d2	4.013	63	21624	11.398	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	45.600%	
21) 2-Butanone-d5	7.080	46	12048	49.226	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	98.460%	
24) Chloroform-d	7.653	84	49339	23.164	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	92.640%	
26) 1,2-Dichloroethane-d4	8.311	65	28320	26.194	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	104.760%	
32) Benzene-d6	8.275	84	81979	21.935	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	87.760%	
36) 1,2-Dichloropropane-d6	9.274	67	28284	26.577	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	106.320%	
41) Toluene-d8	10.323	98	72266	19.482	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	77.920%	
43) trans-1,3-Dichloroprop...	10.579	79	9719	19.321	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	77.280%	
47) 2-Hexanone-d5	10.927	63	9004	51.013	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	102.020%	
56) 1,1,2,2-Tetrachloroeth...	12.695	84	21675	26.586	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	106.360%	
66) 1,2-Dichlorobenzene-d4	13.853	152	21188	21.319	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	85.280%	
Target Compounds						
13) Acetone	4.123	43	1301m	5.954	ug/L	Qvalue
14) Carbon disulfide	4.379	76	2841m	0.992	ug/L	
16) Methylene chloride	4.922	84	5266	4.467	ug/L	89
53) m,p-Xylene	11.841	106	1725	0.844	ug/L	60
63) 1,2,4-Trimethylbenzene	13.249	105	1556	0.492	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
Data File : VW021018.D
Acq On : 02 Dec 2021 02:40
Operator : SY/VA
Sample : M4881-06
Misc : 4.62g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW9E2

Manual IntegrationsAPPROVED

Quant Time: Dec 02 07:29:58 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 02 07:10:34 2021
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/03/2021
Supervised By :Amit Patel 12/07/2021

