

Quantitation Report (QT/LSC Reviewed)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021030.D
 Acq On : 02 Dec 2021 07:29
 Operator : SY/VA
 Sample : M4881-18
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 EW9F4

Quant Time: Dec 03 00:23:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 Qlast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/03/2021
 Supervised By : Amit Patel 12/07/2021

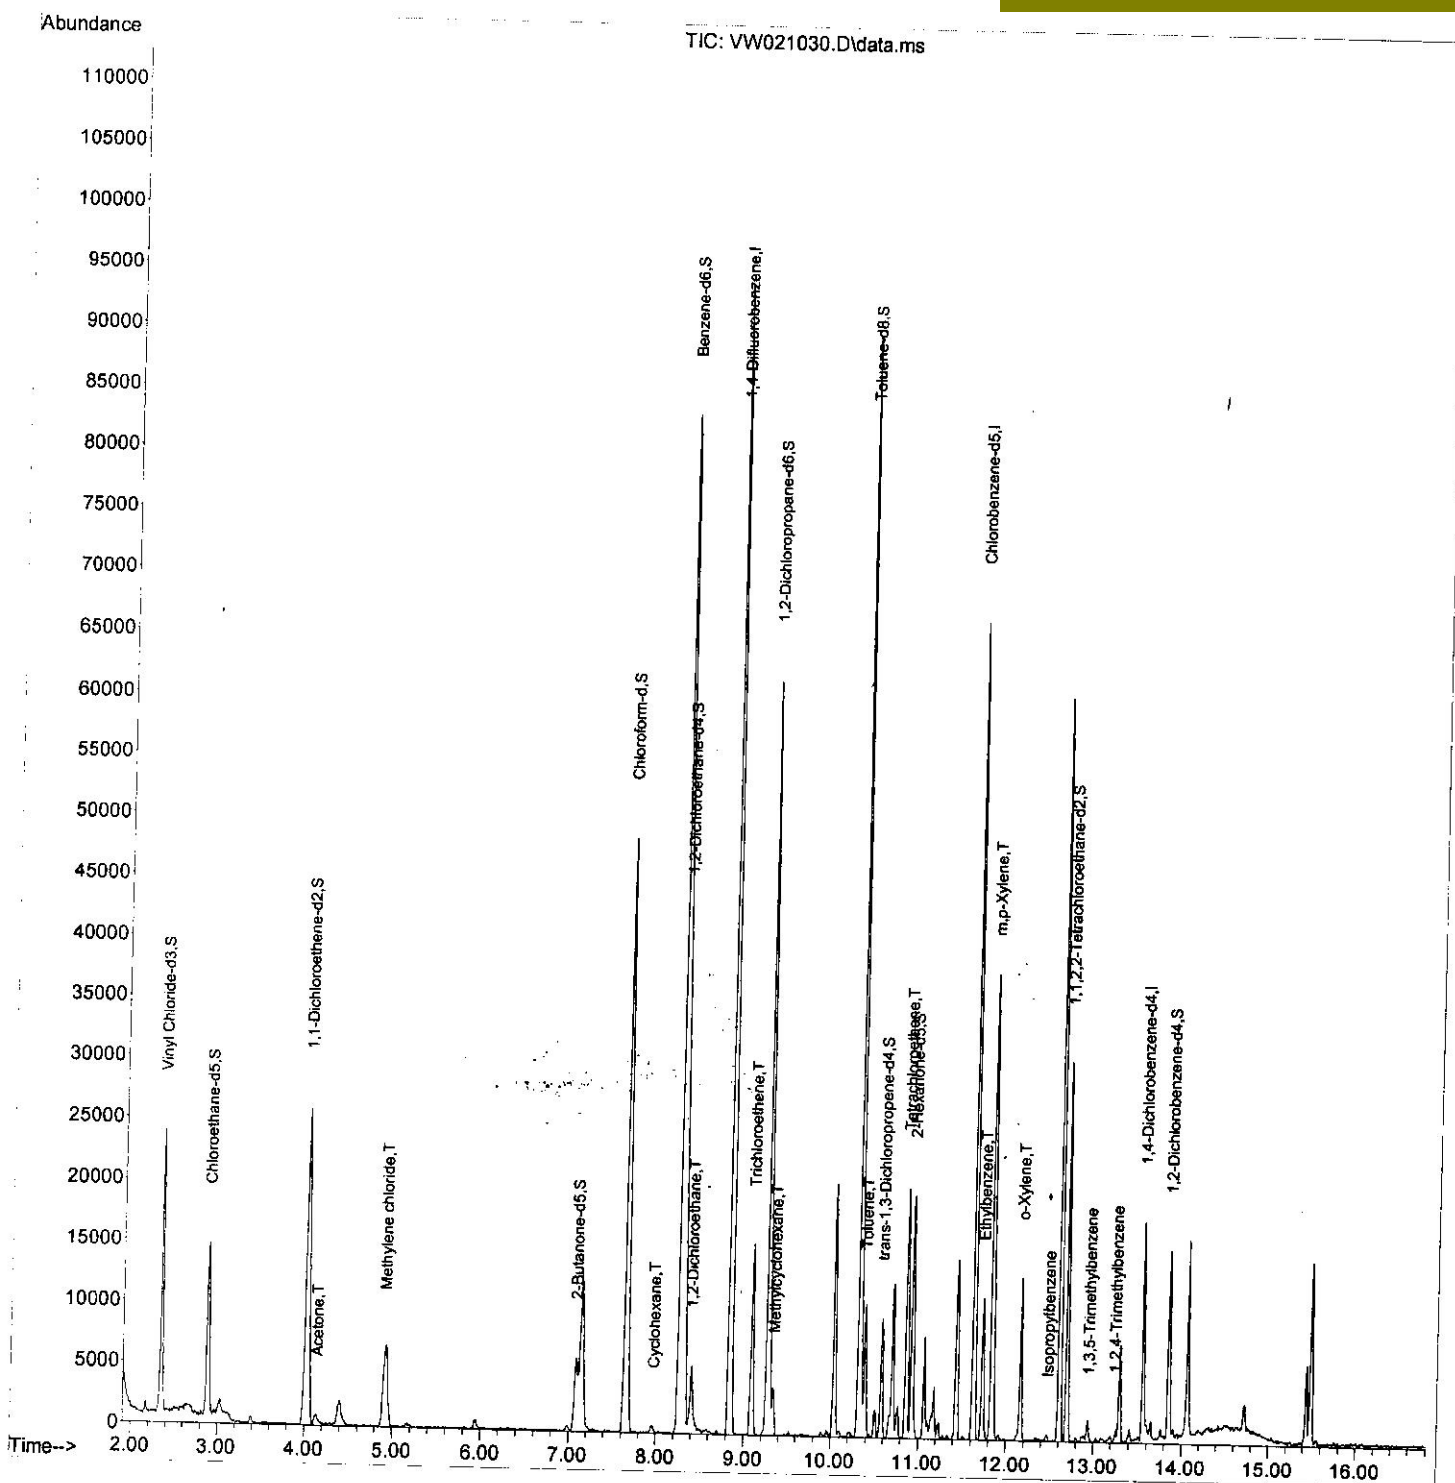

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021030.D
 Acq On : 02 Dec 2021 07:29
 Operator : SY/VA
 Sample : M4881-18
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 EW9F4

Quant Time: Dec 03 00:23:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 Qlast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/03/2021
 Supervised By :Amit Patel 12/07/2021

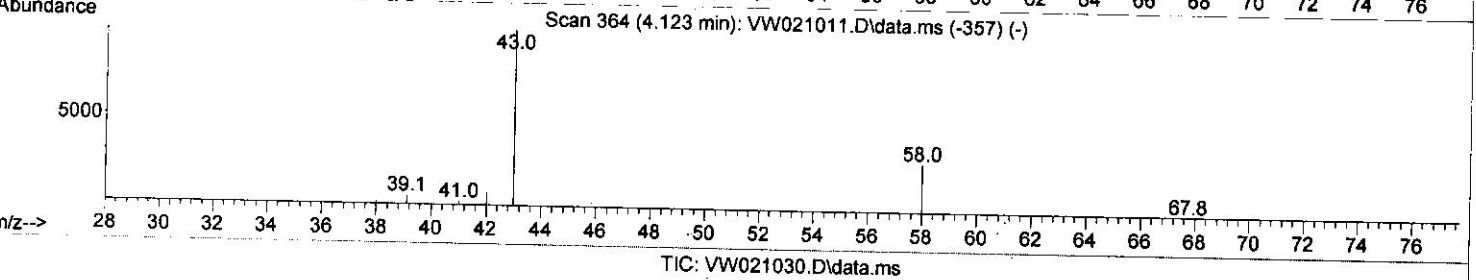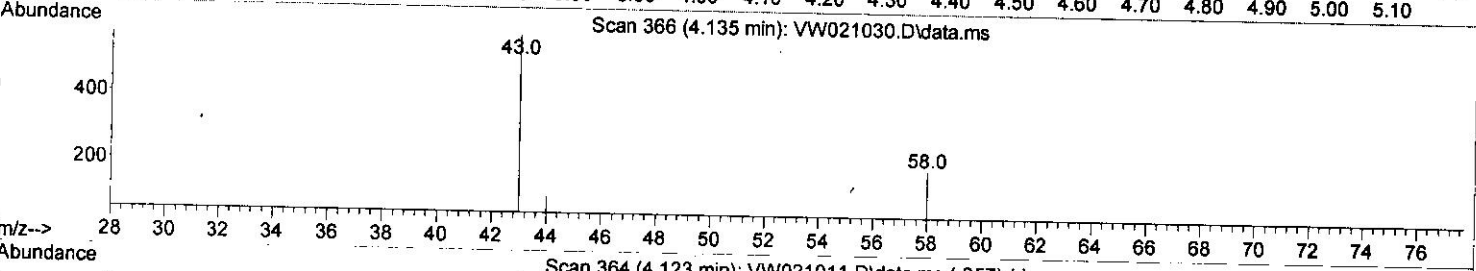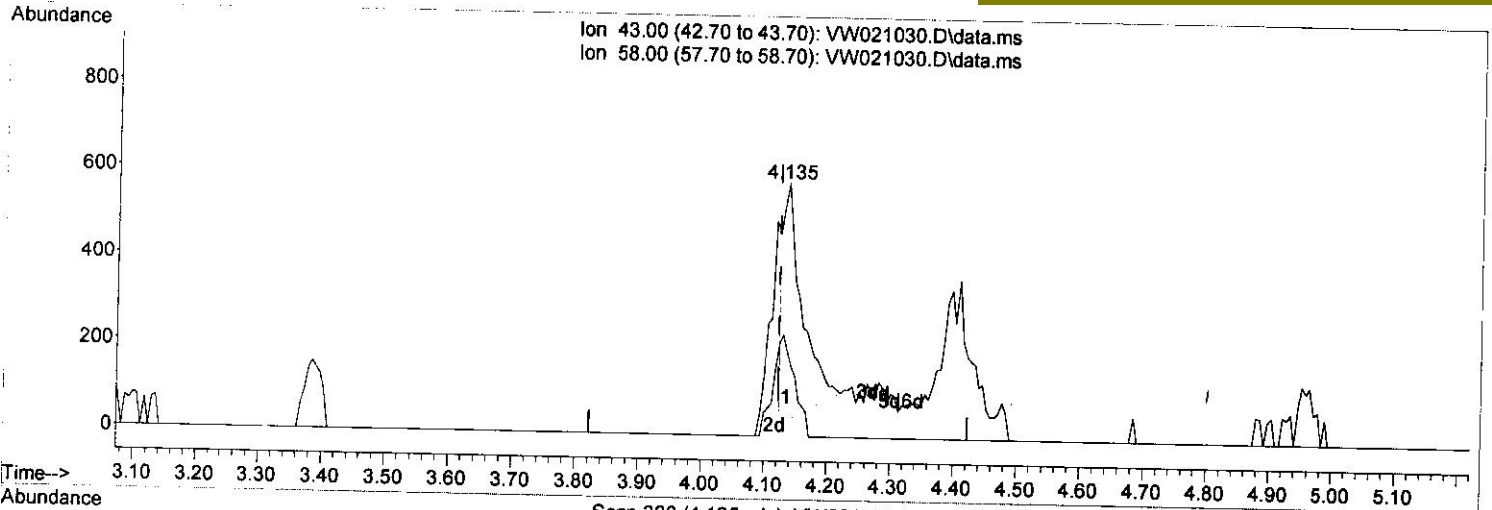

(13) Acetone (T)

4.135min (+ 0.012) 5.33 ug/L

response 1113

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	48.97
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021030.D
 Acq On : 02 Dec 2021 07:29
 Operator : SY/VA
 Sample : M4881-18
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 EW9F4

Quant Time: Dec 03 00:23:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/03/2021
 Supervised By : Amit Patel 12/07/2021

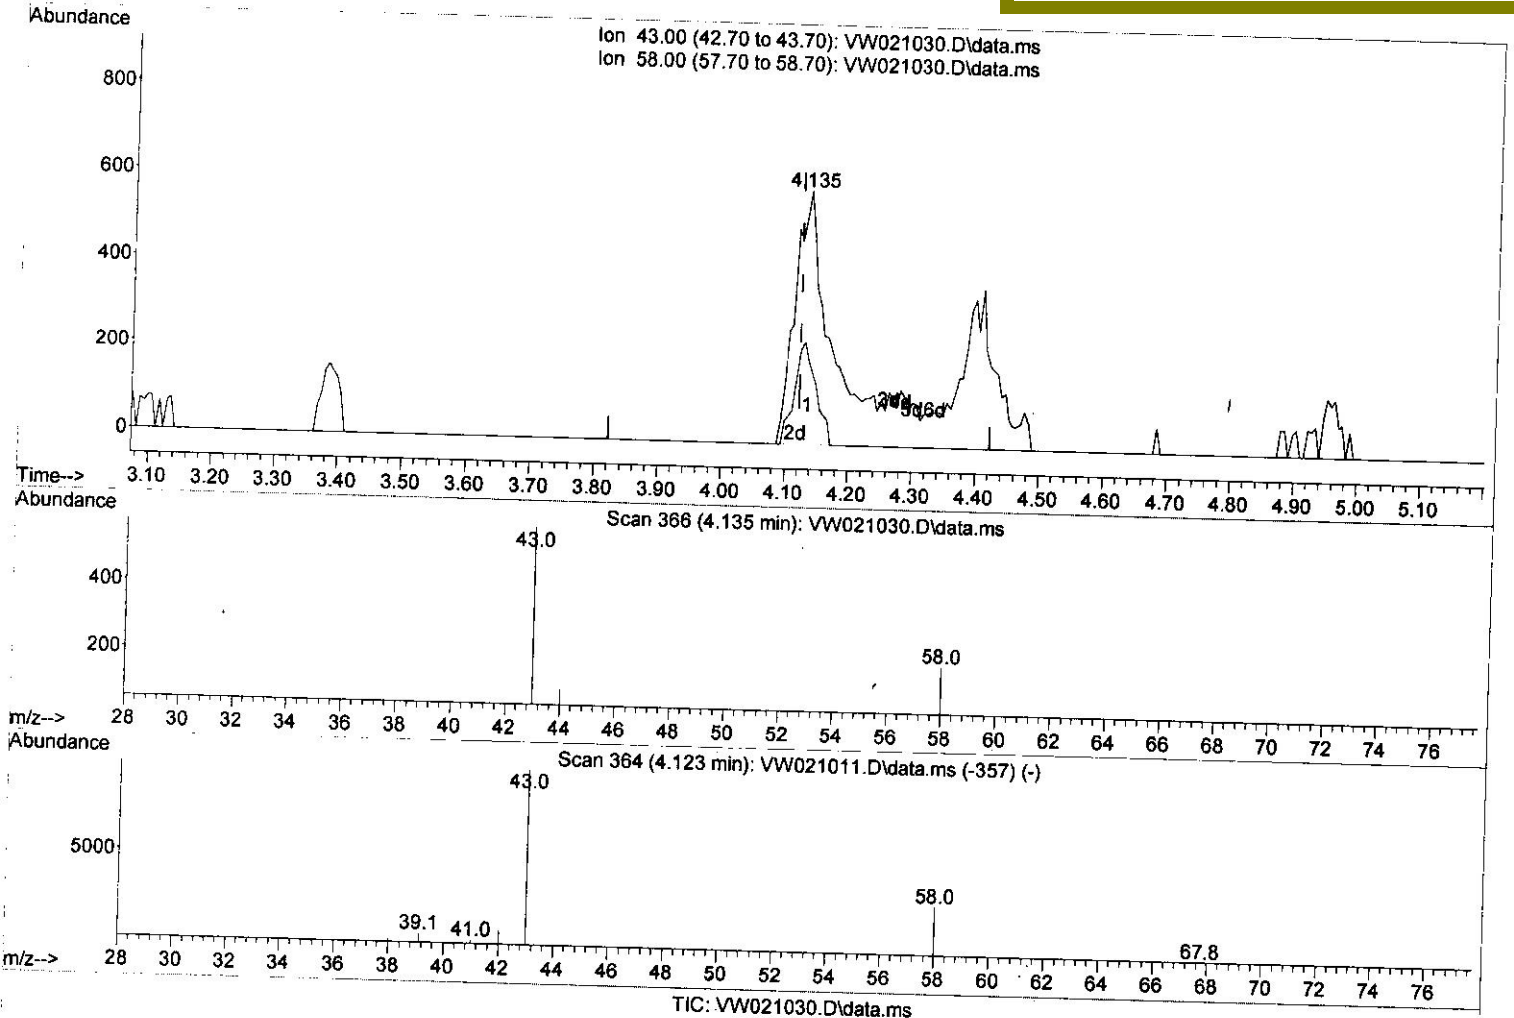

(13) Acetone (T)

4.135min (+ 0.012) 9.52 ug/L m } mp 12/11/21

response 1988

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	27.41
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021030.D
 Acq On : 02 Dec 2021 07:29
 Operator : SY/VA
 Sample : M4881-18
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 EW9F4

Quant Time: Dec 03 00:23:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/03/2021
 Supervised By :Amit Patel 12/07/2021

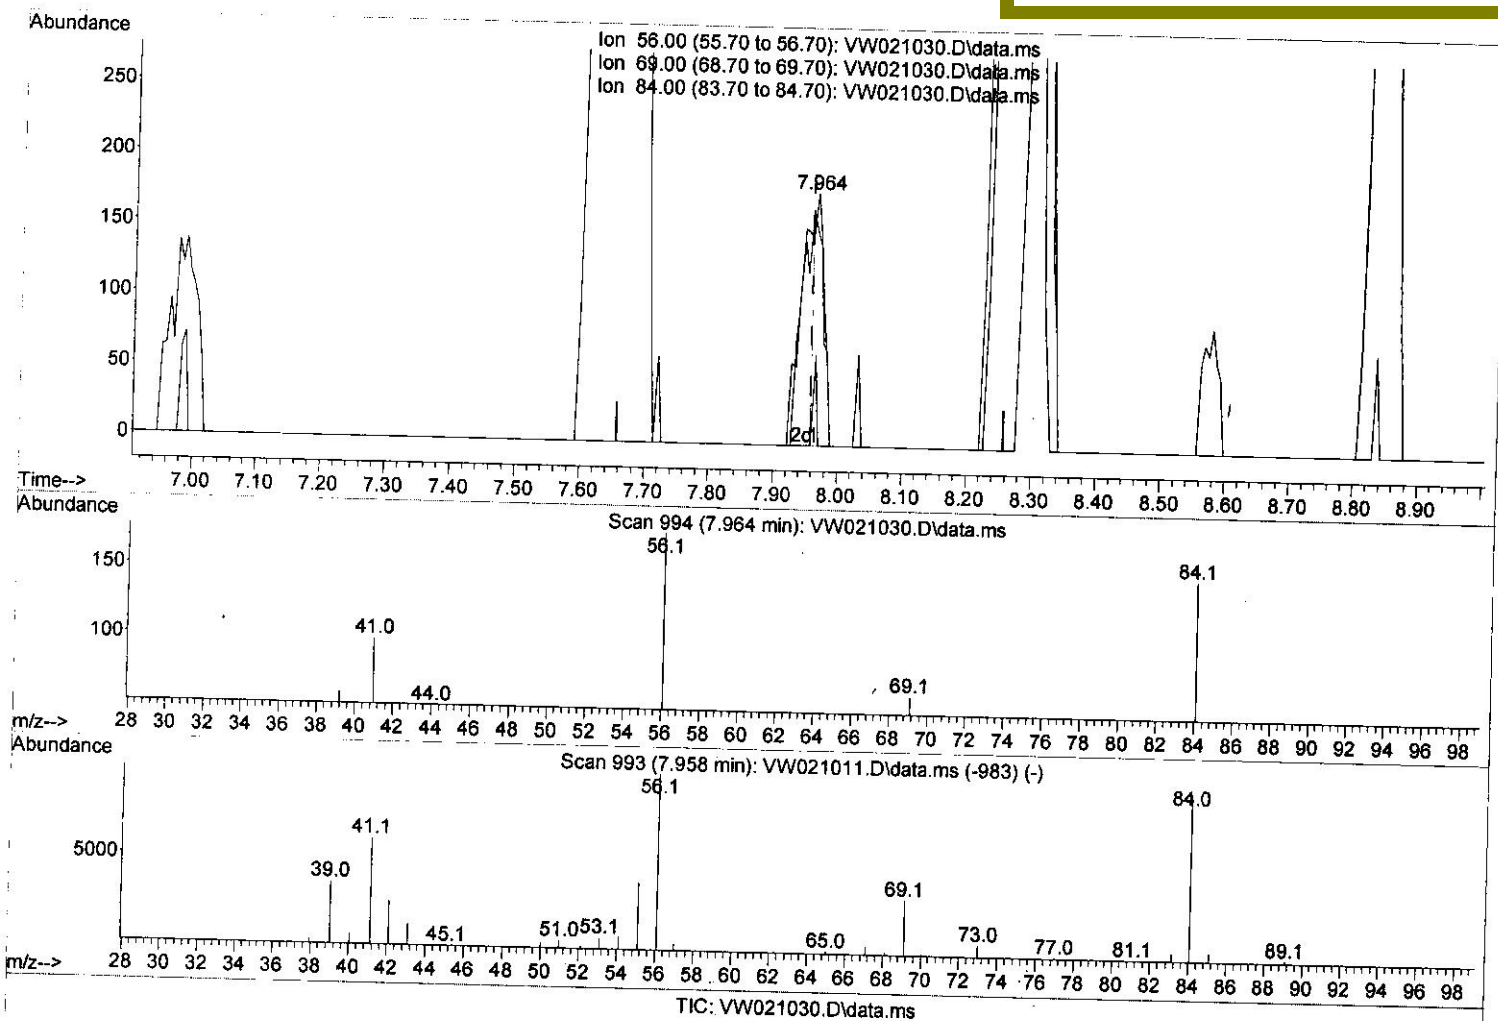

(29) Cyclohexane (T)

7.964min (+ 0.006) 0.22 ug/L

response 177

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	29.40	0.00#
84.00	79.30	215.25#
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021030.D
 Acq On : 02 Dec 2021 07:29
 Operator : SY/VA
 Sample : M4881-18
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 EW9F4

Quant Time: Dec 03 00:23:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/03/2021
 Supervised By : Amit Patel 12/07/2021

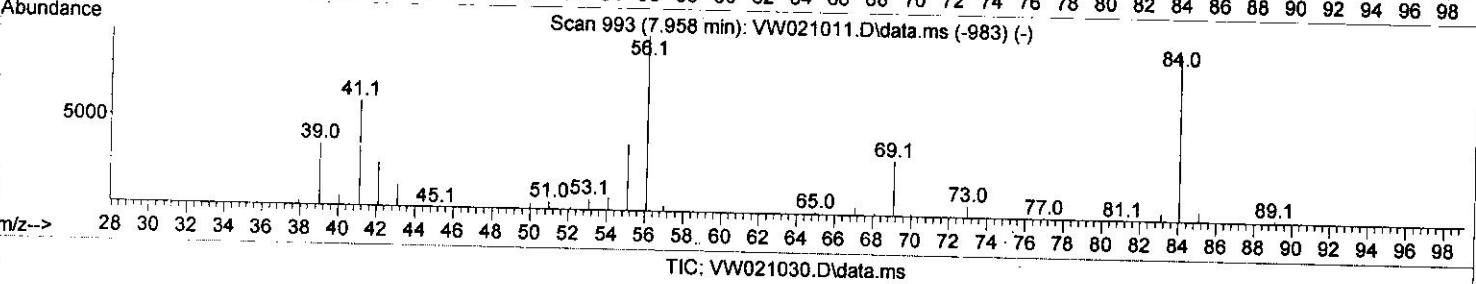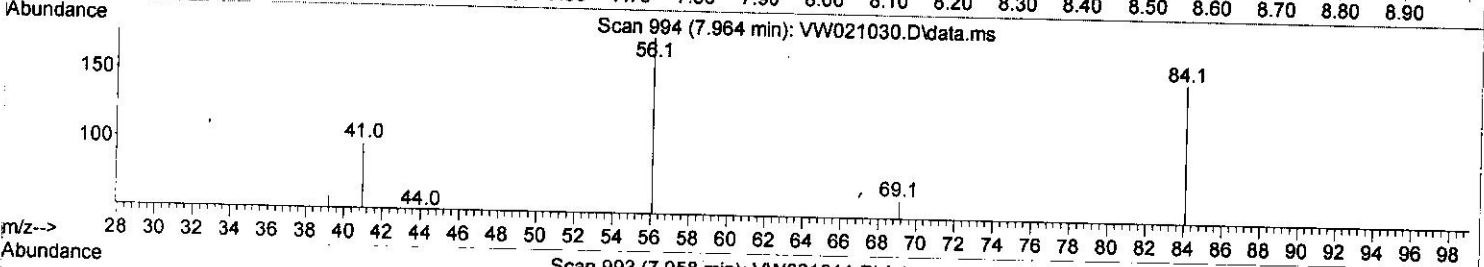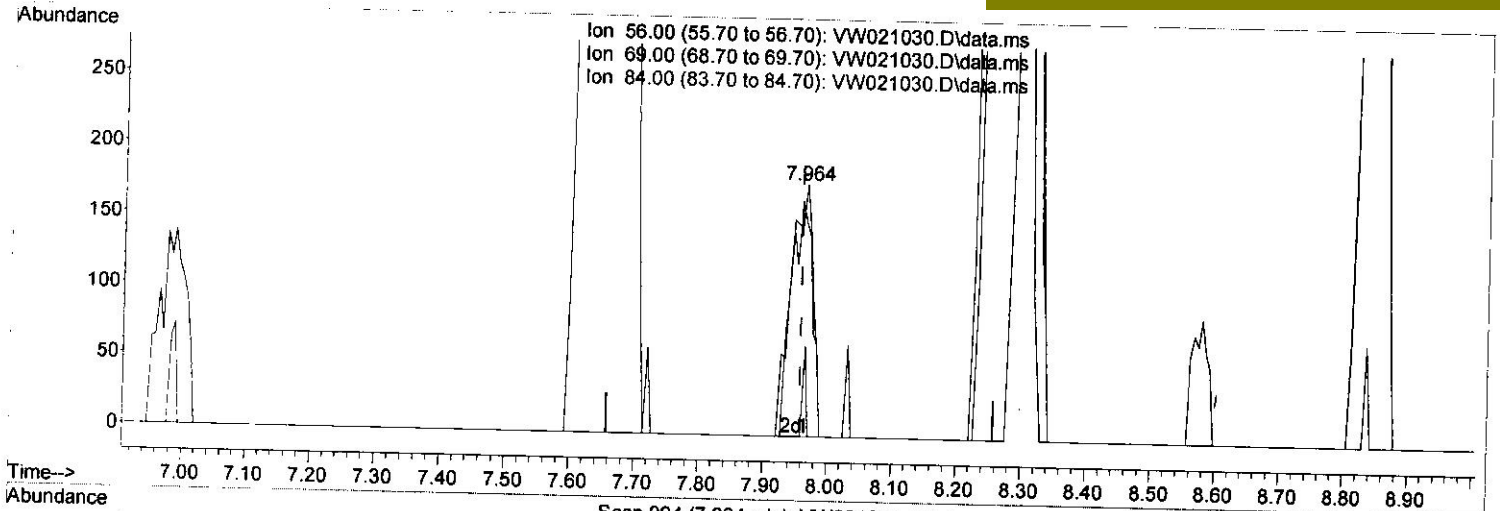

TIC: VW021030.D\data.ms

(29) Cyclohexane (T)

7.964min (+ 0.006) 0.52 ug/L m

Handwritten: 3 m.p. 12/11/21

response 422

Ion	Exp%	Act%
56.00	100.00	100.00
69.00	29.40	0.00#
84.00	79.30	90.28
0.00	0.00	0.00

Quantitation Report (QT/LSC Reviewed)

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021030.D
 Acq On : 02 Dec 2021 07:29
 Operator : SY/VA
 Sample : M4881-18
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 EW9F4

Quant Time: Dec 03 00:23:33 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 02 07:10:34 2021
 Response via : Initial Calibration

Manual Integrations APPROVED

Reviewed By : Semsettin Yesilyurt 12/03/2021
 Supervised By : Amit Patel 12/07/2021

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	80815	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	36569	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	4792	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	20484	21.852	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	87.400%	
7) Chloroethane-d5	2.885	69	15629	25.851	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	=	103.400%	
11) 1,1-Dichloroethene-d2	4.019	63	23962	13.212	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	=	52.840%	
21) 2-Butanone-d5	7.080	46	10782	46.081	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	92.160%	
24) Chloroform-d	7.647	84	49237	24.180	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	=	96.720%	
26) 1,2-Dichloroethane-d4	8.305	65	23488	22.725	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	=	90.880%	
32) Benzene-d6	8.275	84	81792	42.437	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	=	169.760%#	
36) 1,2-Dichloropropane-d6	9.275	67	26281	47.885	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	=	191.520%#	
41) Toluene-d8	10.323	98	56258	29.408	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	=	117.640%	
43) trans-1,3-Dichloroprop...	10.579	79	5034	19.405	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	=	77.640%	
47) 2-Hexanone-d5	10.927	63	6590	72.397	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	=	144.800%#	
56) 1,1,2,2-Tetrachloroeth...	12.689	84	14044	33.403	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	=	133.600%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	3956	23.162	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	=	92.640%	
Target Compounds						
13) Acetone	4.135	43	1988m	9.516	ug/L	
16) Methylene chloride	4.916	84	5338	4.736	ug/L	81
27) 1,2-Dichloroethane	8.397	62	4275	3.572	ug/L	97
29) Cyclohexane	7.964	56	422m	0.518	ug/L	
34) Trichloroethene	9.092	95	4910	8.478	ug/L	85
35) Methylcyclohexane	9.342	83	1436	1.504	ug/L #	92
42) Toluene	10.384	91	8240	3.538	ug/L	91
46) Tetrachloroethene	10.860	164	4612	8.673	ug/L	96
52) Ethylbenzene	11.731	91	7833	3.035	ug/L	97
53) m,p-Xylene	11.829	106	11930	11.323	ug/L	82
54) o-Xylene	12.164	106	3424	3.384	ug/L	99
60) Isopropylbenzene	12.469	105	361	0.553	ug/L #	80
62) 1,3,5-Trimethylbenzene	12.945	105	334	0.607	ug/L #	74
63) 1,2,4-Trimethylbenzene	13.243	105	938	1.727	ug/L #	82

(#) = qualifier out of range (m) = manual integration (+) = signals summed