

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
 Data File : VW021038.D
 Acq On : 02 Dec 2021 11:34
 Operator : SY/VA
 Sample : M4868-09
 Misc : 7.30g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGKP4

Quant Time: Dec 03 02:23:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 03 01:25:28 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	126720	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	114886	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	66628	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	25980	17.675	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.680%
7) Chloroethane-d5	2.879	69	19600	20.675	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	82.720%
11) 1,1-Dichloroethene-d2	4.019	63	33153	11.657	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	46.640%
21) 2-Butanone-d5	7.074	46	16247	44.284	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	88.560%
24) Chloroform-d	7.647	84	62544	19.588	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	78.360%
26) 1,2-Dichloroethane-d4	8.305	65	34304	21.166	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	84.680%
32) Benzene-d6	8.275	84	117202	19.356	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	77.440%
36) 1,2-Dichloropropane-d6	9.274	67	35317	20.483	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	81.920%
41) Toluene-d8	10.323	98	114276	19.015	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.040%
43) trans-1,3-Dichloroprop...	10.579	79	14665	17.994	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	71.960%
47) 2-Hexanone-d5	10.920	63	13280	46.439	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.880%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	30911	23.402	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	93.600%
66) 1,2-Dichlorobenzene-d4	13.847	152	48093	20.252	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.000%
Target Compounds						
13) Acetone	4.135	43	1131	3.453	ug/L	Qvalue 72


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120221\
Data File : VW021038.D
Acq On : 02 Dec 2021 11:34
Operator : SY/VA
Sample : M4868-09
Misc : 7.30g/10.0mL/MSVOA_W/SOIL
ALS Vial : 9 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGKP4

Quant Time: Dec 03 02:23:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM111521SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 03 01:25:28 2021
Response via : Initial Calibration

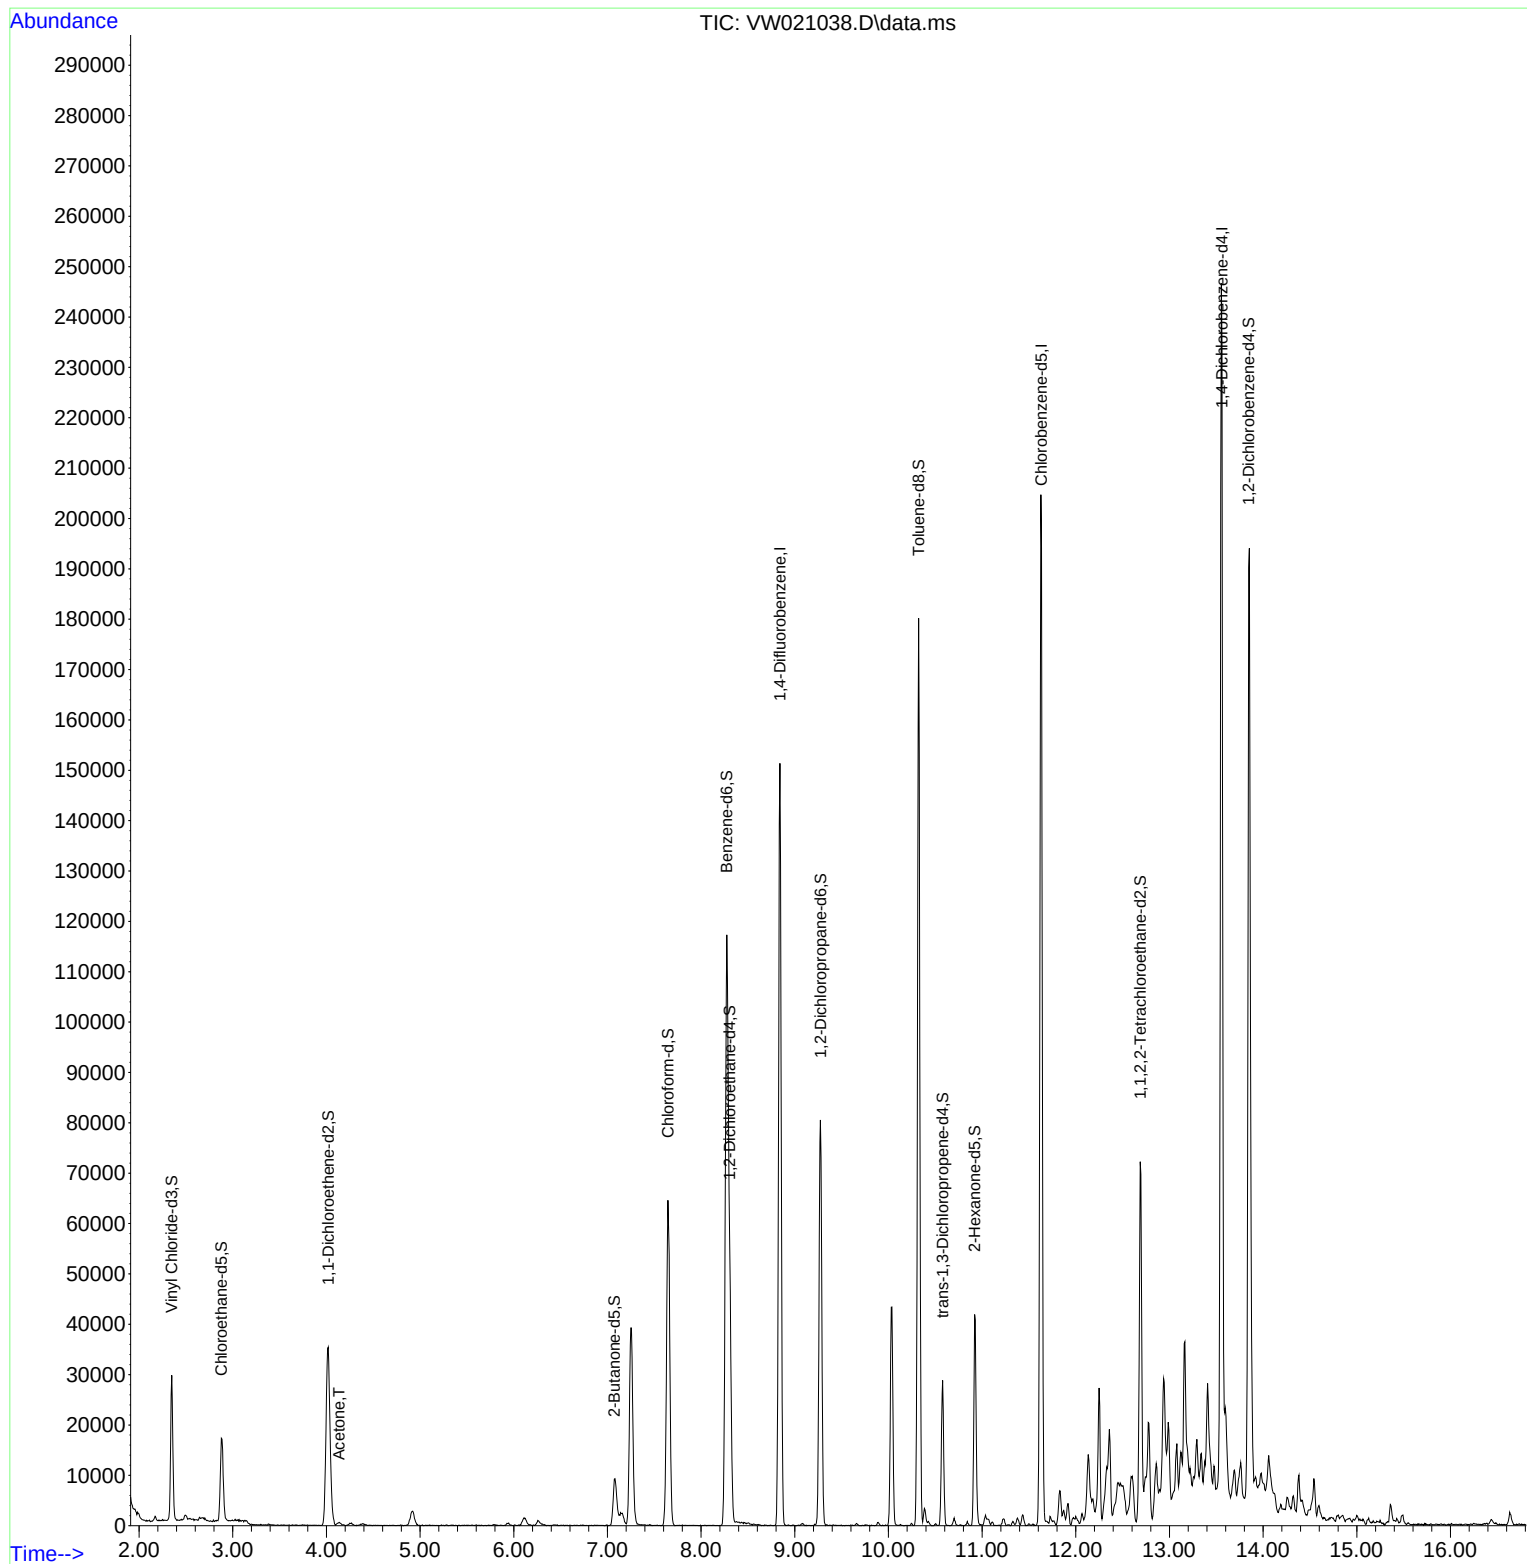

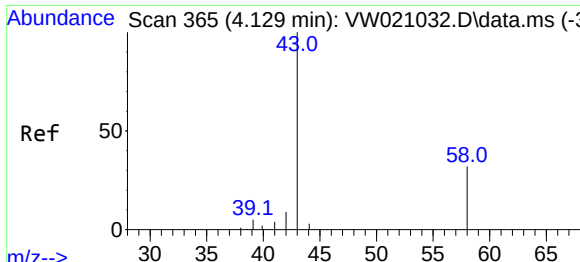

#13
 Acetone
 Concen: 3.453 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.006 min
 Lab File: VW021038.D
 Acq: 02 Dec 2021 11:34

Instrument :
 MSVOA_W
 ClientSampleId :
 BGKP4

Tgt Ion:	43	Resp:	1131
Ion	Ratio	Lower	Upper
43	100		
58	12.0	0.0	52.8

