


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW120318\
 Data File : VW007155.D
 Acq On : 03 Dec 2018 09:13
 Operator : SY/AP
 Sample : BFB82
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB82

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM113018S.M
 Title : VOC Analysis
 Last Update : Tue Dec 04 03:14:20 2018

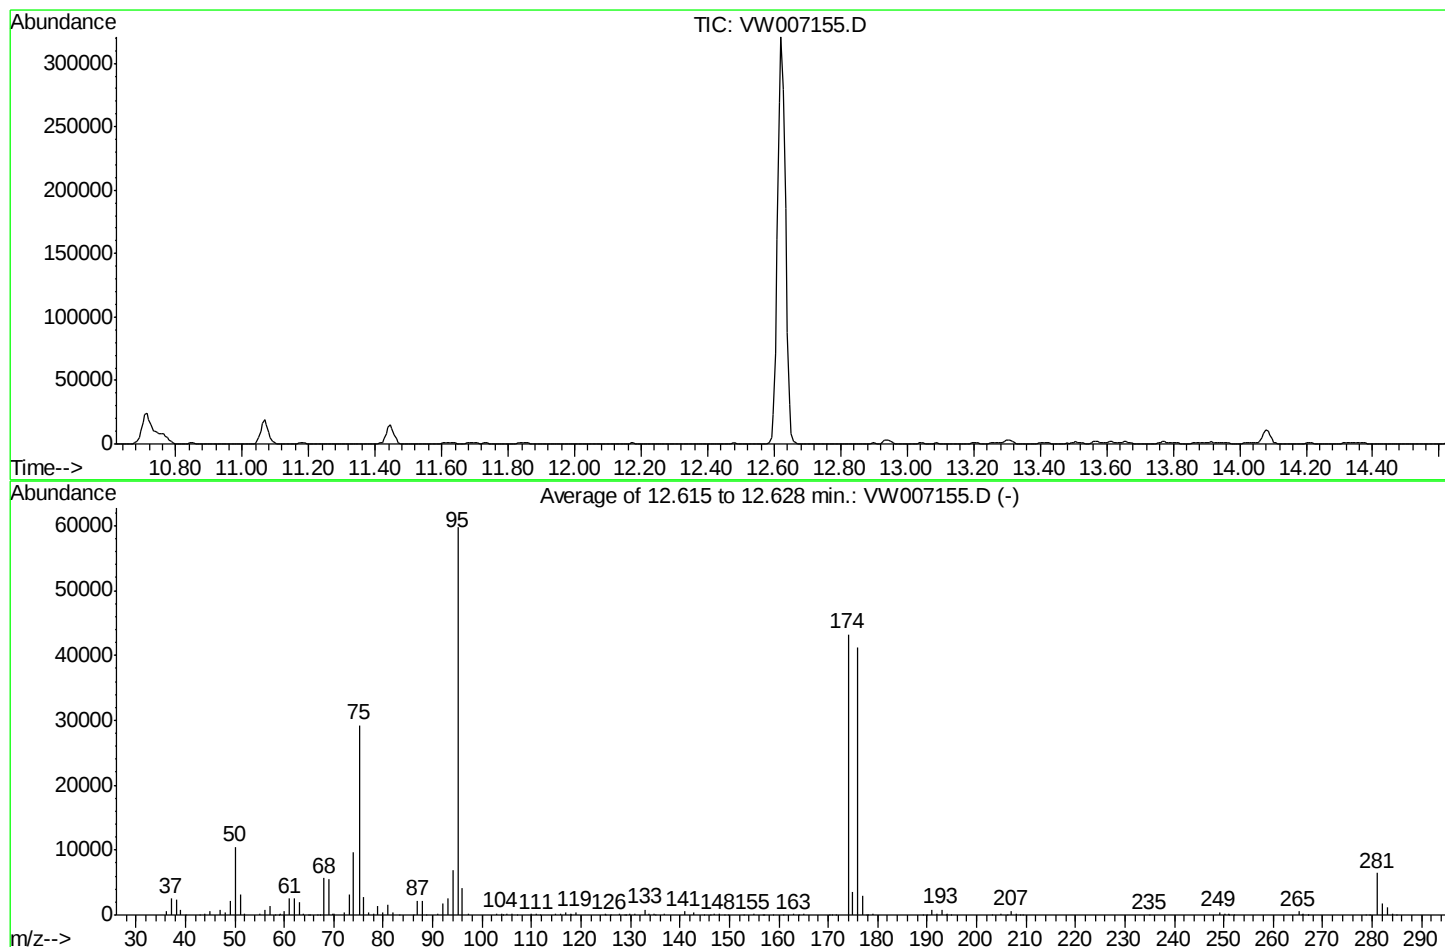

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	10522	PASS
75	95	30	80	49.0	29264	PASS
95	95	100	100	100.0	59736	PASS
96	95	5	9	6.8	4061	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	72.4	43245	PASS
175	174	5	9	8.0	3473	PASS
176	174	95	101	95.3	41194	PASS
177	176	5	9	7.1	2934	PASS

m/z	Abundance
36.00	419.0
37.10	2520.0
38.10	2426.0
39.10	715.0
40.00	128.0
44.00	368.0
45.00	644.0
47.00	686.0
48.10	443.0
49.10	2095.0
50.00	9983.0
51.10	2803.0
52.10	157.0
54.90	175.0
56.00	768.0
57.10	1313.0
58.10	96.0
59.10	191.0
60.00	473.0
61.00	2507.0
62.00	2522.0
63.00	2059.0
63.90	167.0
64.90	83.0
68.00	5243.0
69.10	5118.0
69.90	445.0
72.10	332.0
73.10	3025.0
74.10	9224.0
75.10	27256.0
76.00	2438.0
77.00	310.0
78.00	195.0
78.90	1297.0
80.10	341.0
81.00	1612.0
82.00	370.0
83.30	60.0
87.00	2039.0
88.00	2007.0
88.70	75.0
91.10	245.0
92.00	1556.0
93.00	2448.0
94.00	6763.0
95.10	54856.0
96.00	3821.0
97.20	121.0
103.00	278.0
103.90	228.0
104.10	231.0
105.00	108.0
105.90	193.0
110.00	146.0
110.90	106.0
111.90	107.0
115.00	128.0
115.90	181.0
117.00	369.0
117.90	266.0
119.00	461.0
125.10	352.0
125.80	59.0
128.00	193.0
128.90	88.0
130.00	247.0
130.90	131.0
133.00	1160.0
133.90	250.0
134.90	199.0
136.90	90.0
140.90	404.0
143.00	434.0
144.90	127.0
146.00	97.0
147.00	266.0
147.80	204.0
149.10	67.0
150.00	60.0
152.90	54.0
154.90	137.0
157.10	88.0
158.90	124.0
160.90	122.0
163.00	257.0
165.00	235.0
171.60	88.0
174.00	36200.0
175.00	3005.0
176.00	34776.0
177.00	2716.0

Instrument :
MSVOA_W
ClientSampleId :
BFB82

178.20	106.0
179.10	342.0
189.20	83.0
191.00	875.0
192.00	156.0
193.00	1138.0
193.90	242.0
194.90	113.0
203.00	154.0
205.00	268.0
207.10	866.0
208.10	194.0
208.80	64.0
209.30	59.0
235.00	89.0
249.10	560.0
250.10	144.0
250.90	180.0
251.00	180.0
252.00	92.0
265.10	640.0
266.10	235.0
267.00	158.0
278.80	90.0
279.40	105.0
281.10	7735.0
282.10	2437.0
283.10	1352.0
284.00	327.0
285.00	110.0

Instrument :
MSVOA_W
ClientSampleId :
BFB82

Scan 1750 (12.573 min): VW007155.D
BFB82

m/z	Abundance
40.00	69.0
44.00	102.0

Instrument :
MSVOA_W
ClientSampleId :
BFB82

m/z	Abundance
36.10	595.0
37.10	2342.0
38.10	2041.0
39.00	935.0
40.00	178.0
42.80	59.0
43.90	294.0
45.00	506.0
47.10	596.0
48.00	303.0
49.10	1956.0
50.10	9916.0
51.10	2883.0
52.00	141.0
55.00	115.0
56.00	731.0
57.10	1392.0
58.10	91.0
58.80	57.0
60.10	569.0
61.10	2284.0
62.00	2608.0
63.10	1689.0
64.00	168.0
67.10	130.0
68.00	5192.0
69.10	5472.0
70.00	476.0
72.10	312.0
73.00	2814.0
74.00	9052.0
75.10	27584.0
76.10	2703.0
77.10	322.0
78.00	301.0
79.00	1467.0
79.90	475.0
80.90	1409.0
82.00	324.0
86.10	142.0
87.00	1975.0
88.00	1848.0
90.90	194.0
92.00	1771.0
93.00	2446.0
94.10	6609.0
95.00	58728.0
96.00	4003.0
97.00	92.0
102.90	206.0
103.90	310.0
105.00	107.0
105.90	203.0
107.00	59.0
110.00	95.0
111.10	134.0
114.90	65.0
115.90	236.0
116.90	291.0
118.00	238.0
119.00	376.0
124.80	138.0
125.80	71.0
127.80	176.0
129.10	61.0
130.00	233.0
131.00	114.0
133.00	450.0
134.80	137.0
136.90	144.0
141.00	579.0
142.90	574.0
145.00	59.0
146.10	68.0
146.90	98.0
147.90	200.0
149.00	90.0
149.80	95.0
154.90	127.0
157.10	127.0
158.90	85.0
161.00	70.0
162.80	54.0
164.90	90.0
170.80	61.0
174.00	45656.0
175.00	3535.0
176.00	43448.0
177.00	2853.0
177.80	101.0
179.00	174.0
191.10	463.0

Instrument :
MSVOA_W
ClientSampleId :
BFB82

192.00	151.0
192.90	464.0
194.00	111.0
205.00	183.0
206.10	61.0
207.10	389.0
208.10	59.0
249.10	334.0
250.10	86.0
251.00	116.0
265.00	389.0
265.80	79.0
266.10	92.0
267.10	113.0
281.10	4354.0
282.10	1216.0
283.10	763.0
284.00	176.0
285.00	58.0

Instrument :
MSVOA_W
ClientSampleId :
BFB82

m/z	Abundance
36.10	507.0
37.10	2828.0
38.10	2470.0
39.10	952.0
40.00	111.0
44.10	350.0
45.00	657.0
47.10	942.0
48.00	447.0
49.10	2598.0
50.10	11667.0
51.00	3573.0
52.10	176.0
55.00	121.0
56.00	817.0
57.00	1730.0
58.10	99.0
59.00	130.0
60.10	536.0
61.10	2659.0
62.00	2833.0
63.10	2109.0
64.00	263.0
65.10	69.0
66.80	111.0
68.00	6458.0
69.00	6226.0
70.10	428.0
72.10	356.0
73.00	3681.0
74.10	11008.0
75.10	32952.0
76.10	2882.0
77.00	405.0
77.80	218.0
79.00	1662.0
80.00	432.0
80.90	1801.0
81.90	410.0
83.20	60.0
86.10	104.0
86.90	2758.0
87.90	2714.0
90.90	305.0
92.00	2033.0
93.00	2561.0
94.10	7300.0
95.00	65624.0
96.10	4359.0
97.10	202.0
102.80	120.0
103.90	325.0
105.00	125.0
105.90	340.0
107.10	69.0
110.00	97.0
111.00	131.0
111.80	76.0
114.90	128.0
115.90	232.0
117.00	577.0
118.10	230.0
118.90	409.0
125.00	215.0
125.90	50.0
127.90	171.0
128.80	109.0
129.90	311.0
130.90	121.0
133.00	810.0
133.70	293.0
135.10	166.0
136.90	132.0
140.90	657.0
142.80	461.0
145.00	81.0
146.10	73.0
147.00	124.0
147.90	141.0
149.00	133.0
149.90	60.0
152.80	78.0
155.00	164.0
156.80	103.0
158.90	94.0
161.00	116.0
163.00	127.0
163.90	59.0
164.90	95.0
170.30	51.0
170.80	58.0
174.00	47880.0

Instrument :
MSVOA_W
ClientSampleId :
BFB82

175.00	3880.0
176.00	45360.0
177.00	3235.0
178.00	145.0
179.10	196.0
189.90	68.0
191.10	821.0
192.00	278.0
193.00	1012.0
194.10	219.0
194.90	112.0
203.10	135.0
205.00	200.0
206.10	69.0
207.00	566.0
208.10	106.0
208.80	85.0
235.10	64.0
249.00	596.0
250.10	146.0
251.10	156.0
252.00	70.0
265.10	637.0
266.00	236.0
267.20	169.0
281.10	7215.0
282.10	1917.0
283.10	1253.0
284.10	292.0
285.00	50.0

Instrument :
MSVOA_W
ClientSampleId :
BFB82