

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120320\
 Data File : VW017535.D
 Acq On : 03 Dec 2020 15:59
 Operator : SY/VA
 Sample : L4920-11
 Misc : 5.13G/10ML/MSVOA W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 BG4F7

Manual Integrations
 APPROVED

MMDadoda
 12/21/2020 1:35:25 PM

Quant Time: Dec 20 00:34:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 00:31:51 2020
 Response via : Initial Calibration

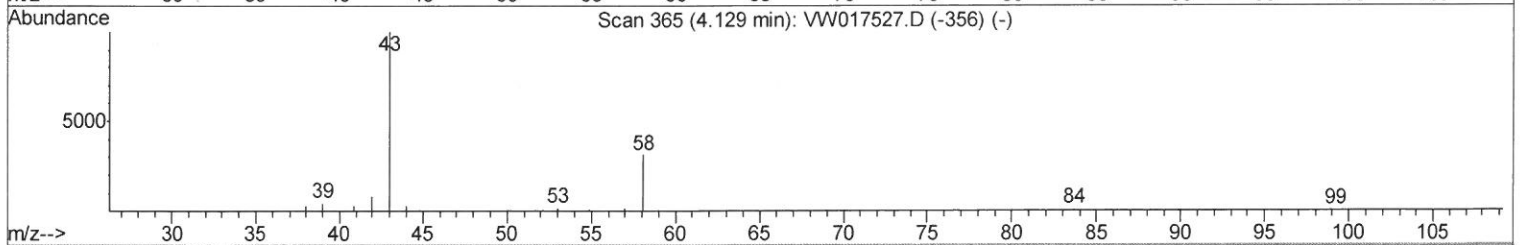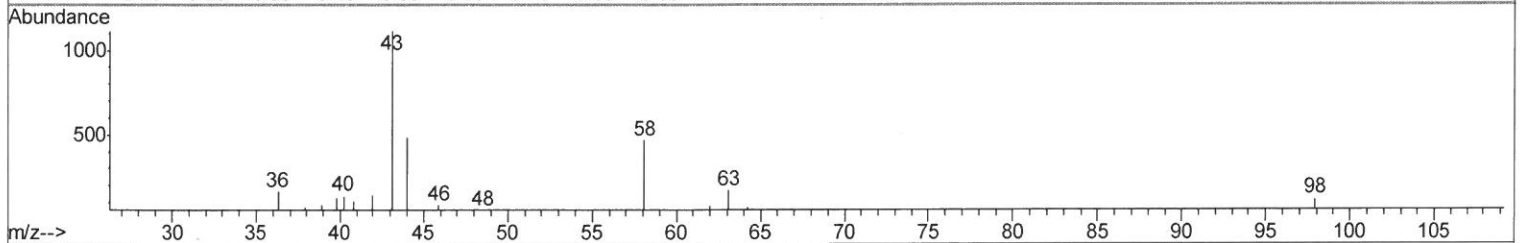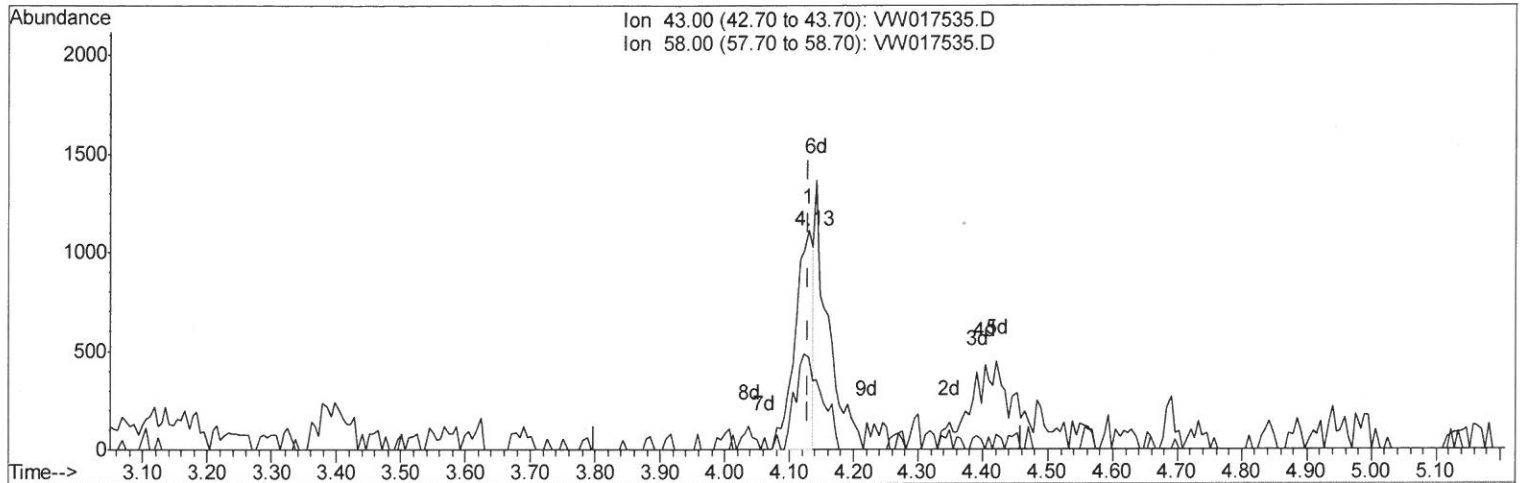

TIC: VW017535.D

(13) Acetone (T)

4.129min (+0.000) 1.61ug/L

response 2154

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	58.26
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120320\
 Data File : VW017535.D
 Acq On : 03 Dec 2020 15:59
 Operator : SY/VA
 Sample : L4920-11
 Misc : 5.13G/10ML/MSVOA W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 BG4F7

Manual Integrations
APPROVED

MMDadoda
 12/21/2020 1:35:25 PM

Quant Time: Dec 20 00:34:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 00:31:51 2020
 Response via : Initial Calibration

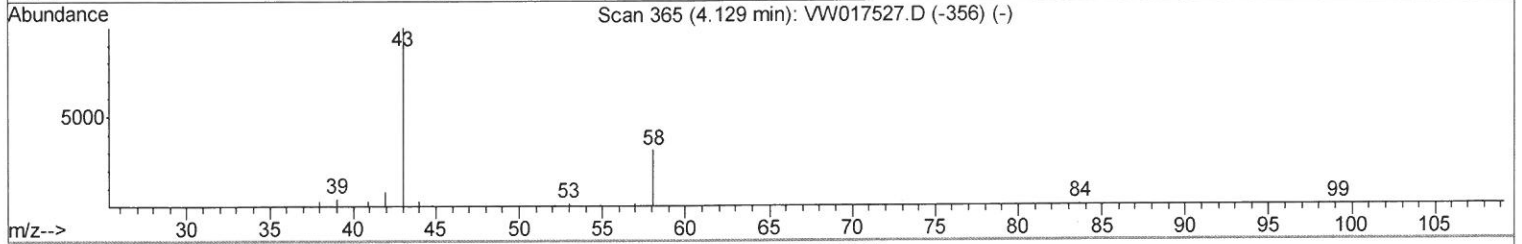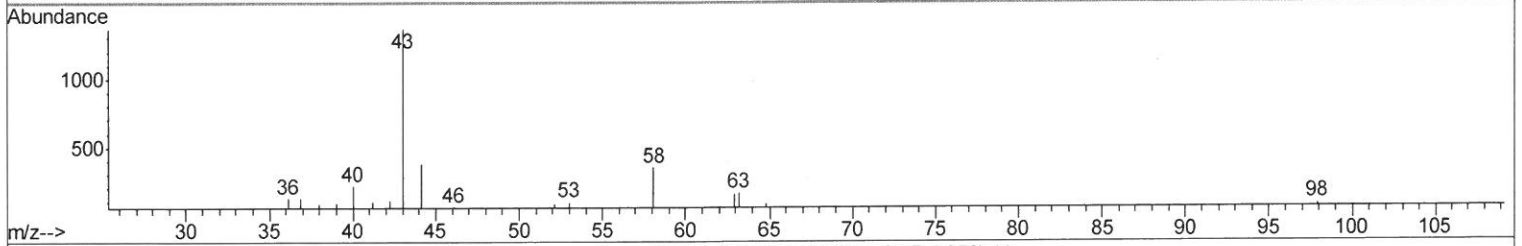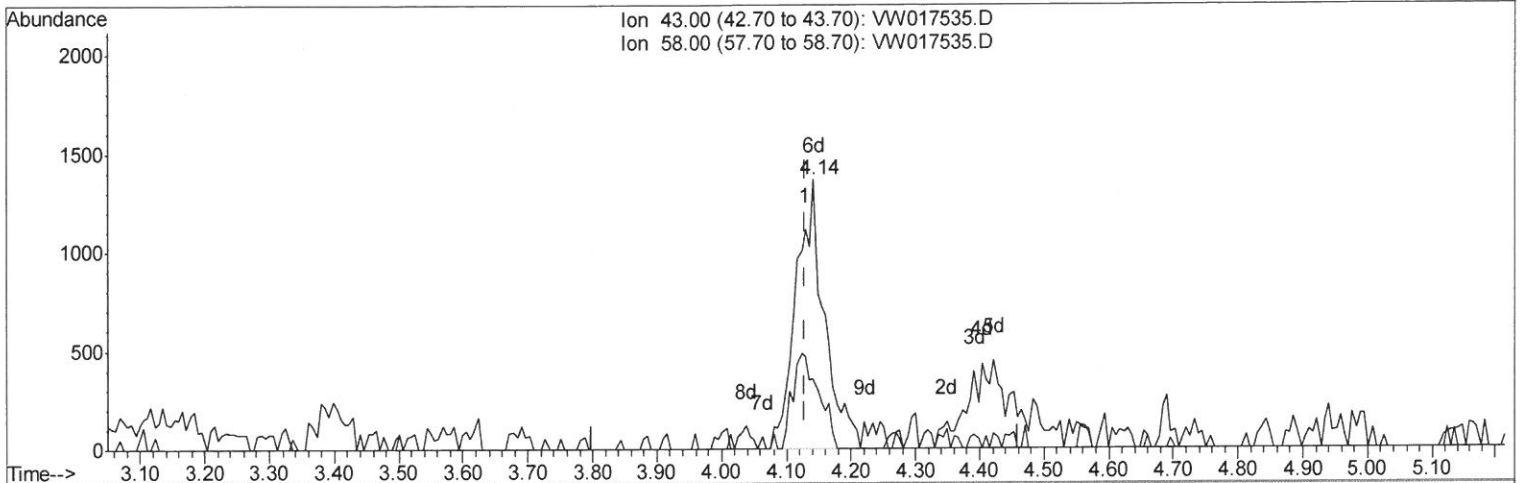

TIC: VW017535.D

(13) Acetone (T)

4.141min (+0.012) 3.08ug/L m

response 4133

Ion	Exp%	Act%
43.00	100	100
58.00	34.20	30.37
0.00	0.00	0.00
0.00	0.00	0.00

12/21/2020

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120320\
 Data File : VW017535.D
 Acq On : 03 Dec 2020 15:59
 Operator : SY/VA
 Sample : L4920-11
 Misc : 5.13G/10ML/MSVOA W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BG4F7

Manual Integrations
 APPROVED

MMDadoda
 12/21/2020 1:35:25 PM

Ouant Time: Dec 20 01:02:11 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 00:31:51 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	502622	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	458398	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	226254	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	101408	15.34	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	61.36%
7) Chloroethane-d5	2.89	69	89757	16.09	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	64.36%
10) 1,1-Dichloroethene-d2	4.02	63	182081	12.37	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	49.48%
20) 2-Butanone-d5	7.08	46	62608	44.90	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.80%
24) Chloroform-d	7.65	84	265940	18.62	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	74.48%
26) 1,2-Dichloroethane-d4	8.31	65	141297	20.17	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	80.68%
29) Benzene-d6	8.27	84	511778	18.16	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	72.64%
33) 1,2-Dichloropropane-d6	9.27	67	149742	19.20	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	76.80%
37) Toluene-d8	10.33	98	463384	18.05	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	72.20%
38) trans-1,3-Dichloropropene-	10.58	79	62930	18.06	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	72.24%
39) 2-Hexanone-d5	10.93	63	41014	42.48	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.96%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	115598	20.60	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	82.40%
61) 1,2-Dichlorobenzene-d4	13.85	152	170006	20.30	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	81.20%

Target Compounds

13) Acetone	4.14	43	4133m	3.080	ug/L	93
16) Methylene chloride	4.93	84	31270	4.144	ug/L	89
35) Trichloroethene	9.09	95	1656	0.217	ug/L	95
47) Tetrachloroethene	10.87	164	376373	57.834	ug/L	95

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120320\
Data File : VW017535.D
Acq On : 03 Dec 2020 15:59
Operator : SY/VA
Sample : L4920-11
Misc : 5.13G/10ML/MSVOA W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BG4F7

Manual Integrations
APPROVED

MMDadoda
12/21/2020 1:35:25 PM

Quant Time: Dec 20 01:02:11 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Sun Dec 20 00:31:51 2020
Response via : Initial Calibration

