

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120321\
 Data File : VW021090.D
 Acq On : 04 Dec 2021 02:28
 Operator : SY/VA
 Sample : M4883-20
 Misc : 5.30g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9H6

Quant Time: Dec 04 05:44:16 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120321SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 04 04:50:24 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.848	114	98124	25.000	ug/L	# 0.00
28) Chlorobenzene-d5		11.634	117	93377	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.554	152	42738	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.349	65	47936	35.063	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 140.240%		
7) Chloroethane-d5		2.885	69	30049	32.834	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 131.320%		
11) 1,1-Dichloroethene-d2		4.019	63	52812	24.181	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 96.720%		
21) 2-Butanone-d5		7.080	46	18878	60.538	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 121.080%		
24) Chloroform-d		7.653	84	76275	31.039	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 124.160%		
26) 1,2-Dichloroethane-d4		8.305	65	44416	33.038	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 132.160%#		
32) Benzene-d6		8.275	84	151850	31.805	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 127.200%		
36) 1,2-Dichloropropane-d6		9.274	67	42489	32.023	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 128.080%#		
41) Toluene-d8		10.323	98	145658	29.753	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 119.000%		
43) trans-1,3-Dichloroprop...		10.579	79	18592	30.860	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 123.440%		
47) 2-Hexanone-d5		10.927	63	15714	61.902	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 123.800%		
56) 1,1,2,2-Tetrachloroeth...		12.695	84	34586	28.176	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 112.720%		
66) 1,2-Dichlorobenzene-d4		13.853	152	43795	28.600	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 114.400%		
Target Compounds							Qvalue
13) Acetone		4.129	43	1996	7.027	ug/L	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120321\
Data File : VW021090.D
Acq On : 04 Dec 2021 02:28
Operator : SY/VA
Sample : M4883-20
Misc : 5.30g/10.0mL/MSVOA_W/SOIL
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW9H6

Quant Time: Dec 04 05:44:16 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120321SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 04 04:50:24 2021
Response via : Initial Calibration

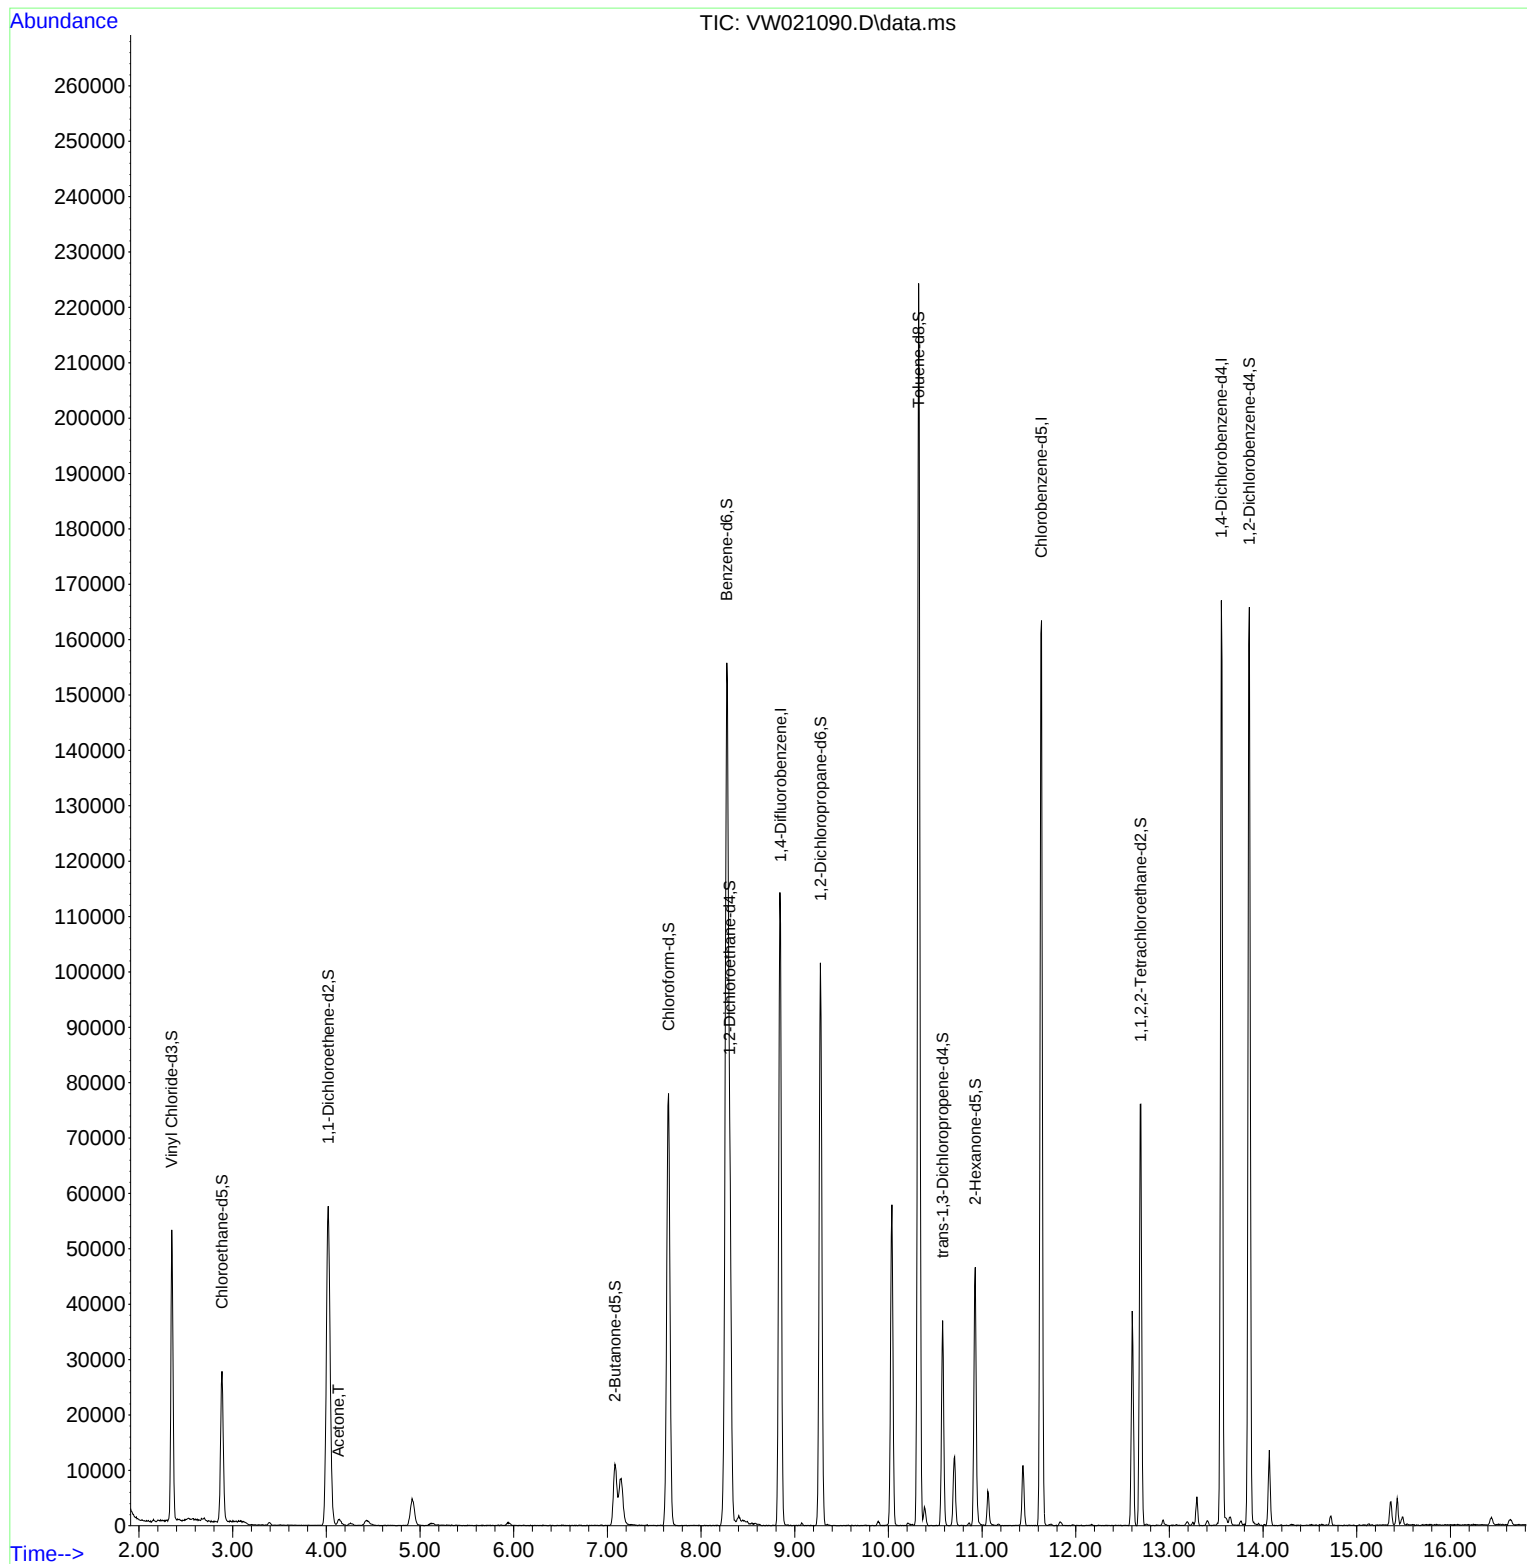

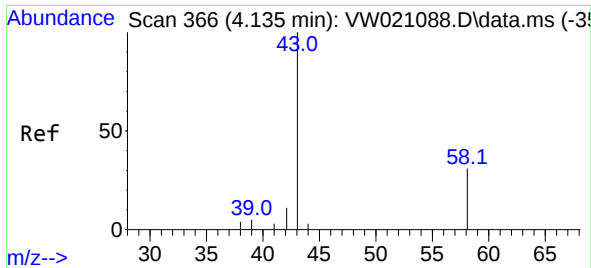

#13
 Acetone
 Concen: 7.027 ug/L
 RT: 4.129 min Scan# 30
 Delta R.T. -0.006 min
 Lab File: VW021090.D
 Acq: 04 Dec 2021 02:28

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9H6

Tgt Ion: 43 Resp: 1996
 Ion Ratio Lower Upper
 43 100
 58 15.2 0.0 52.8

