



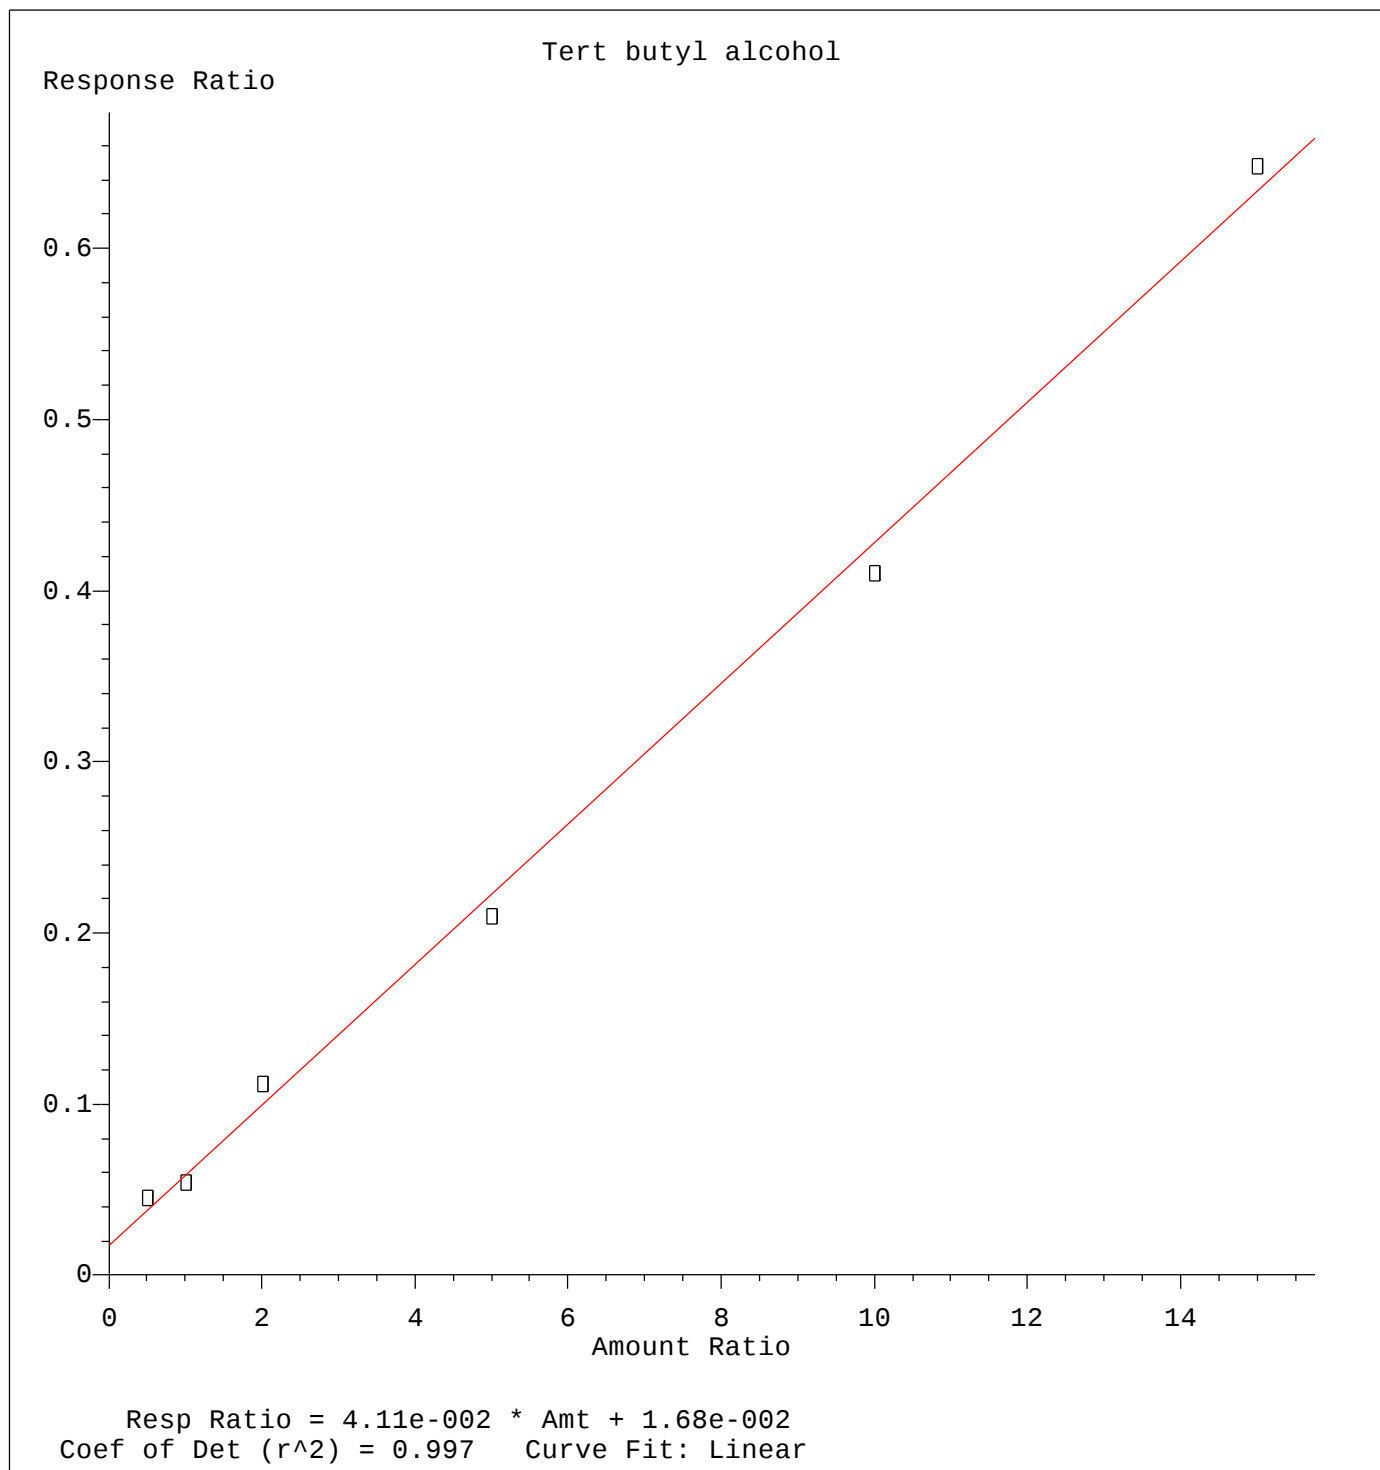

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W120418S.M
Calibration Table Last Updated: Wed Dec 05 01:35:23 2018

Methylene Chloride

Response Ratio

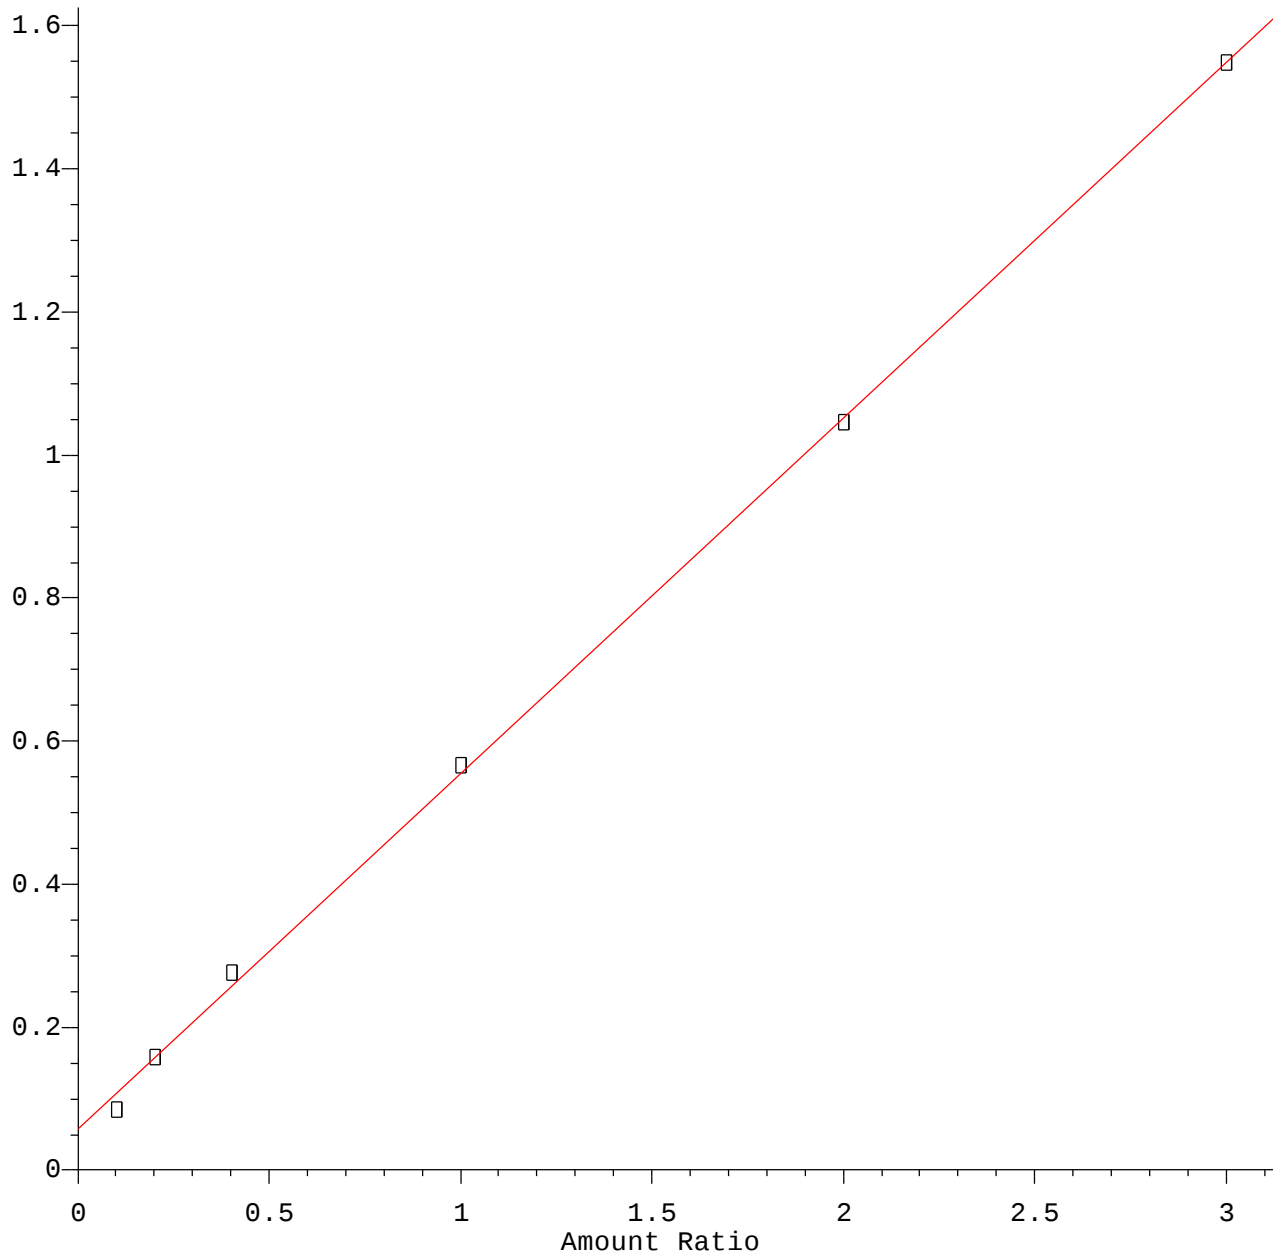

Resp Ratio = $4.97 \times 10^{-1} \times \text{Amt} + 5.79 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W120418S.M
Calibration Table Last Updated: Wed Dec 05 01:35:23 2018