

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120420\
 Data File : VW017556.D
 Acq On : 04 Dec 2020 15:17
 Operator : SY/VA
 Sample : L4941-07
 Misc : 5.09G/10ML/MSVOA W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 C0A22

Manual Integrations
 APPROVED

MMDadoda
 12/21/2020 1:36:16 PM

Quant Time: Dec 20 01:47:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 01:44:20 2020
 Response via : Initial Calibration

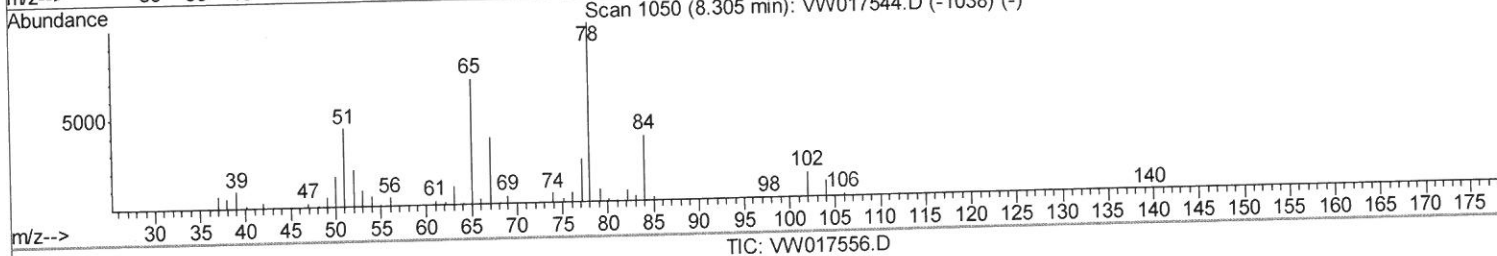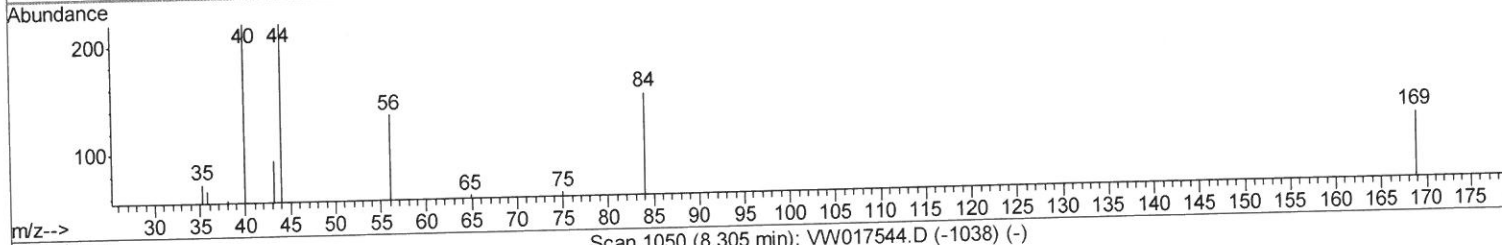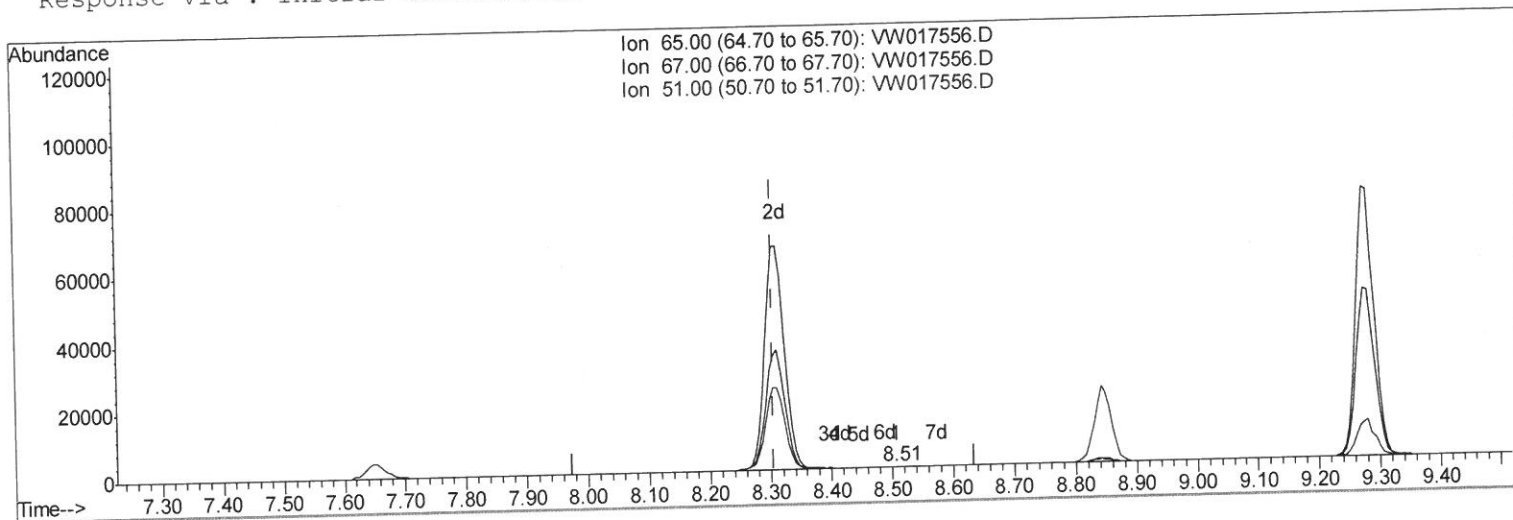

(26) 1,2-Dichloroethane-d4 (S)

8.506min (+0.201) 0.00ug/L

response 117

Ion	Exp%	Act%
65.00	100	100
67.00	53.90	61.54
51.00	108.50	104.27
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120420\
 Data File : VW017556.D
 Acq On : 04 Dec 2020 15:17
 Operator : SY/VA
 Sample : L4941-07
 Misc : 5.09G/10ML/MSVOA W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 C0A22

Manual Integrations
APPROVED

MMDadoda
 12/21/2020 1:36:16 PM

Quant Time: Dec 20 01:47:25 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 01:44:20 2020
 Response via : Initial Calibration

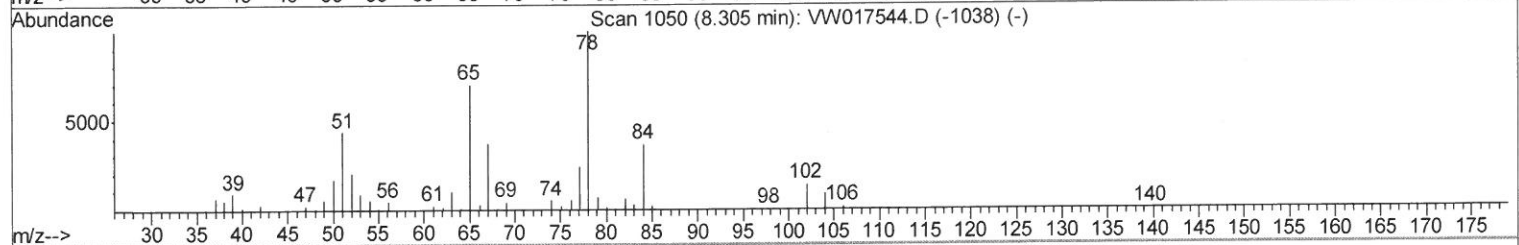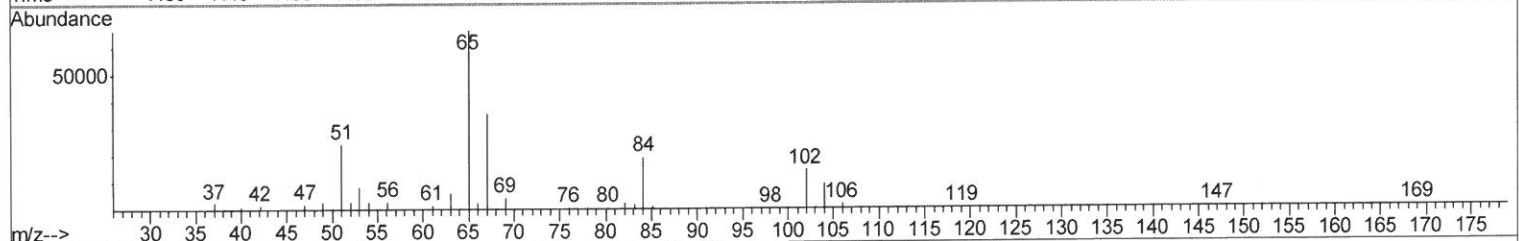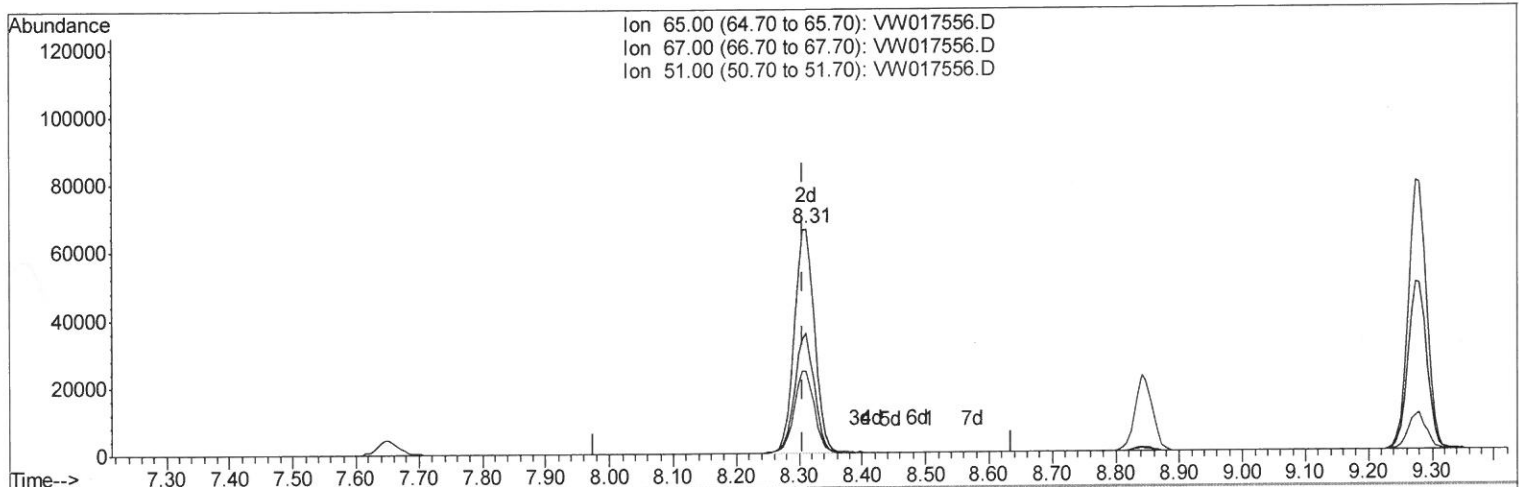

TIC: VW017556.D

(26) 1,2-Dichloroethane-d4 (S)

8.311min (+0.006) 4.73ug/L m

response 149676

Ion	Exp%	Act%
65.00	100	100
67.00	53.90	0.05#
51.00	108.50	0.08#
0.00	0.00	0.00

> 12/21/20 sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120420\
 Data File : VW017556.D
 Acq On : 04 Dec 2020 15:17
 Operator : SY/VA
 Sample : L4941-07
 Misc : 5.09G/10ML/MSVOA W/SOIL
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0AZ2

Manual Integrations
 APPROVED

MMDadoda
 12/21/2020 1:36:16 PM

Quant Time: Dec 20 02:40:28 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
 Quant Title : VOC Analysis
 QLast Update : Sun Dec 20 01:44:20 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	2268291	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1931998	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	858806	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	109326	3.66	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	14.64%#
7) Chloroethane-d5	2.89	69	97255	3.86	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	15.44%#
10) 1,1-Dichloroethene-d2	4.03	63	194212	2.92	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	11.68%#
20) 2-Butanone-d5	7.08	46	58249	9.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	18.52%#
24) Chloroform-d	7.65	84	284395	4.41	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	17.64%#
26) 1,2-Dichloroethane-d4	8.31	65	149676m	4.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	18.92%#
29) Benzene-d6	8.28	84	540501	4.55	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	18.20%#
33) 1,2-Dichloropropane-d6	9.27	67	159432	4.85	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	19.40%#
37) Toluene-d8	10.33	98	488149	4.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	18.04%#
38) trans-1,3-Dichloropropene-	10.58	79	65406	4.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	17.80%#
39) 2-Hexanone-d5	10.93	63	37681	9.26	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	18.52%#
48) 1,1,2,2-Tetrachloroethane-	12.69	84	112886	4.77	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	19.08%#
61) 1,2-Dichlorobenzene-d4	13.85	152	147105	4.63	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	18.52%#

Target Compounds				Ovalue
16) Methylene chloride	4.92	84	44846	1.317 ug/L 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120420\
Data File : VW017556.D
Acq On : 04 Dec 2020 15:17
Operator : SY/VA
Sample : L4941-07
Misc : 5.09G/10ML/MSVOA W/SOIL
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0AZ2

Manual Integrations
APPROVED

MMDadoda
12/21/2020 1:36:16 PM

Quant Time: Dec 20 02:40:28 2020
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM112420S.M
Quant Title : VOC Analysis
QLast Update : Sun Dec 20 01:44:20 2020
Response via : Initial Calibration

