


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW120518\
 Data File : VW007254.D
 Acq On : 06 Dec 2018 02:24
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W120418S.M
 Title : SW846 8260
 Last Update : Wed Dec 05 01:35:23 2018

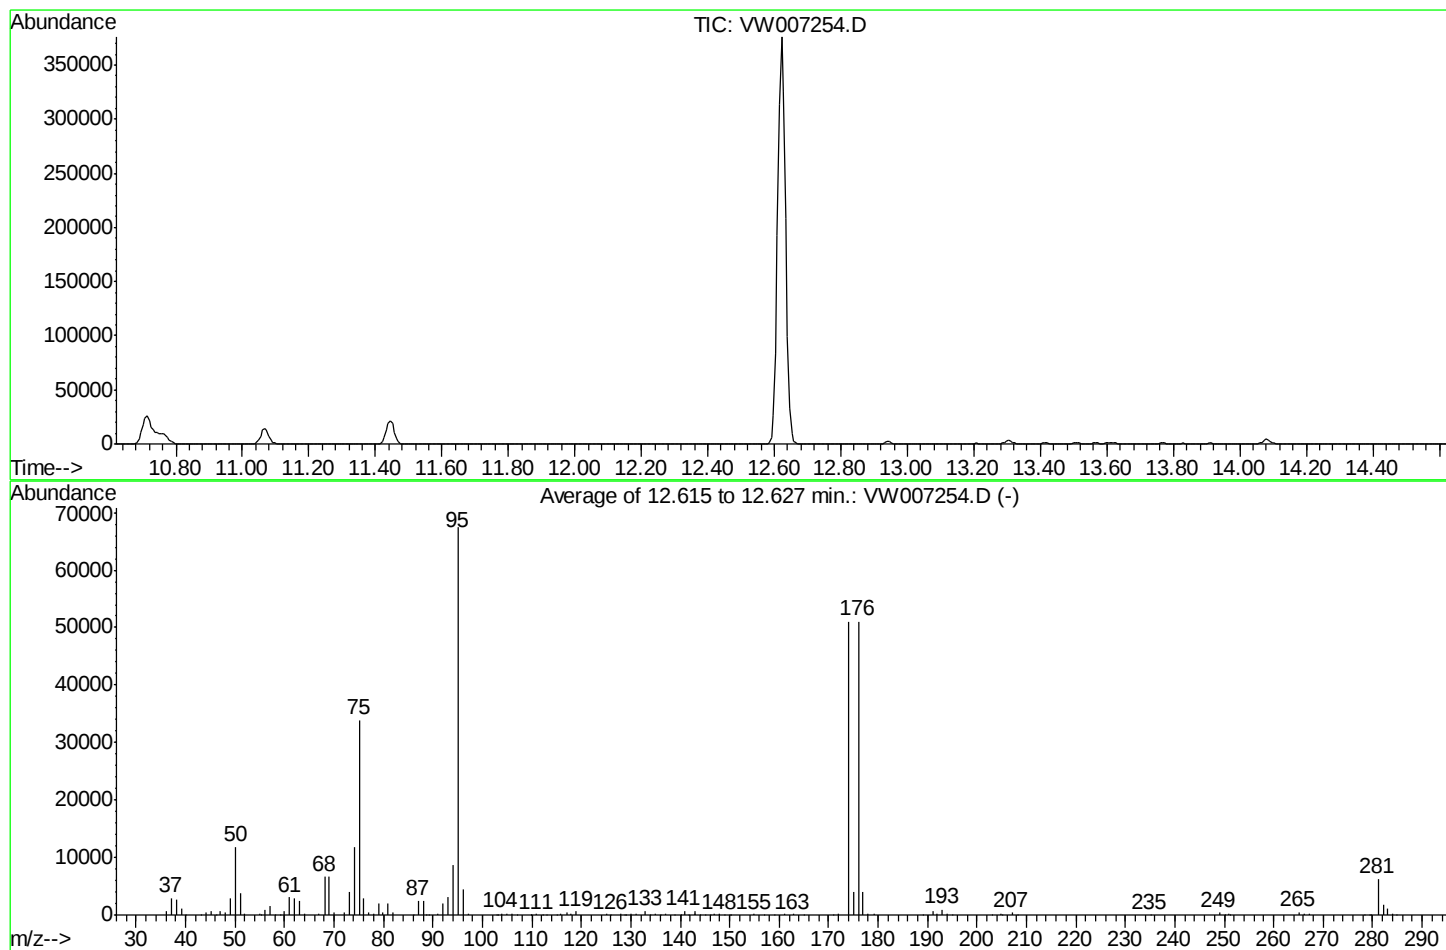

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.7	11907	PASS
75	95	30	60	50.2	33864	PASS
95	95	100	100	100.0	67437	PASS
96	95	5	9	6.7	4522	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.5	50893	PASS
175	174	5	9	8.1	4111	PASS
176	174	95	101	100.3	51061	PASS
177	176	5	9	7.7	3930	PASS