

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120618\
 Data File : VW007290.D
 Acq On : 06 Dec 2018 20:25
 Operator : SY/AP
 Sample : J6214-01RE
 Misc : 3.47G/5ML/MSVOA W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 07 01:17:15 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W120418S.M
 Quant Title : SW846 8260
 QLast Update : Wed Dec 05 01:35:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.95	168	28746	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.85	114	46310	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.63	117	36811	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.56	152	13109	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.31	65	14265	53.30	ug/l	0.00
Spiked Amount			Recovery	=	106.60%	
35) Dibromofluoromethane	7.89	113	12516	47.20	ug/l	0.00
Spiked Amount			Recovery	=	94.40%	
50) Toluene-d8	10.32	98	39447	33.77	ug/l	0.00
Spiked Amount			Recovery	=	67.54%	
62) 4-Bromofluorobenzene	12.62	95	12758	28.94	ug/l	0.00
Spiked Amount			Recovery	=	57.88%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	4.14	43	492	7.765	ug/l #	45
20) Methylene Chloride	4.93	84	1170	Below Cal	#	81
31) Cyclohexane	7.95	56	556	1.047	ug/l #	1
36) 1,1-Dichloropropene	7.96	75	2171	4.818	ug/l #	47
38) Carbon Tetrachloride	7.95	117	3025	6.577	ug/l #	18
51) 4-Methyl-2-Pentanone	10.23	43	238	1.526	ug/l #	35
59) 2-Hexanone	10.93	43	703	6.216	ug/l #	23
68) m/p-Xylenes	11.84	106	939	1.597	ug/l #	69
69) o-Xylene	12.18	106	565	1.029	ug/l	81
73) Isopropylbenzene	12.47	105	1537	1.442	ug/l	95
74) N-amyl acetate	12.26	43	5267	27.863	ug/l #	62
75) 1,1,2,2-Tetrachloroethane	12.69	83	320	2.311	ug/l #	1
76) 1,2,3-Trichloropropane	12.62	75	6288	61.948	ug/l #	100
77) Bromobenzene	12.88	156	680	2.955	ug/l #	20
78) n-propylbenzene	12.81	91	4318	3.399	ug/l	95
80) 1,3,5-Trimethylbenzene	12.94	105	3344	3.666	ug/l	95
81) trans-1,4-Dichloro-2-buten	12.62	75	6288	133.520	ug/l #	17
83) tert-Butylbenzene	13.21	119	806	1.011	ug/l	93
84) 1,2,4-Trimethylbenzene	13.26	105	28510	30.621	ug/l	98
85) sec-Butylbenzene	13.39	105	5340	4.693	ug/l #	71
86) p-Isopropyltoluene	13.51	119	4446	4.389	ug/l	93
89) n-Butylbenzene	13.83	91	8458	8.935	ug/l #	74
90) Hexachloroethane	14.10	117	2712	17.569	ug/l #	14
92) 1,2-Dibromo-3-Chloropropan	14.47	75	191	7.120	ug/l #	1
95) Naphthalene	15.37	128	7924	15.599	ug/l	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW120618\
Data File : VW007290.D
Acq On : 06 Dec 2018 20:25
Operator : SY/AP
Sample : J6214-01RE
Misc : 3.47G/5ML/MSVOA W/SOIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 07 01:17:15 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W120418S.M
Quant Title : SW846 8260
QLast Update : Wed Dec 05 01:35:23 2018
Response via : Initial Calibration

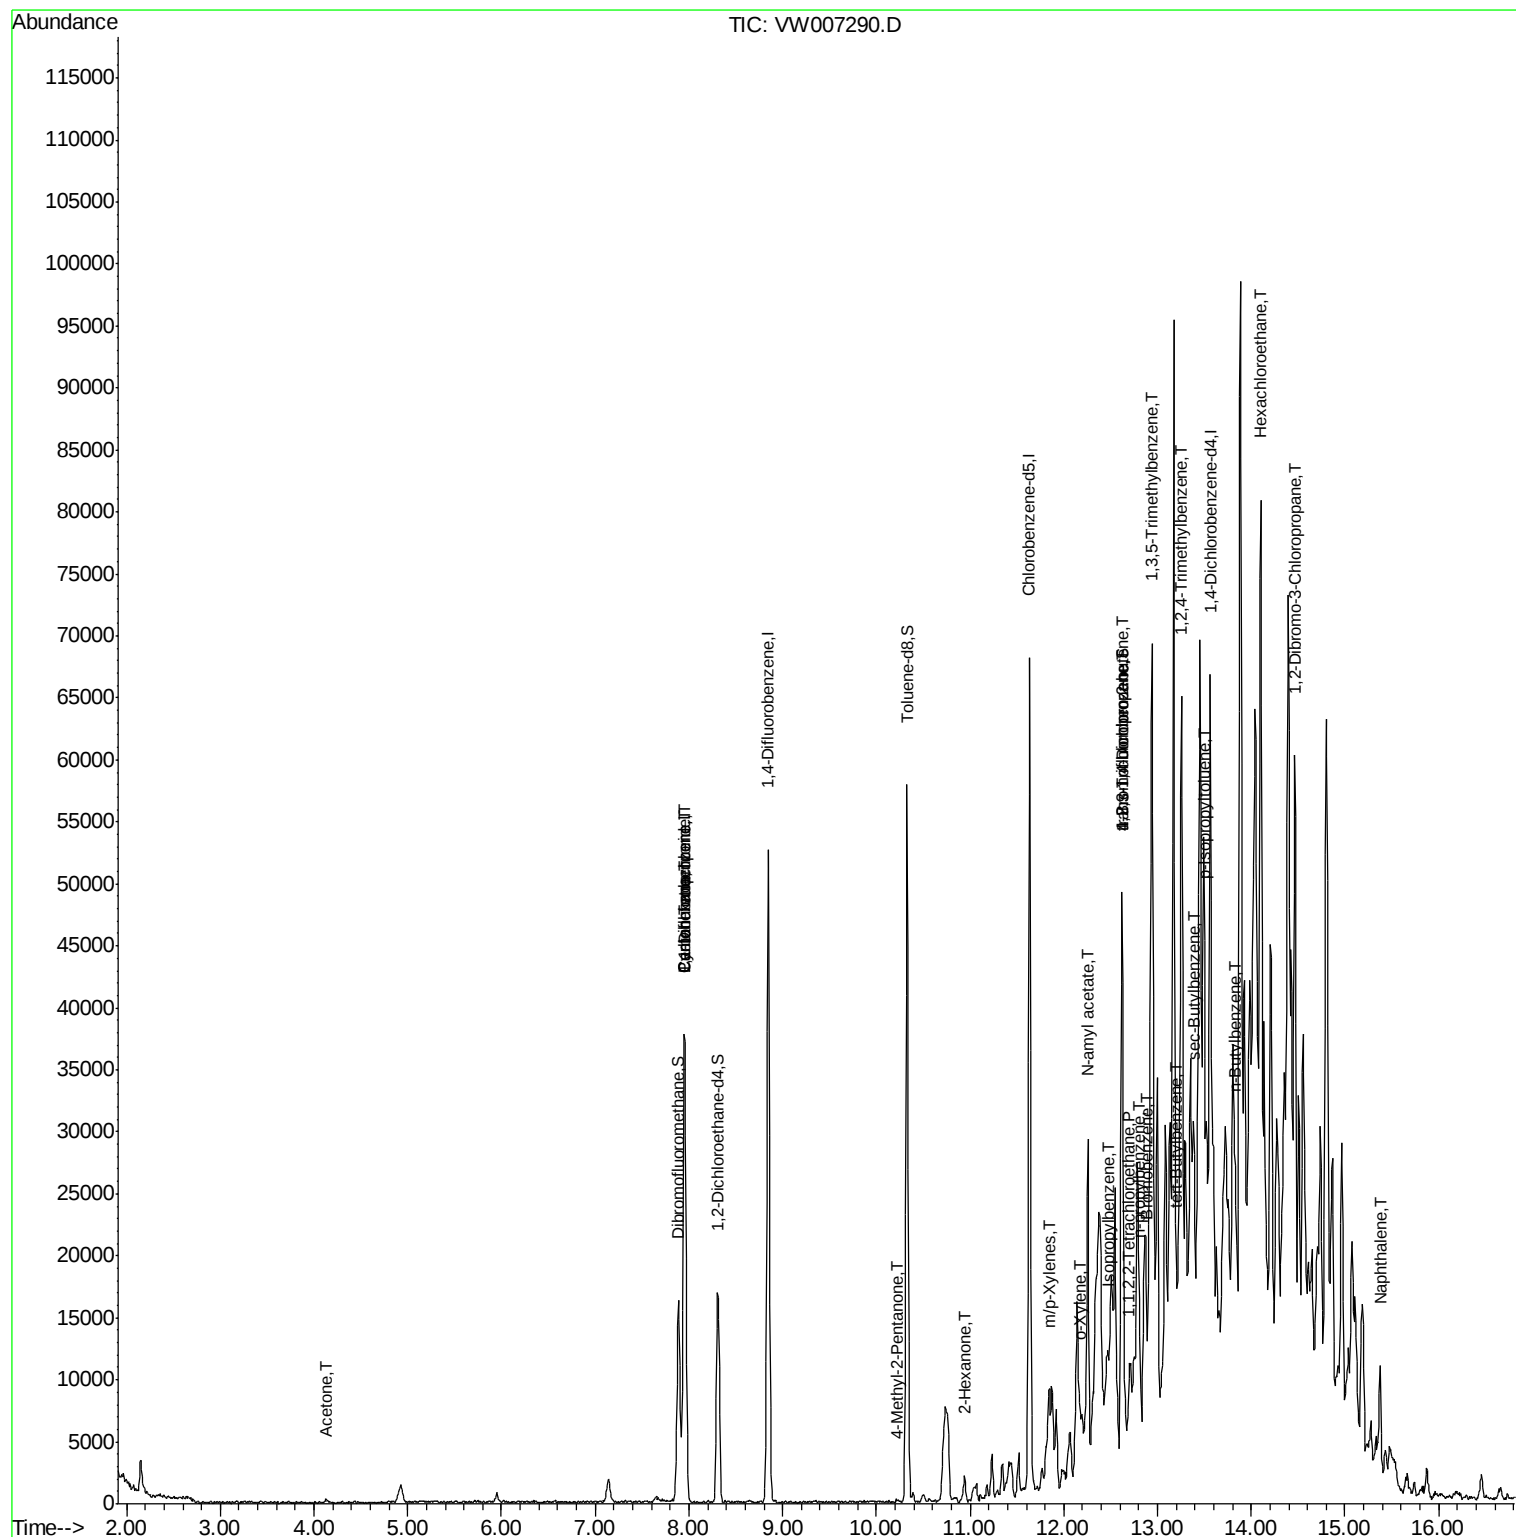



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.00 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W


ClientSampleId :

Tot Ion:168 Resp: 28746

Ion Ratio Lower Upper

168 100

99 62.8 47.8 71.8

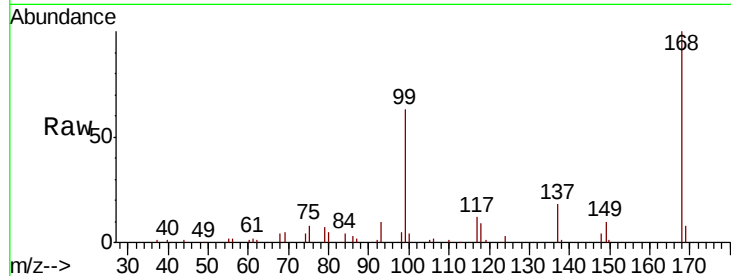

Abundance Ion 167.90 (167.60 to 168.60): VW

Ion 98.90 (98.60 to 99.60): VW

7.95

15000



10000

5000

0

Time-->

7.85 7.90 7.95 8.00 8.05



#16

Acetone

Concen: 7.765 ug/l

RT: 4.14 min Scan# 366

Delta R.T. 0.01 min

Lab File: VW007290.D


Acq: 06 Dec 2018 20:25

Tgt Ion: 43 Resp: 492

Ion Ratio Lower Upper

43 100

58 0.0 23.8 35.8#



Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

4.14

250

200

150


100


50

0

Time-->

4.10 4.15 4.20




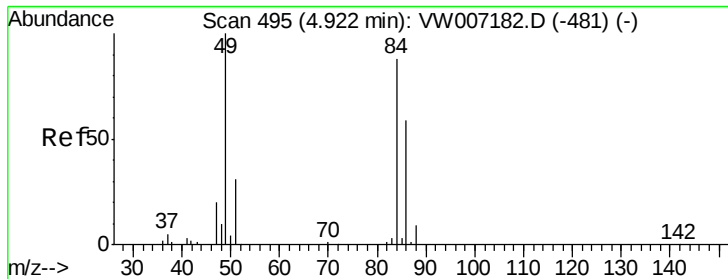




#20
Methvlene Chloride
Concen: Below Cal
RT: 4.93 min Scan# 496
Delta R.T. 0.01 min
Lab File: VW007290.D
Acq: 06 Dec 2018 20:25

Instrument :
MSVOA_W
ClientSampleId :

Tot Ion: 84 Resp: 1170
Ion Ratio Lower Upper
84 100
49 84.8 90.6 135.8#
51 49.3 27.6 41.4#
86 64.8 53.7 80.5

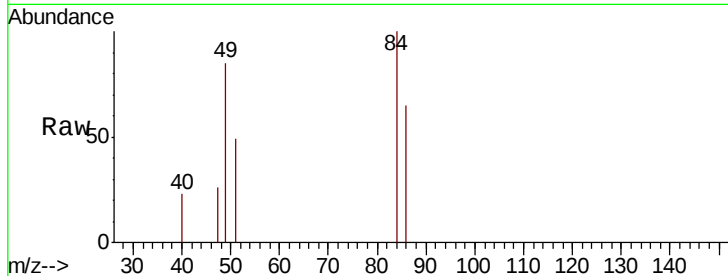


Abundance Ion 83.90 (83.60 to 84.60): VW
Ion 48.90 (48.60 to 49.60): VW
Ion 50.90 (50.60 to 51.60): VW
Ion 85.90 (85.60 to 86.60): VW

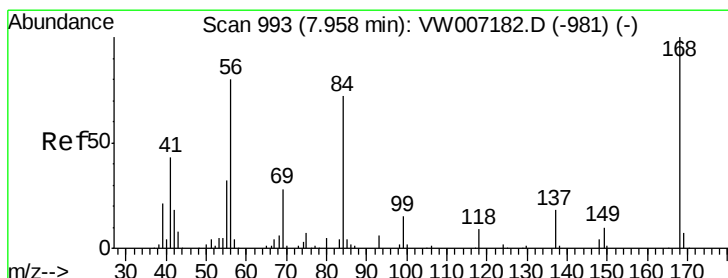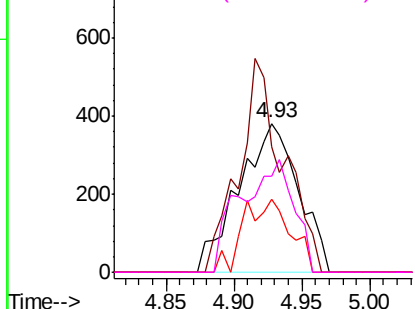
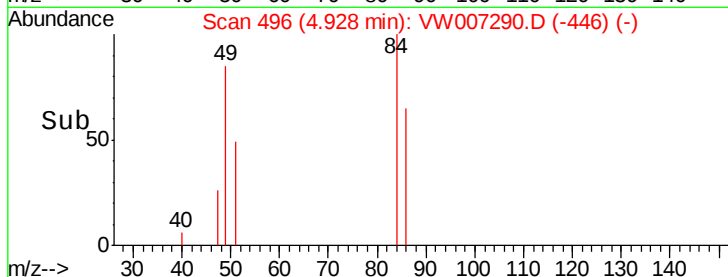



#31
Cyclohexane
Concen: 1.047 ug/l
RT: 7.95 min Scan# 992
Delta R.T. -0.01 min
Lab File: VW007290.D
Acq: 06 Dec 2018 20:25

Tgt Ion: 56 Resp: 556
Ion Ratio Lower Upper
56 100
69 229.6 28.2 42.2#
84 172.8 72.1 108.1#

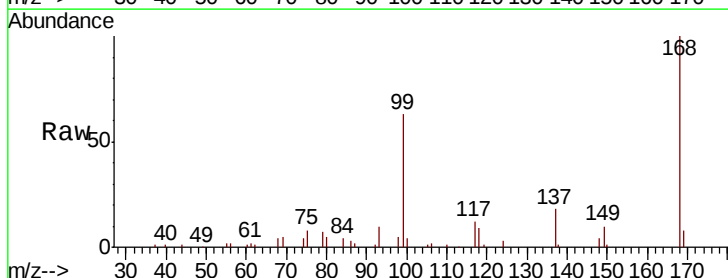

Abundance Ion 56.00 (55.70 to 56.70): VW
Ion 69.00 (68.70 to 69.70): VW
Ion 84.00 (83.70 to 84.70): VW



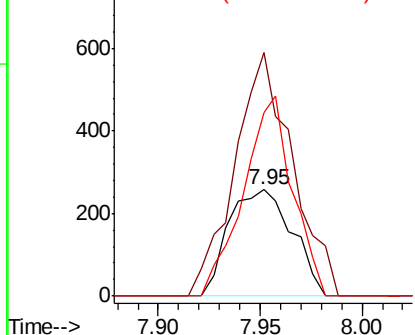
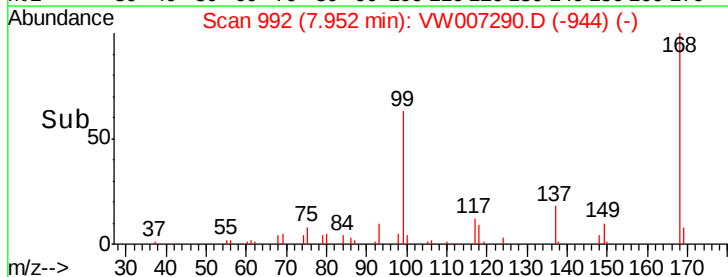




#33
 1,2-Dichloroethane-d4
 Concen: 53.300 ug/l
 RT: 8.31 min Scan# 1051
 Delta R.T. 0.00 min
 Lab File: VW007290.D
 Acq: 06 Dec 2018 20:25




Instrument :
 MSVOA_W
 ClientSampleId :


Tot Ion: 65 Resp: 14265
 Ion Ratio Lower Upper
 65 100
 67 49.6 0.0 106.4

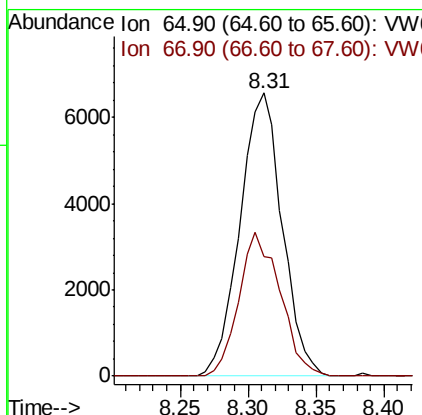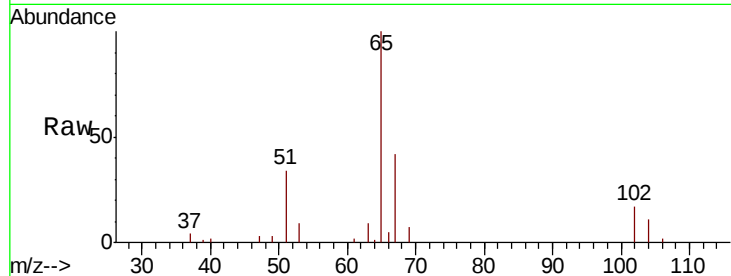

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.85 min Scan# 1139
 Delta R.T. -0.00 min
 Lab File: VW007290.D
 Acq: 06 Dec 2018 20:25

Tgt Ion: 114 Resp: 46310
 Ion Ratio Lower Upper
 114 100
 63 19.0 0.0 40.2
 88 16.0 0.0 30.0

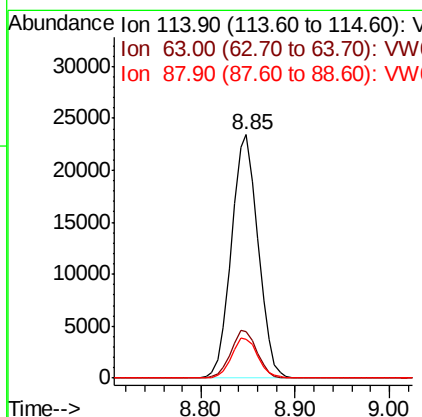



#35

Dibromofluoromethane

Concen: 47.200 ug/l

RT: 7.89 min Scan# 982

Delta R.T. -0.00 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :
MSVOA_W
ClientSampleId :


Tot Ion:113 Resp: 12516

Ion Ratio Lower Upper




113 100

111 100.9 82.2 123.4

192 18.1 14.4 21.6

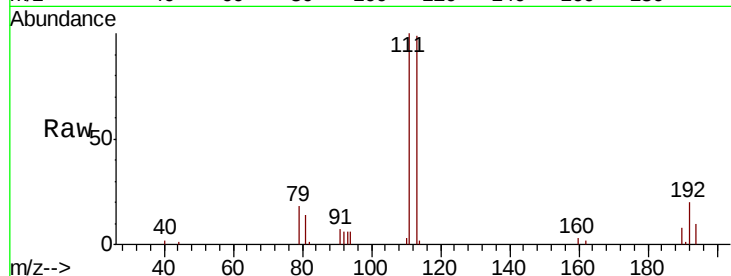

Abundance Ion 112.80 (112.50 to 113.50): V
Ion 110.80 (110.50 to 111.50): V
Ion 191.70 (191.40 to 192.40): V

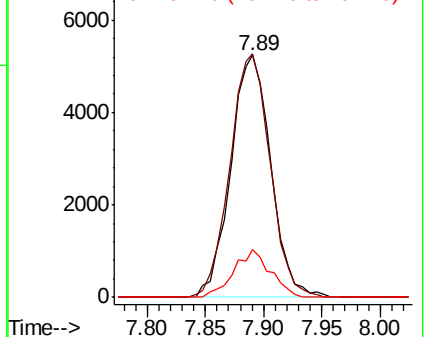

#36

1,1-Dichloropropene

Concen: 4.818 ug/l

RT: 7.96 min Scan# 993

Delta R.T. -0.13 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25


Tgt Ion: 75 Resp: 2171

Ion Ratio Lower Upper



75 100


110 7.1 18.3 54.9#

77 0.0 24.9 37.3#



Abundance Ion 74.90 (74.60 to 75.60): VW
Ion 109.90 (109.60 to 110.60): V
Ion 76.90 (76.60 to 77.60): VW

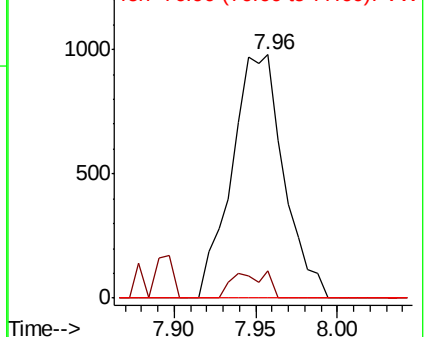



#38

Carbon Tetrachloride

Concen: 6.577 ug/l

RT: 7.95 min Scan# 992

Delta R.T. -0.12 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W

ClientSampleId :


Tot Ion:117 Resp: 3025

Ion Ratio Lower Upper

117 100

119 5.9 74.1 111.1#




121 0.0 23.9 35.9#

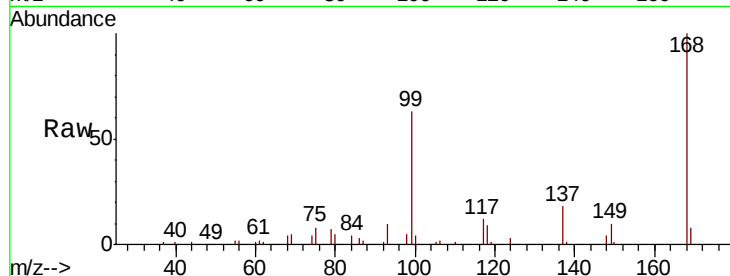

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

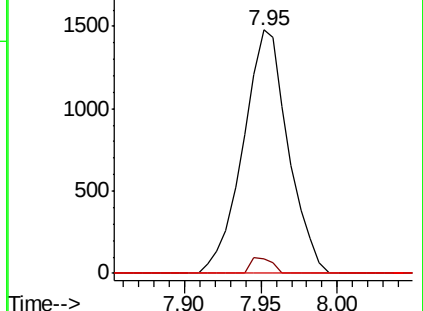

#50

Toluene-d8

Concen: 33.771 ug/l

RT: 10.32 min Scan# 1381

Delta R.T. -0.01 min

Lab File: VW007290.D


Acq: 06 Dec 2018 20:25

Tgt Ion: 98 Resp: 39447

Ion Ratio Lower Upper



98 100


100 65.2 52.7 79.1



Abundance Ion 98.00 (97.70 to 98.70): VW

Ion 100.00 (99.70 to 100.70): VW

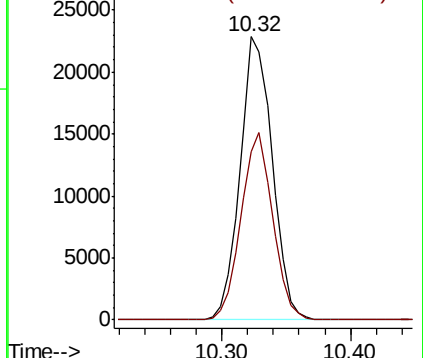

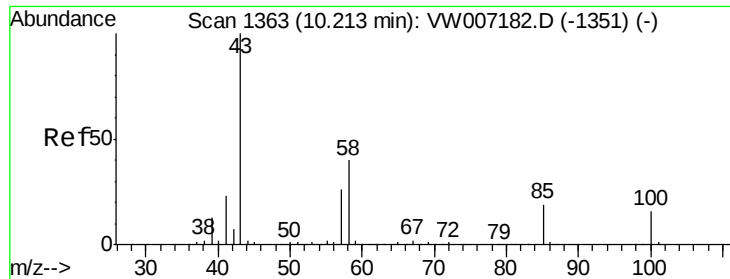

#51

4-Methyl-2-Pentanone

Concen: 1.526 ug/l

RT: 10.23 min Scan# 1365

Delta R.T. 0.01 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W


ClientSampled :

Tot Ion: 43 Resp: 238

Ion Ratio Lower Upper

43 100

58 0.0 32.3 48.5#

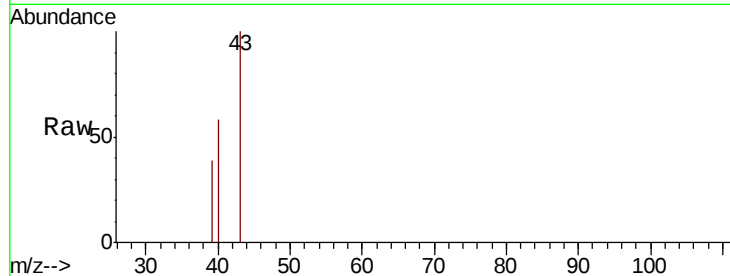

Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

10.23



150

100

50

0

Time-->



#59

2-Hexanone

Concen: 6.216 ug/l

RT: 10.93 min Scan# 1481

Delta R.T. -0.04 min

Lab File: VW007290.D


Acq: 06 Dec 2018 20:25

Tgt Ion: 43 Resp: 703

Ion Ratio Lower Upper

43 100

58 0.0 28.1 84.4#



Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 58.00 (57.70 to 58.70): VW

10.93

400


300


200

100

0

Time-->







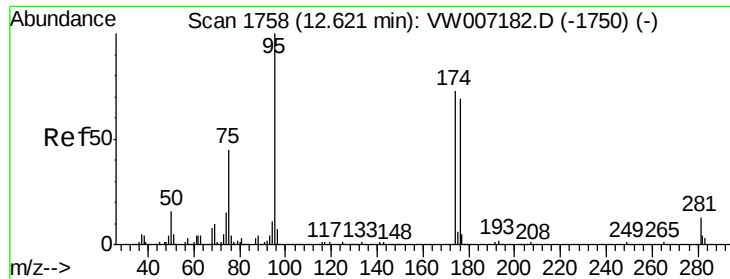

#62
4-Bromofluorobenzene
Concen: 28.938 ug/l
RT: 12.62 min Scan# 1758
Delta R.T. 0.00 min
Lab File: VW007290.D
Acq: 06 Dec 2018 20:25




Instrument :
MSVOA_W
ClientSampled :


Tot Ion: 95 Resp: 12758
Ion Ratio Lower Upper
95 100
174 73.4 0.0 148.0
176 70.9 0.0 139.4

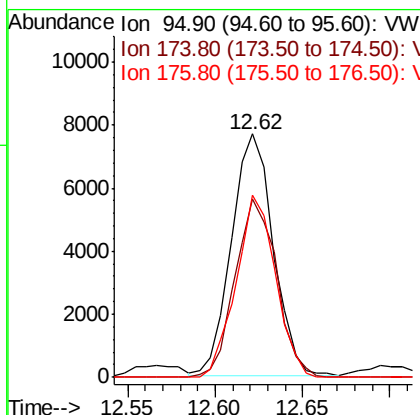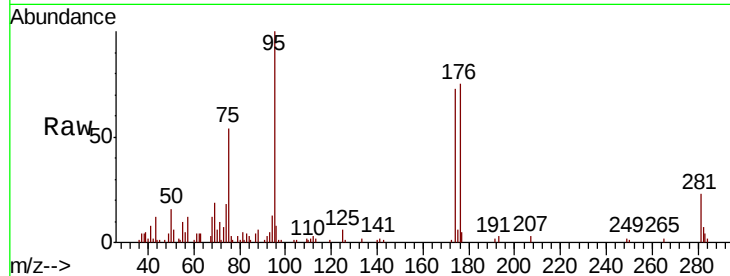

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.63 min Scan# 1596
Delta R.T. -0.00 min
Lab File: VW007290.D
Acq: 06 Dec 2018 20:25

Tgt Ion: 117 Resp: 36811
Ion Ratio Lower Upper
117 100
82 52.3 47.4 71.2
119 29.6 26.8 40.2

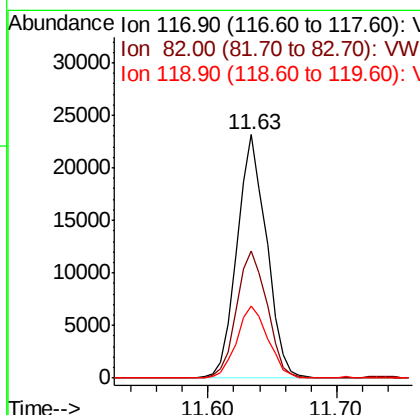



#68

m/p-Xylenes

Concen: 1.597 ug/l

RT: 11.84 min Scan# 1629

Delta R.T. -0.01 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W


ClientSampleId :

Tot Ion:106 Resp: 939

Ion Ratio Lower Upper




106 100

91 247.9 160.2 240.4#



Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VW

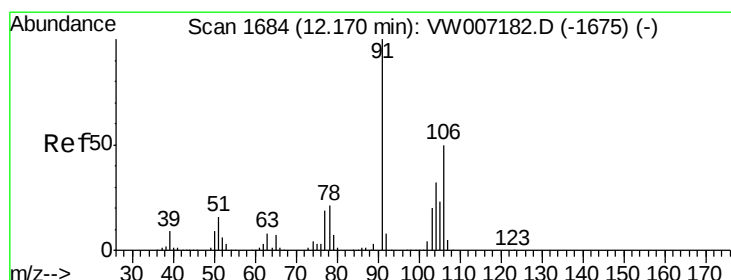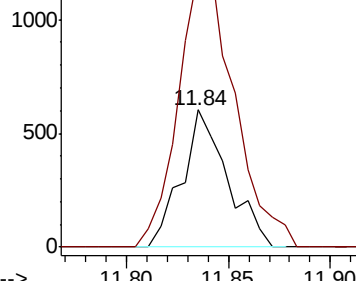

#69

o-Xylene

Concen: 1.029 ug/l

RT: 12.18 min Scan# 1685

Delta R.T. 0.01 min

Lab File: VW007290.D


Acq: 06 Dec 2018 20:25

Tgt Ion:106 Resp: 565

Ion Ratio Lower Upper



106 100


91 239.8 104.9 314.7

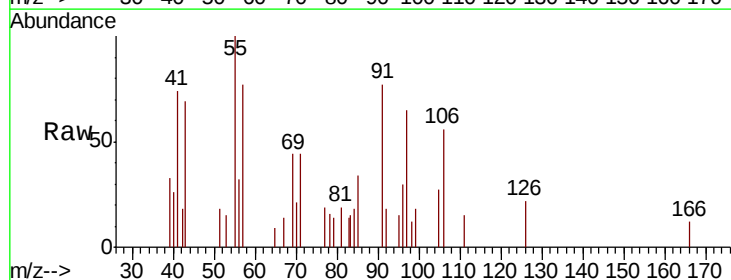

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VW

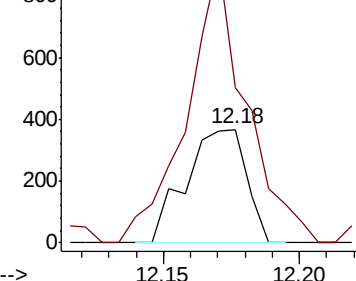

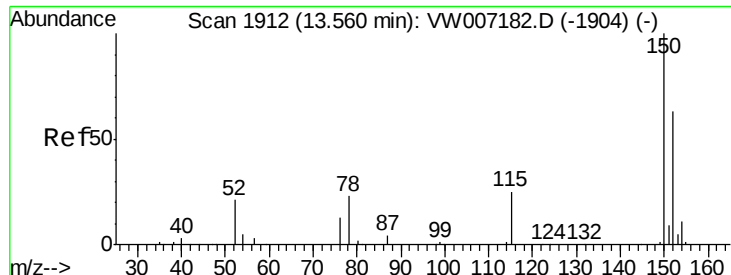

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.56 min Scan# 1912

Delta R.T. -0.00 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W

ClientSampleId :


Tot Ion:152 Resp: 13109

Ion Ratio Lower Upper

152 100

115 59.1 31.3 93.8




150 151.9 0.0 358.0

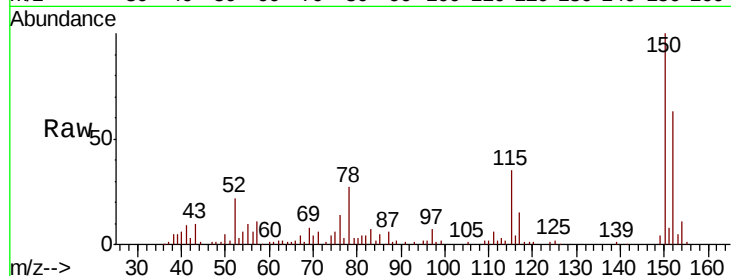

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

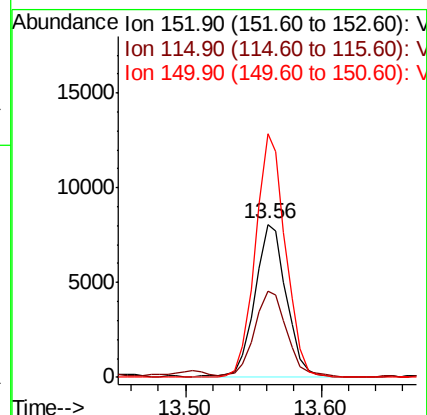

#73

Isopropylbenzene

Concen: 1.442 ug/l

RT: 12.47 min Scan# 1733

Delta R.T. -0.00 min

Lab File: VW007290.D


Acq: 06 Dec 2018 20:25

Tgt Ion:105 Resp: 1537

Ion Ratio Lower Upper



105 100


120 23.7 13.2 39.6



Abundance Ion 105.00 (104.70 to 105.70): V

Ion 120.00 (119.70 to 120.70): V

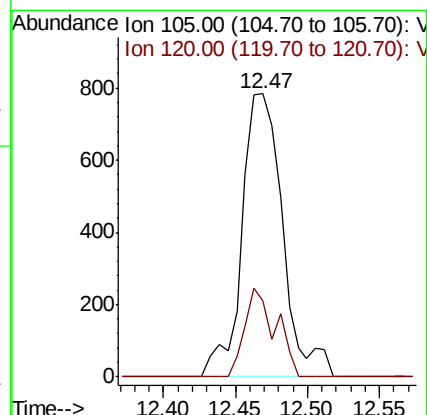



#74

N-amvl acetate

Concen: 27.863 ug/l

RT: 12.26 min Scan# 1698

Delta R.T. -0.02 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W

ClientSampled :

Tot Ion: 43 Resp: 5267



Ion Ratio Lower Upper

43 100

70 21.5 34.0 51.0#

55 40.5 19.0 28.6#

61 0.0 19.7 29.5#


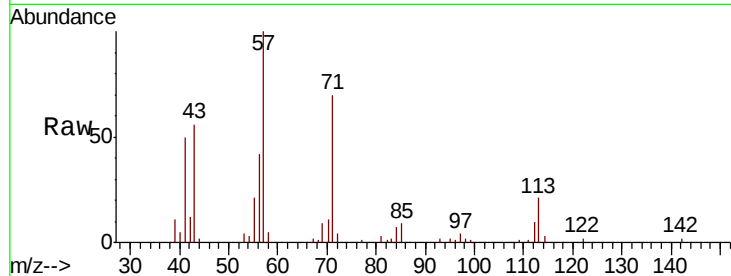


Abundance Ion 43.00 (42.70 to 43.70): VW

Ion 70.00 (69.70 to 70.70): VW

Ion 55.00 (54.70 to 55.70): VW

Ion 61.00 (60.70 to 61.70): VW

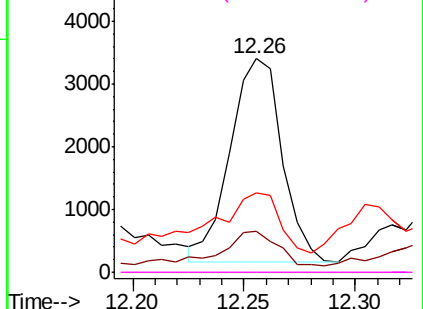

#75

1,1,2,2-Tetrachloroethane

Concen: 2.311 ug/l

RT: 12.69 min Scan# 1769

Delta R.T. -0.03 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25



Tgt Ion: 83 Resp: 320

Ion Ratio Lower Upper

83 100

131 0.0 6.0 18.1#


85 169.4 33.0 99.0#




Abundance Ion 82.90 (82.60 to 83.60): VW

Ion 130.80 (130.50 to 131.50): V

Ion 84.90 (84.60 to 85.60): VW




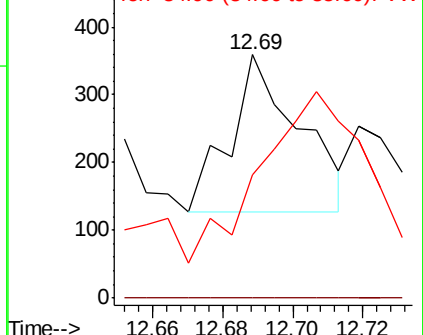


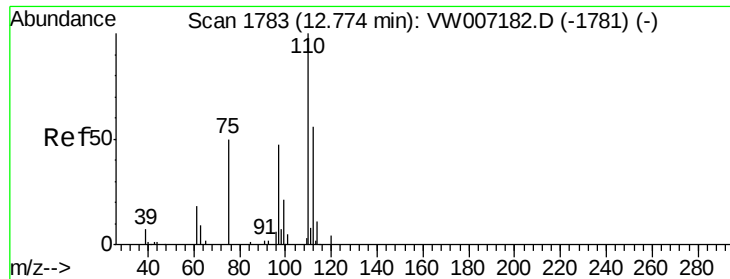

#76
 1,2,3-Trichloropropane
 Concen: 61.948 ug/l
 RT: 12.62 min Scan# 1758
 Delta R.T. -0.15 min
 Lab File: VW007290.D
 Acq: 06 Dec 2018 20:25




Instrument :
 MSVOA_W
 ClientSampleId :


Tot Ion: 75 Resp: 6288
 Ion Ratio Lower Upper
 75 100
 77 2.8 0.0 0.0#

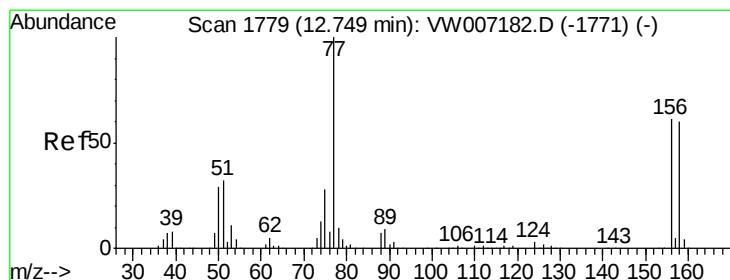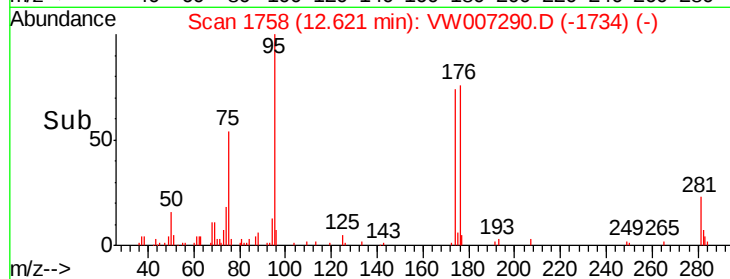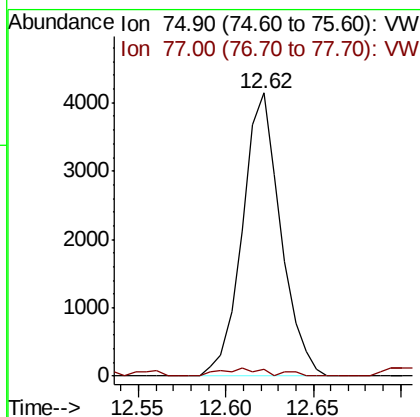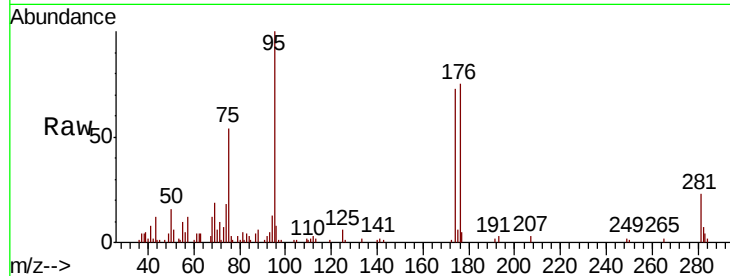

#77
 Bromobenzene
 Concen: 2.955 ug/l
 RT: 12.88 min Scan# 1801
 Delta R.T. 0.13 min
 Lab File: VW007290.D
 Acq: 06 Dec 2018 20:25

Tgt Ion: 156 Resp: 680
 Ion Ratio Lower Upper
 156 100
 77 84.3 92.0 276.1#
 158 0.0 49.0 147.0#

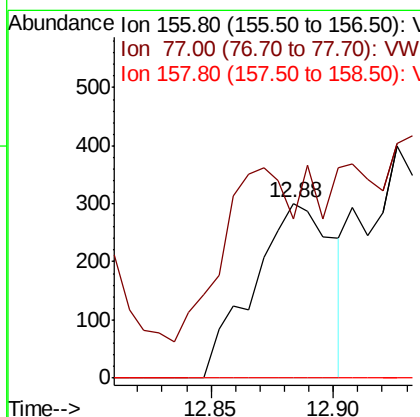



#78

n-propylbenzene

Concen: 3.399 ug/l

RT: 12.81 min Scan# 1789

Delta R.T. -0.00 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W





ClientSampleId :

Tot Ion: 91 Resp: 4318

Ion Ratio Lower Upper

91 100

120 27.3 12.5 37.5

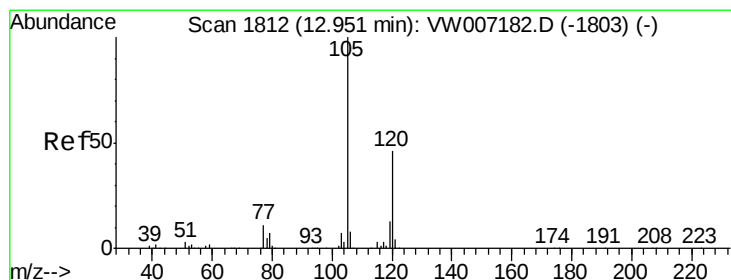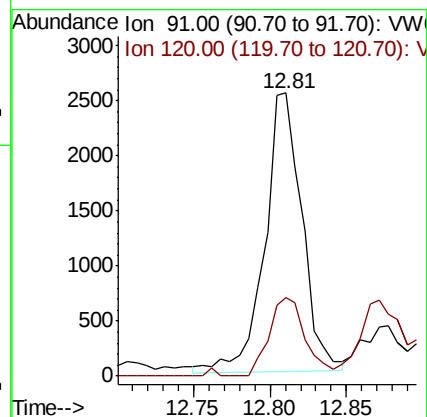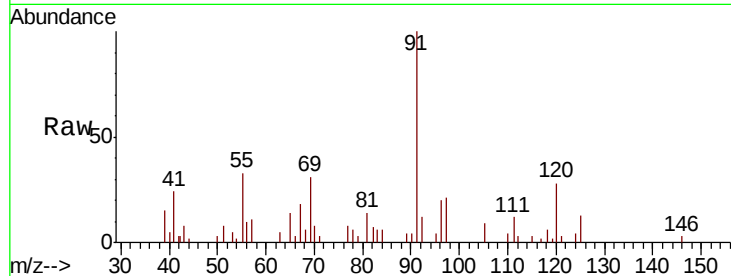

#80

1,3,5-Trimethylbenzene

Concen: 3.666 ug/l

RT: 12.94 min Scan# 1811

Delta R.T. -0.01 min

Lab File: VW007290.D




Acq: 06 Dec 2018 20:25


Tgt Ion:105 Resp: 3344

Ion Ratio Lower Upper

105 100

120 51.3 23.8 71.5

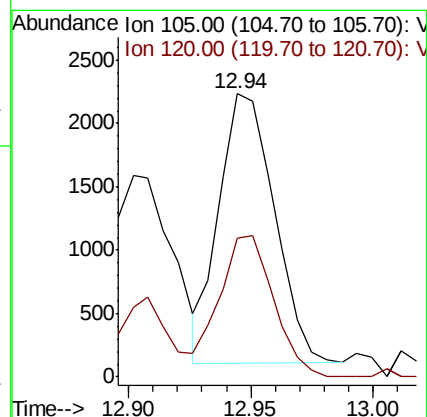

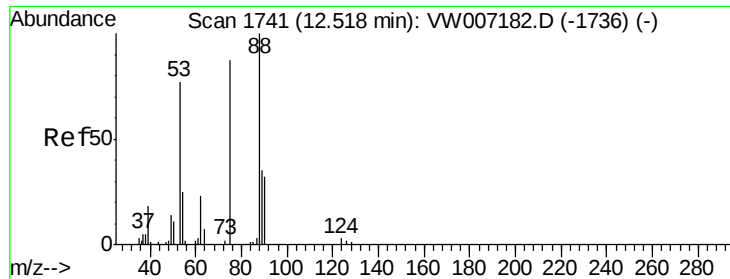

#81

trans-1,4-Dichloro-2-butene

Concen: 133.520 ug/l

RT: 12.62 min Scan# 1758

Delta R.T. 0.10 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W

ClientSampleId :


Tot Ion: 75 Resp: 6288

Ion Ratio Lower Upper

75 100

53 5.6 72.8 109.2#




89 0.0 36.4 54.6#



Abundance Ion 74.90 (74.60 to 75.60): VW

Ion 53.00 (52.70 to 53.70): VW

Ion 88.90 (88.60 to 89.60): VW

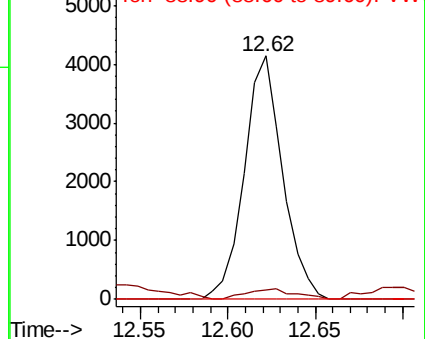

#83

tert-Butylbenzene

Concen: 1.011 ug/l

RT: 13.21 min Scan# 1854

Delta R.T. -0.01 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25


Tgt Ion: 119 Resp: 806

Ion Ratio Lower Upper

119 100

91 66.5 34.0 101.8



134 15.5 13.2 39.5




Abundance Ion 119.00 (118.70 to 119.70): V

Ion 91.00 (90.70 to 91.70): VW

Ion 134.00 (133.70 to 134.70): V




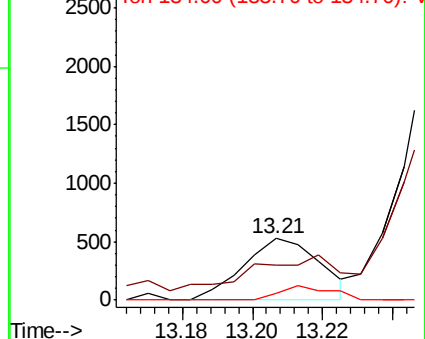




#84
1,2,4-Trimethylbenzene
Concen: 30.621 ug/l
RT: 13.26 min Scan# 1862
Delta R.T. 0.00 min
Lab File: VW007290.D
Acq: 06 Dec 2018 20:25




Instrument :
MSVOA_W
ClientSampleId :


Tot Ion:105 Resp: 28510
Ion Ratio Lower Upper
105 100
120 43.2 21.1 63.3

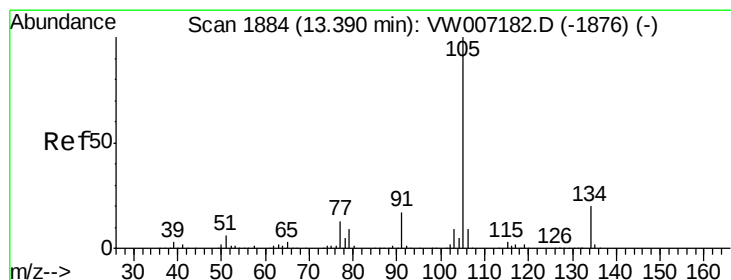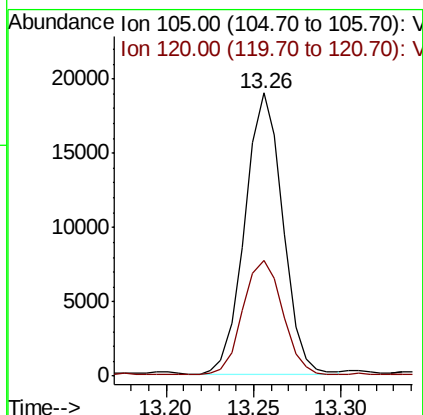

#85
sec-Butylbenzene
Concen: 4.693 ug/l
RT: 13.39 min Scan# 1884
Delta R.T. -0.00 min
Lab File: VW007290.D
Acq: 06 Dec 2018 20:25

Tgt Ion:105 Resp: 5340
Ion Ratio Lower Upper
105 100
134 33.8 10.3 30.8#



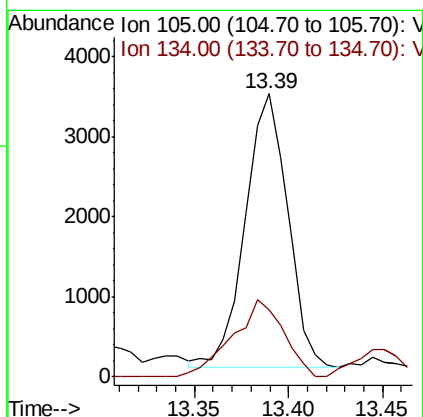
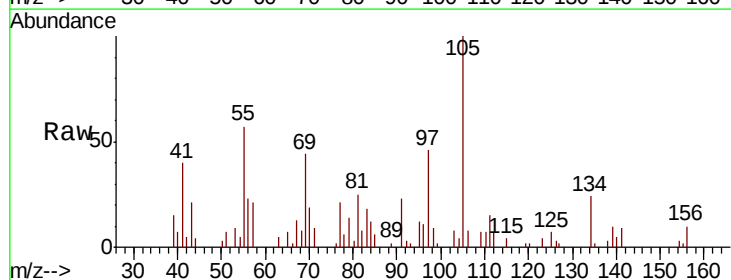


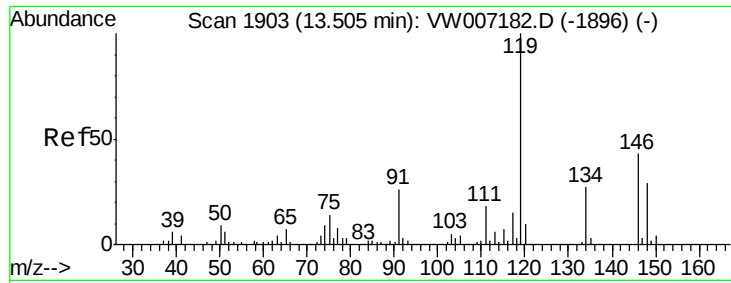

#86
 p-Isopropyltoluene
 Concen: 4.389 ug/l
 RT: 13.51 min Scan# 1903
 Delta R.T. -0.00 min
 Lab File: VW007290.D
 Acq: 06 Dec 2018 20:25




Instrument :
 MSVOA_W
 ClientSampleId :


Tot Ion: 119 Resp: 4446
 Ion Ratio Lower Upper
 119 100
 134 30.2 13.2 39.6
 91 28.0 12.4 37.2

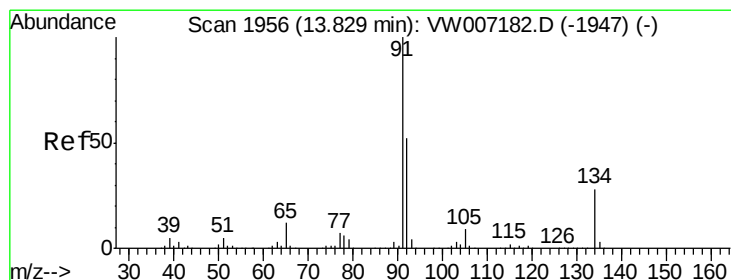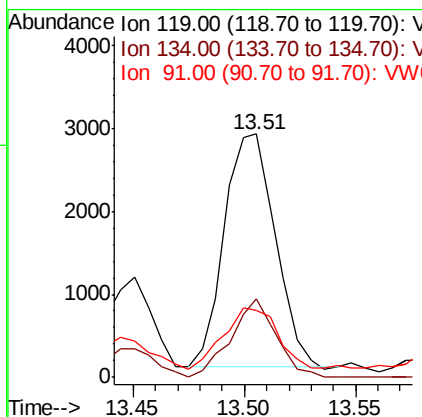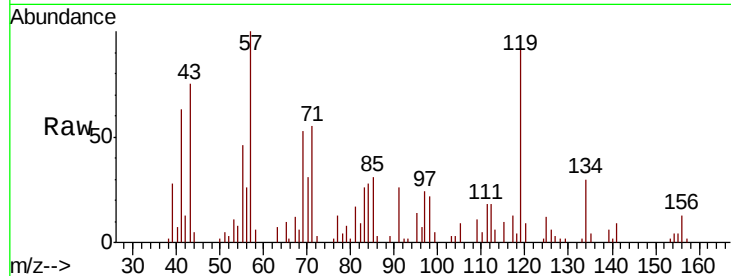

#89
 n-Butylbenzene
 Concen: 8.935 ug/l
 RT: 13.83 min Scan# 1956
 Delta R.T. 0.00 min
 Lab File: VW007290.D
 Acq: 06 Dec 2018 20:25

Tgt Ion: 91 Resp: 8458
 Ion Ratio Lower Upper
 91 100
 92 45.1 26.5 79.5
 134 0.0 14.1 42.2#

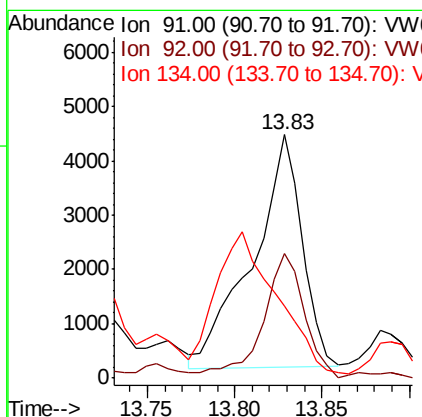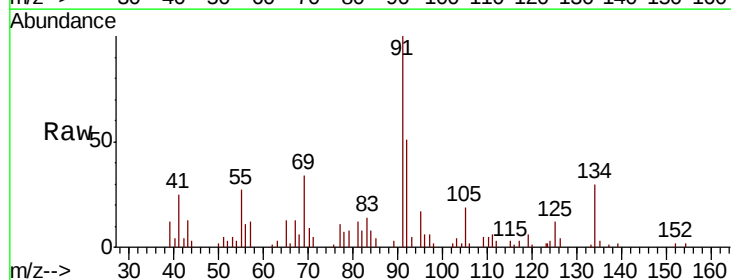

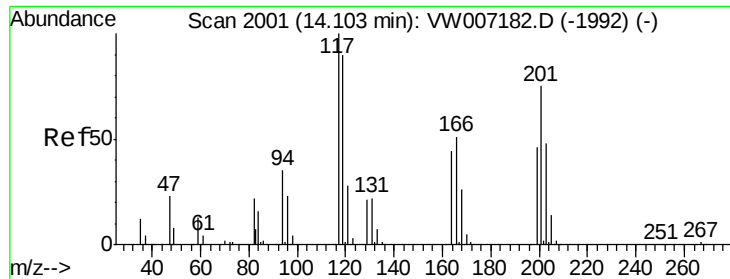

#90

Hexachloroethane

Concen: 17.569 ug/l

RT: 14.10 min Scan# 2001

Delta R.T. -0.00 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25

Instrument :

MSVOA_W


ClientSampleId :

Tot Ion:117 Resp: 2712

Ion Ratio Lower Upper

117 100

201 0.0 36.0 108.1#

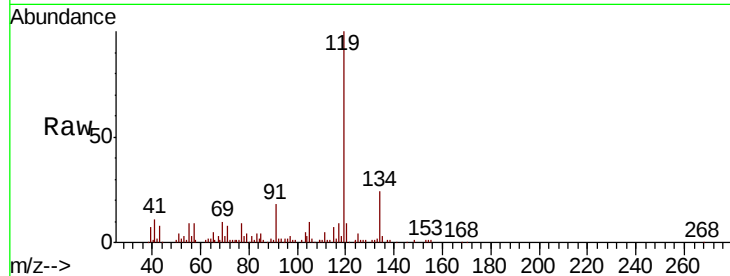

Abundance Ion 116.80 (116.50 to 117.50): V

Ion 200.70 (200.40 to 201.40): V

14.10

14.05

14.10

14.15

14.20

14.25

14.30

14.35

14.40

14.45

14.50

14.55

14.60

14.65

14.70

14.75

14.80

14.85

14.90

14.95

15.00

15.05

15.10

15.15



15.20

15.25

15.30

15.35

15.40

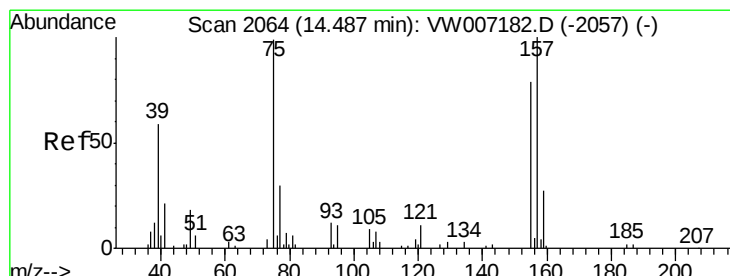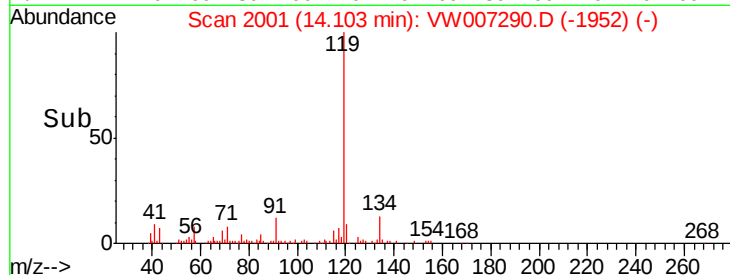

#92

1,2-Dibromo-3-Chloropropane

Concen: 7.120 ug/l

RT: 14.47 min Scan# 2061

Delta R.T. -0.02 min

Lab File: VW007290.D

Acq: 06 Dec 2018 20:25


Tgt Ion: 75 Resp: 191

Ion Ratio Lower Upper

75 100

155 0.0 42.4 127.2#

157 0.0 55.3 165.9#

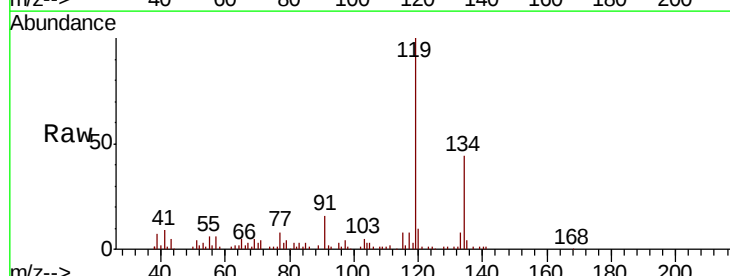

Abundance Ion 74.90 (74.60 to 75.60): VW

Ion 154.80 (154.50 to 155.50): V

Ion 156.80 (156.50 to 157.50): V

14.47

14.44

14.47

14.50

14.53

14.56

14.59

14.62


14.65


14.68

14.71

14.74

14.77






#95
 Naphthalene
 Concen: 15.599 ug/l
 RT: 15.37 min Scan# 2209
 Delta R.T. -0.01 min
 Lab File: VW007290.D
 Acq: 06 Dec 2018 20:25

Instrument :
 MSVOA_W
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
128	100		
127	12.7	10.3	15.5
129	12.4	8.6	13.0



Abundance

Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

