


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW120618\
Data File : VW007280.D
Acq On : 06 Dec 2018 15:01
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W120418S.M
Title : SW846 8260
Last Update : Wed Dec 05 01:35:23 2018

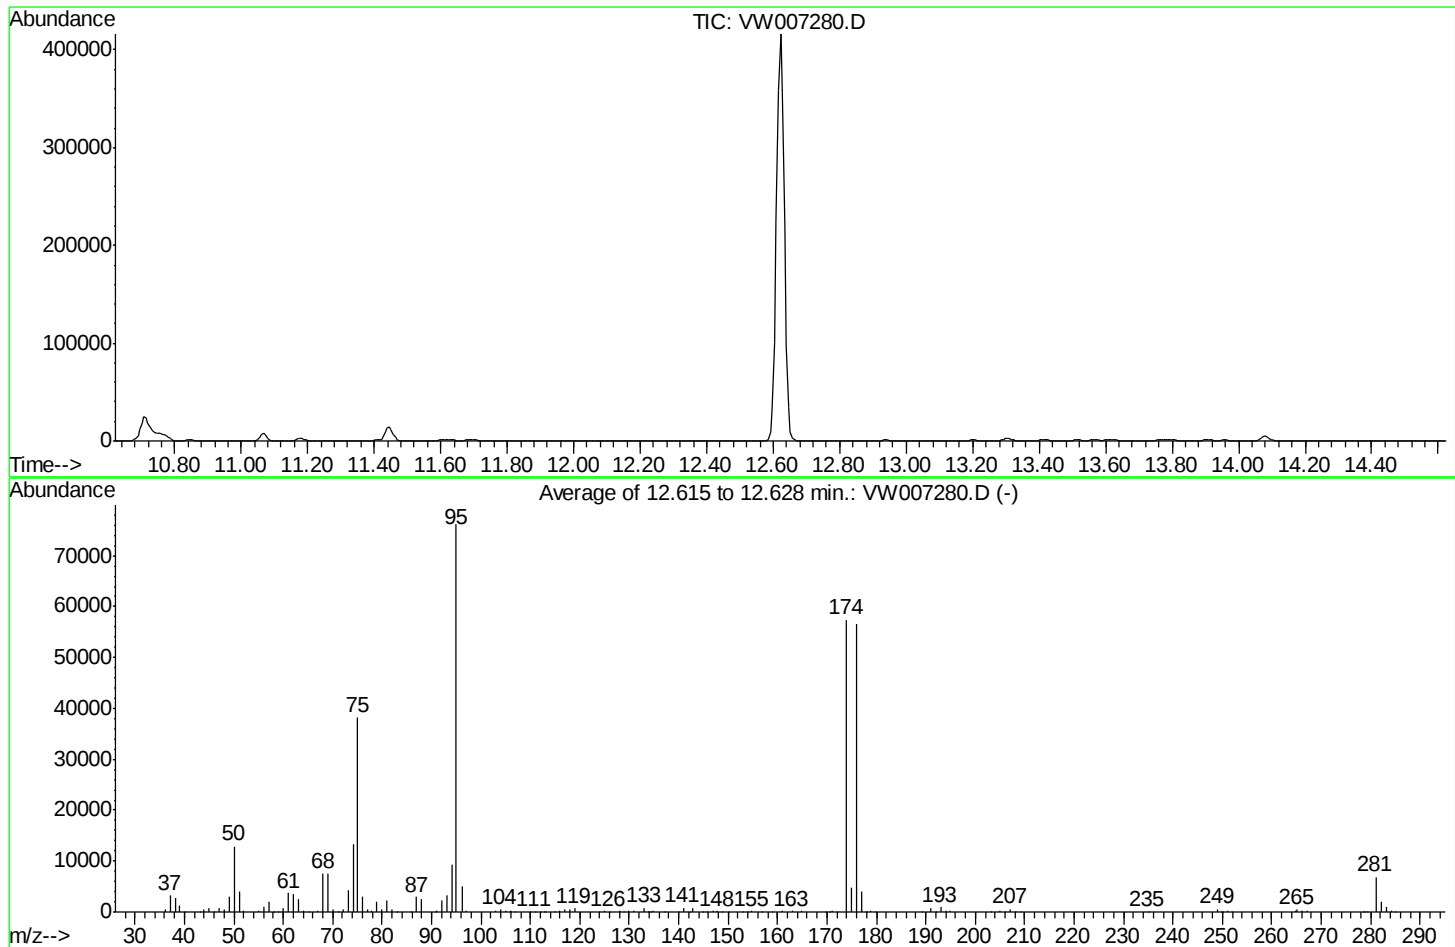

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	12888	PASS
75	95	30	60	50.0	38117	PASS
95	95	100	100	100.0	76160	PASS
96	95	5	9	6.7	5075	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.3	57349	PASS
175	174	5	9	8.2	4687	PASS
176	174	95	101	98.8	56677	PASS
177	176	5	9	7.1	4017	PASS