




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120623\
 Data File : VW027563.D
 Acq On : 06 Dec 2023 12:48
 Operator : SY/MD
 Sample : VW1206SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK598

Manual IntegrationsAPPROVED

Quant Time: Dec 07 07:02:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 07 06:54:07 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/11/2023
 Supervised By :Mahesh Dadoda 12/11/2023

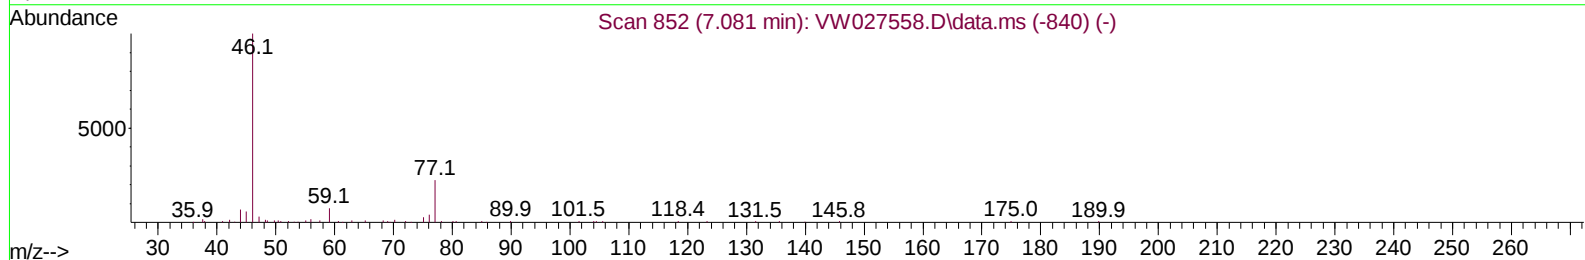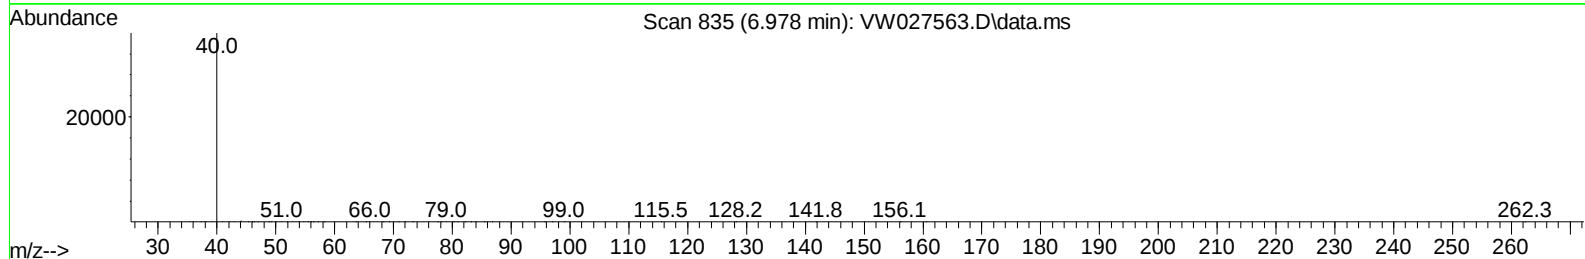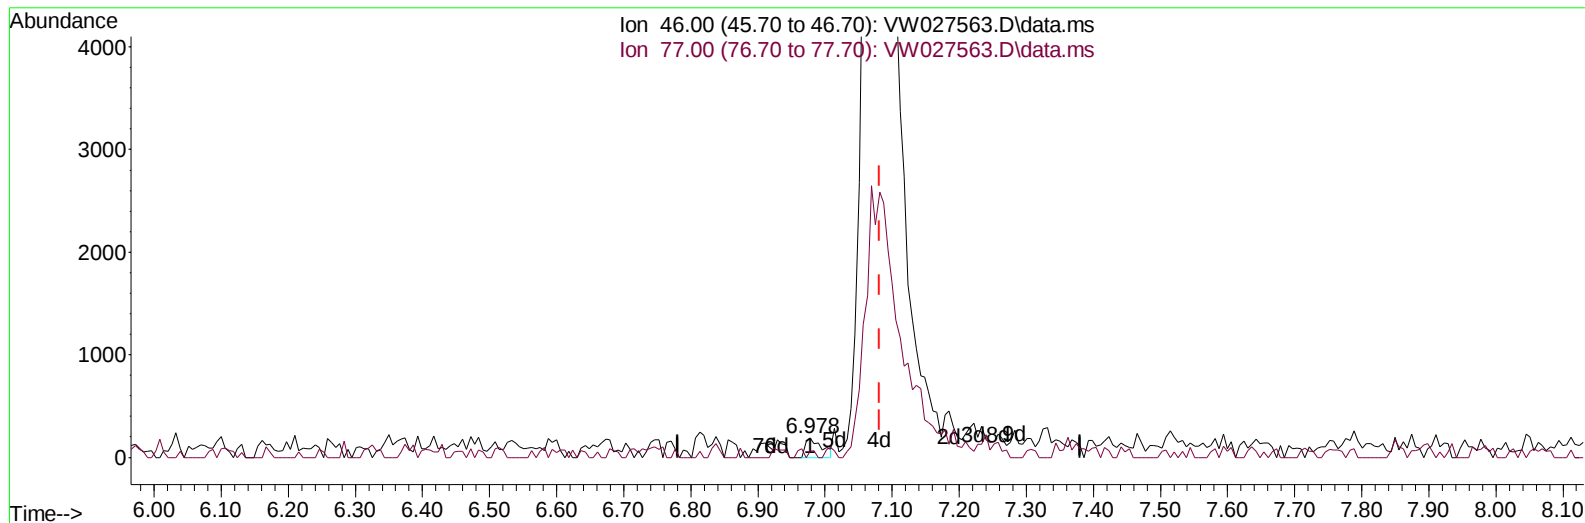

TIC: VW027563.D\data.ms

(21) 2-Butanone-d5 (S)

6.978min (-0.103) 0.26 ug/L

response 315

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	18.30	14.60
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120623\
 Data File : VW027563.D
 Acq On : 06 Dec 2023 12:48
 Operator : SY/MD
 Sample : VW1206SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK598

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/11/2023
 Supervised By :Mahesh Dadoda 12/11/2023

Quant Time: Dec 07 07:02:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 07 06:54:07 2023
 Response via : Initial Calibration

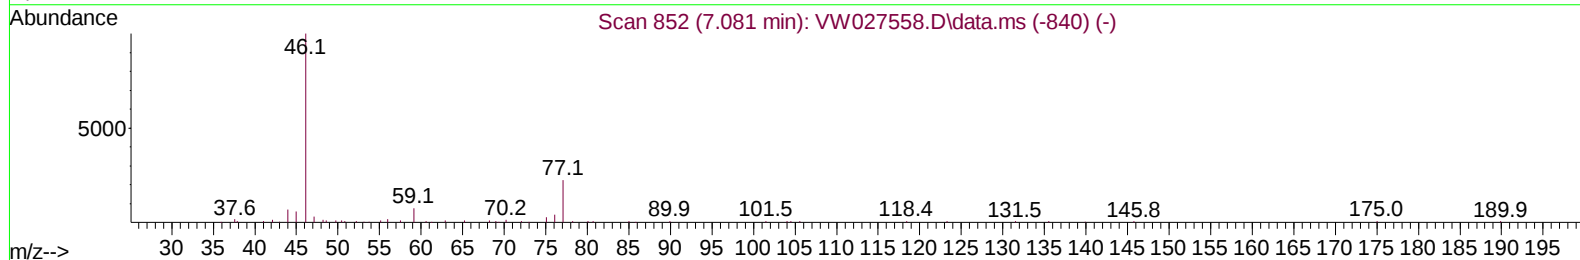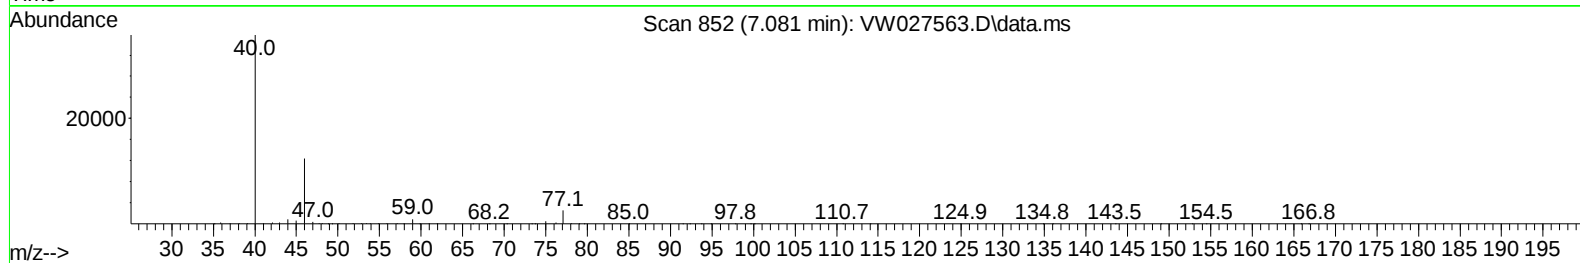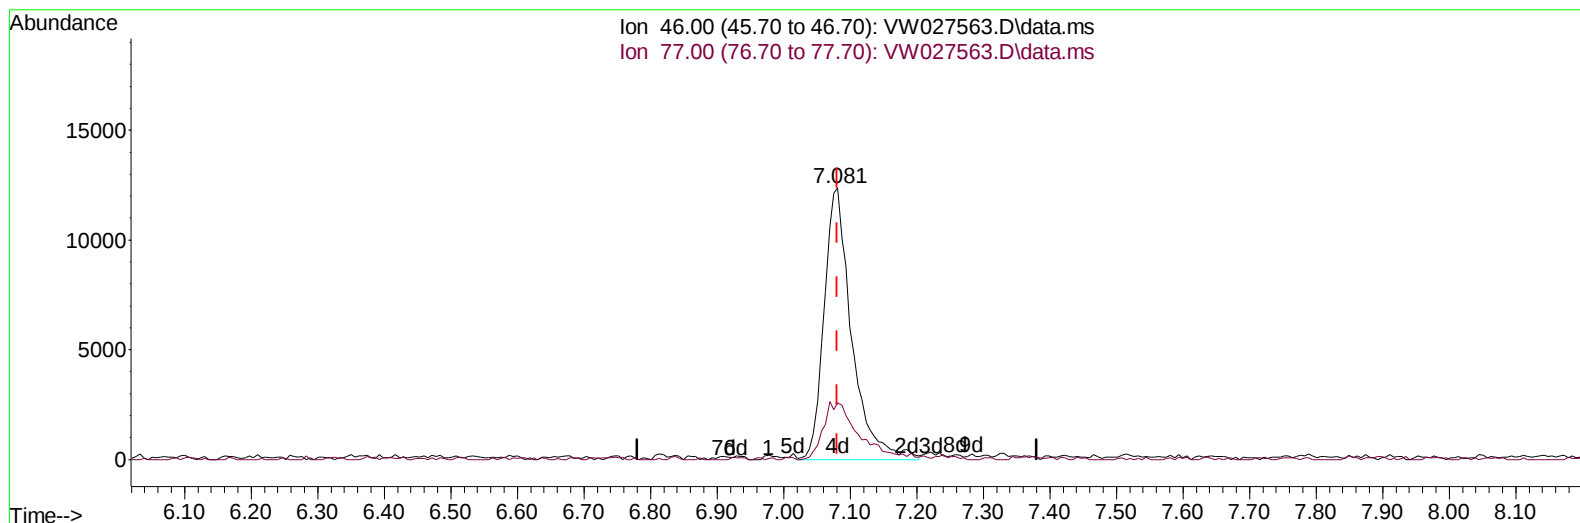

TIC: VW027563.D\data.ms

(21) 2-Butanone-d5 (S)

7.081min (+ 0.000) 28.83 ug/L m

response 35602

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	18.30	0.13#
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120623\
 Data File : VW027563.D
 Acq On : 06 Dec 2023 12:48
 Operator : SY/MD
 Sample : VW1206SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK598

Manual IntegrationsAPPROVED

Quant Time: Dec 07 07:02:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 07 06:54:07 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/11/2023
 Supervised By :Mahesh Dadoda 12/11/2023

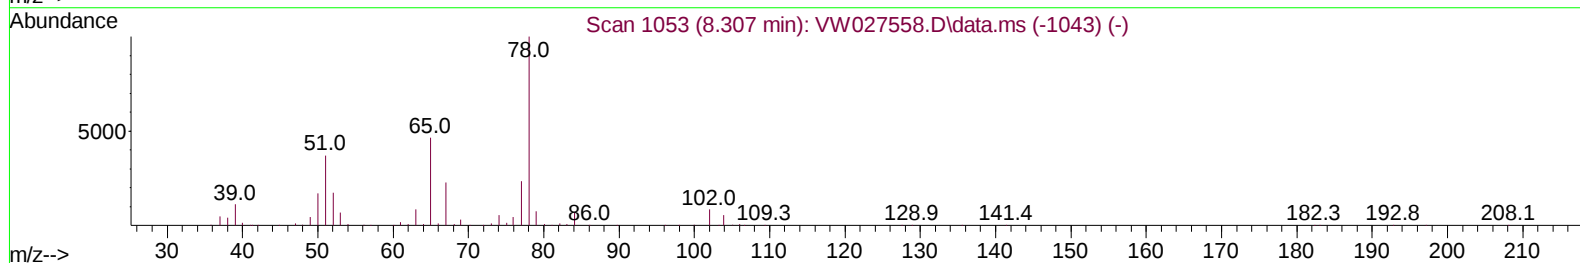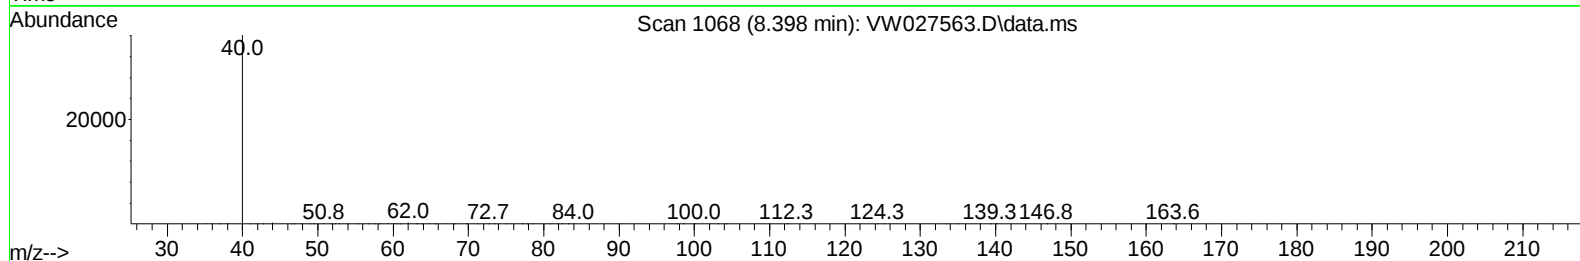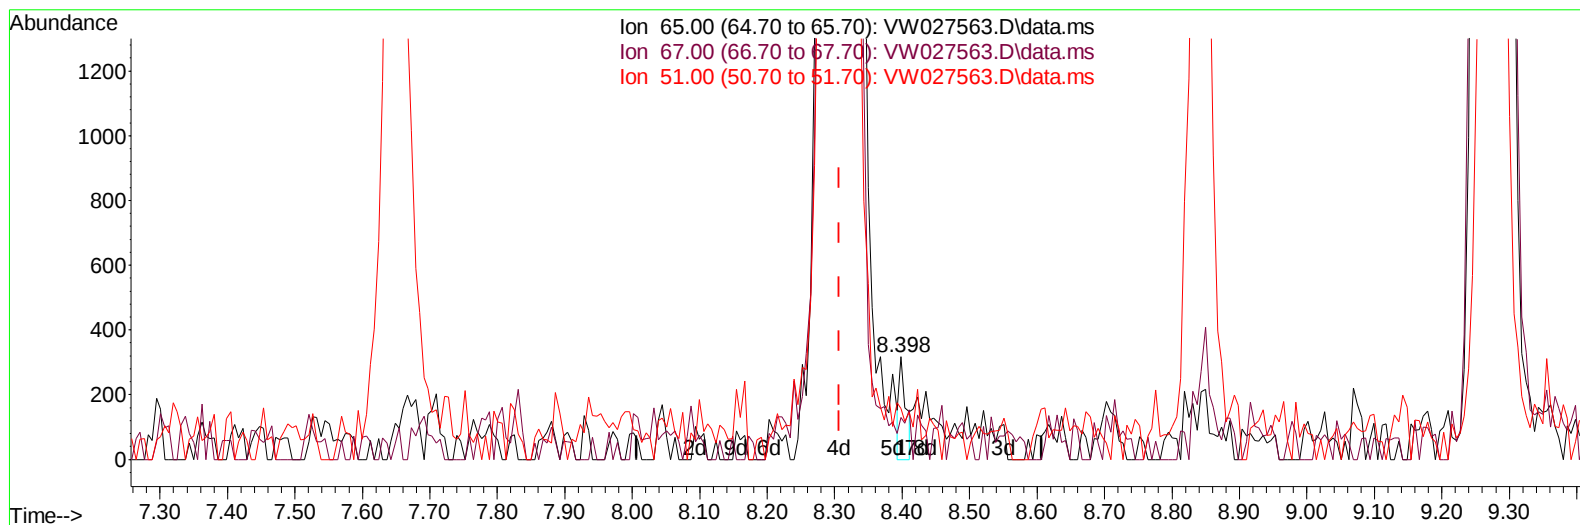

TIC: VW027563.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.398min (+ 0.091) 0.06 ug/L

response 228

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.20	63.60
51.00	135.30	111.40
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120623\
 Data File : VW027563.D
 Acq On : 06 Dec 2023 12:48
 Operator : SY/MD
 Sample : VW1206SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK598

Manual IntegrationsAPPROVED

Quant Time: Dec 07 07:02:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 07 06:54:07 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/11/2023
 Supervised By :Mahesh Dadoda 12/11/2023

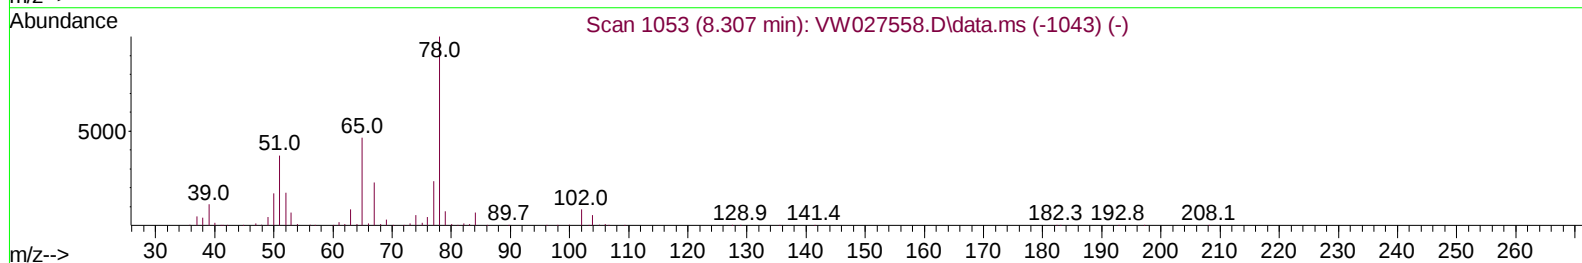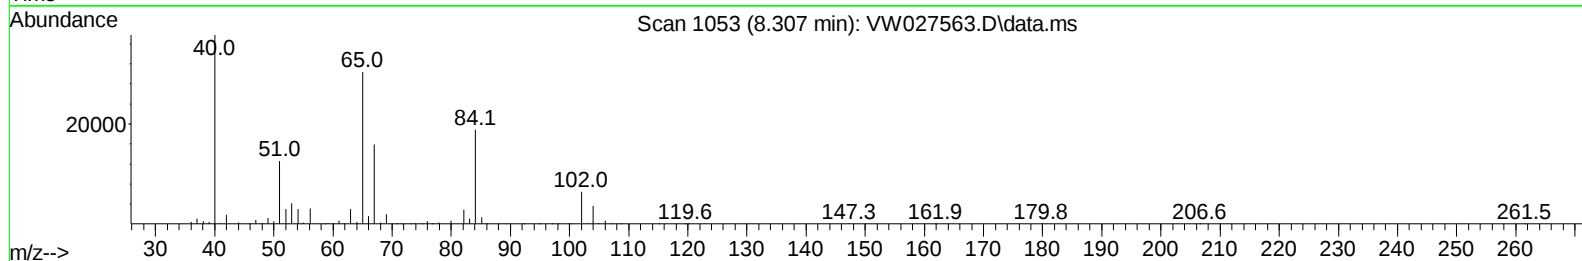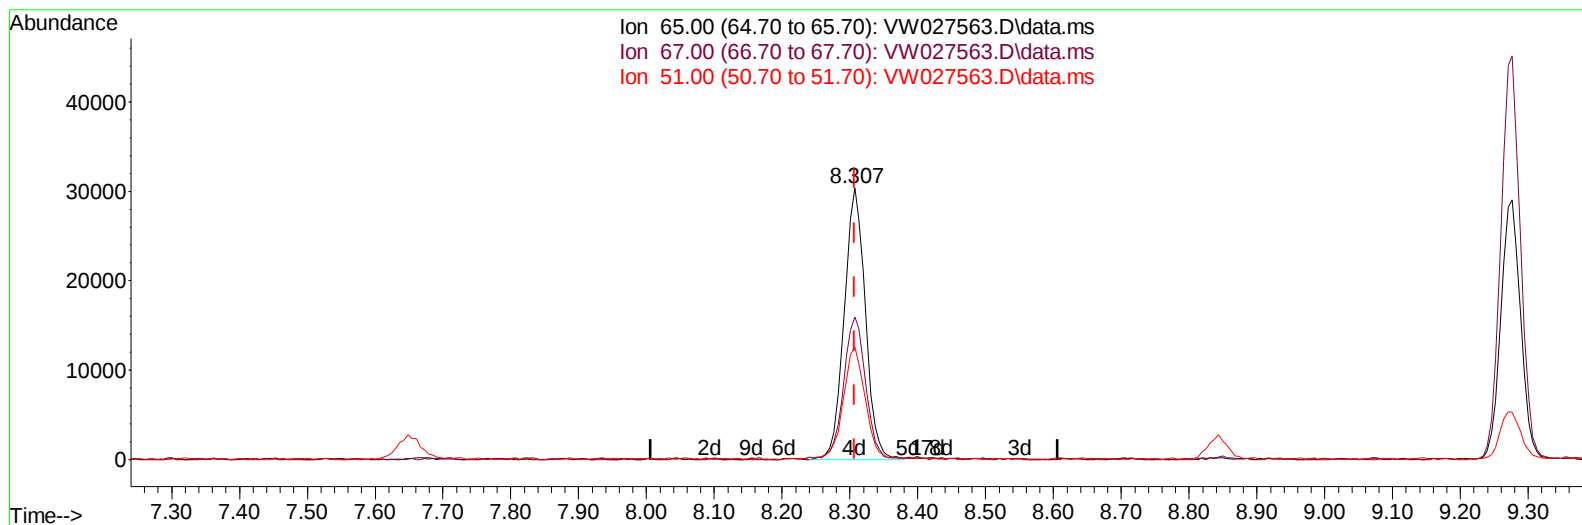

TIC: VW027563.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (-0.000) 18.43 ug/L m

response 65863

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.20	0.22#
51.00	135.30	0.39#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw120623\
 Data File : VW027563.D
 Acq On : 06 Dec 2023 12:48
 Operator : SY/MD
 Sample : VW1206SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK598

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/11/2023
 Supervised By :Mahesh Dadoda 12/11/2023

Quant Time: Dec 07 07:02:01 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Thu Dec 07 06:54:07 2023
 Response via : Initial Calibration

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.843	114		234146	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		191500	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152		85961	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		116044	24.628	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	98.520%		
7) Chloroethane-d5	2.899	69		83858	24.550	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery =	98.200%		
11) 1,1-Dichloroethene-d2	4.027	65		51340	25.750	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery =	103.000%		
21) 2-Butanone-d5	7.081	46		35602m	28.835	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	57.660%		
24) Chloroform-d	7.648	84		151540	21.682	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery =	86.720%		
26) 1,2-Dichloroethane-d4	8.307	65		65863m	18.428	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery =	73.720%		
32) Benzene-d6	8.276	84		338841	25.122	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery =	100.480%		
36) 1,2-Dichloropropane-d6	9.276	67		91626	23.044	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery =	92.160%		
41) Toluene-d8	10.325	98		297345	25.197	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery =	100.800%		
43) trans-1,3-Dichloroprop...	10.575	79		28835	18.753	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery =	75.000%		
47) 2-Hexanone-d5	10.922	63		21591	29.143	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery =	58.280%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84		54806	16.757	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery =	67.040%		
66) 1,2-Dichlorobenzene-d4	13.849	152		65816	21.842	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery =	87.360%		

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120623\
Data File : VW027563.D
Acq On : 06 Dec 2023 12:48
Operator : SY/MD
Sample : VW1206SBL01
Misc : 5.00g/10mL/MSVOA_W/SoIL
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK598

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/11/2023
Supervised By :Mahesh Dadoda 12/11/2023

Quant Time: Dec 07 07:02:01 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
Quant Title : SFAM01.0
QLast Update : Thu Dec 07 06:54:07 2023
Response via : Initial Calibration

