

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW120718\
 Data File : VW007317.D
 Acq On : 07 Dec 2018 20:07
 Operator : SY/AP
 Sample : VIBLK92
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK92

Manual Integrations
 APPROVED

MMDadoda
 12/11/2018 4:08:57 PM

Quant Time: Dec 08 03:22:26 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Quant Title : VOC Analysis
 QLast Update : Sat Dec 08 02:02:23 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	143683	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	123955	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	60998	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	25174	26.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.60%
7) Chloroethane-d5	2.90	69	19833	25.02	ug/L	0.01
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.08%
10) 1,1-Dichloroethene-d2	4.01	63	60342	18.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.76%
20) 2-Butanone-d5	7.08	46	25874	43.86	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	87.72%
24) Chloroform-d	7.65	84	80731	23.82	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.28%
26) 1,2-Dichloroethane-d4	8.31	65	48071	24.92	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.68%
29) Benzene-d6	8.27	84	164932	24.50	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.00%
33) 1,2-Dichloropropane-d6	9.27	67	46423	24.16	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.64%
37) Toluene-d8	10.32	98	157815	25.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.00%
38) trans-1,3-Dichloropropene-	10.58	79	23067	23.49	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	93.96%
39) 2-Hexanone-d5	10.93	63	21024	45.46	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.92%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	39727	22.69	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.76%
61) 1,2-Dichlorobenzene-d4	13.86	152	52891	24.65	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.60%

Target Compounds					Qvalue
16) Methylene chloride	4.92	84	5051m	2.176	ug/L

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW120718\
Data File : VW007317.D
Acq On : 07 Dec 2018 20:07
Operator : SY/AP
Sample : VIBLK92
Misc : 5.00G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1


Instrument :
MSVOA_W
ClientSampleId :
VIBLK92

Manual Integrations
APPROVED

MMDadoda
12/11/2018 4:08:57 PM

Quant Time: Dec 08 03:22:26 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
Quant Title : VOC Analysis
QLast Update : Sat Dec 08 02:02:23 2018
Response via : Initial Calibration

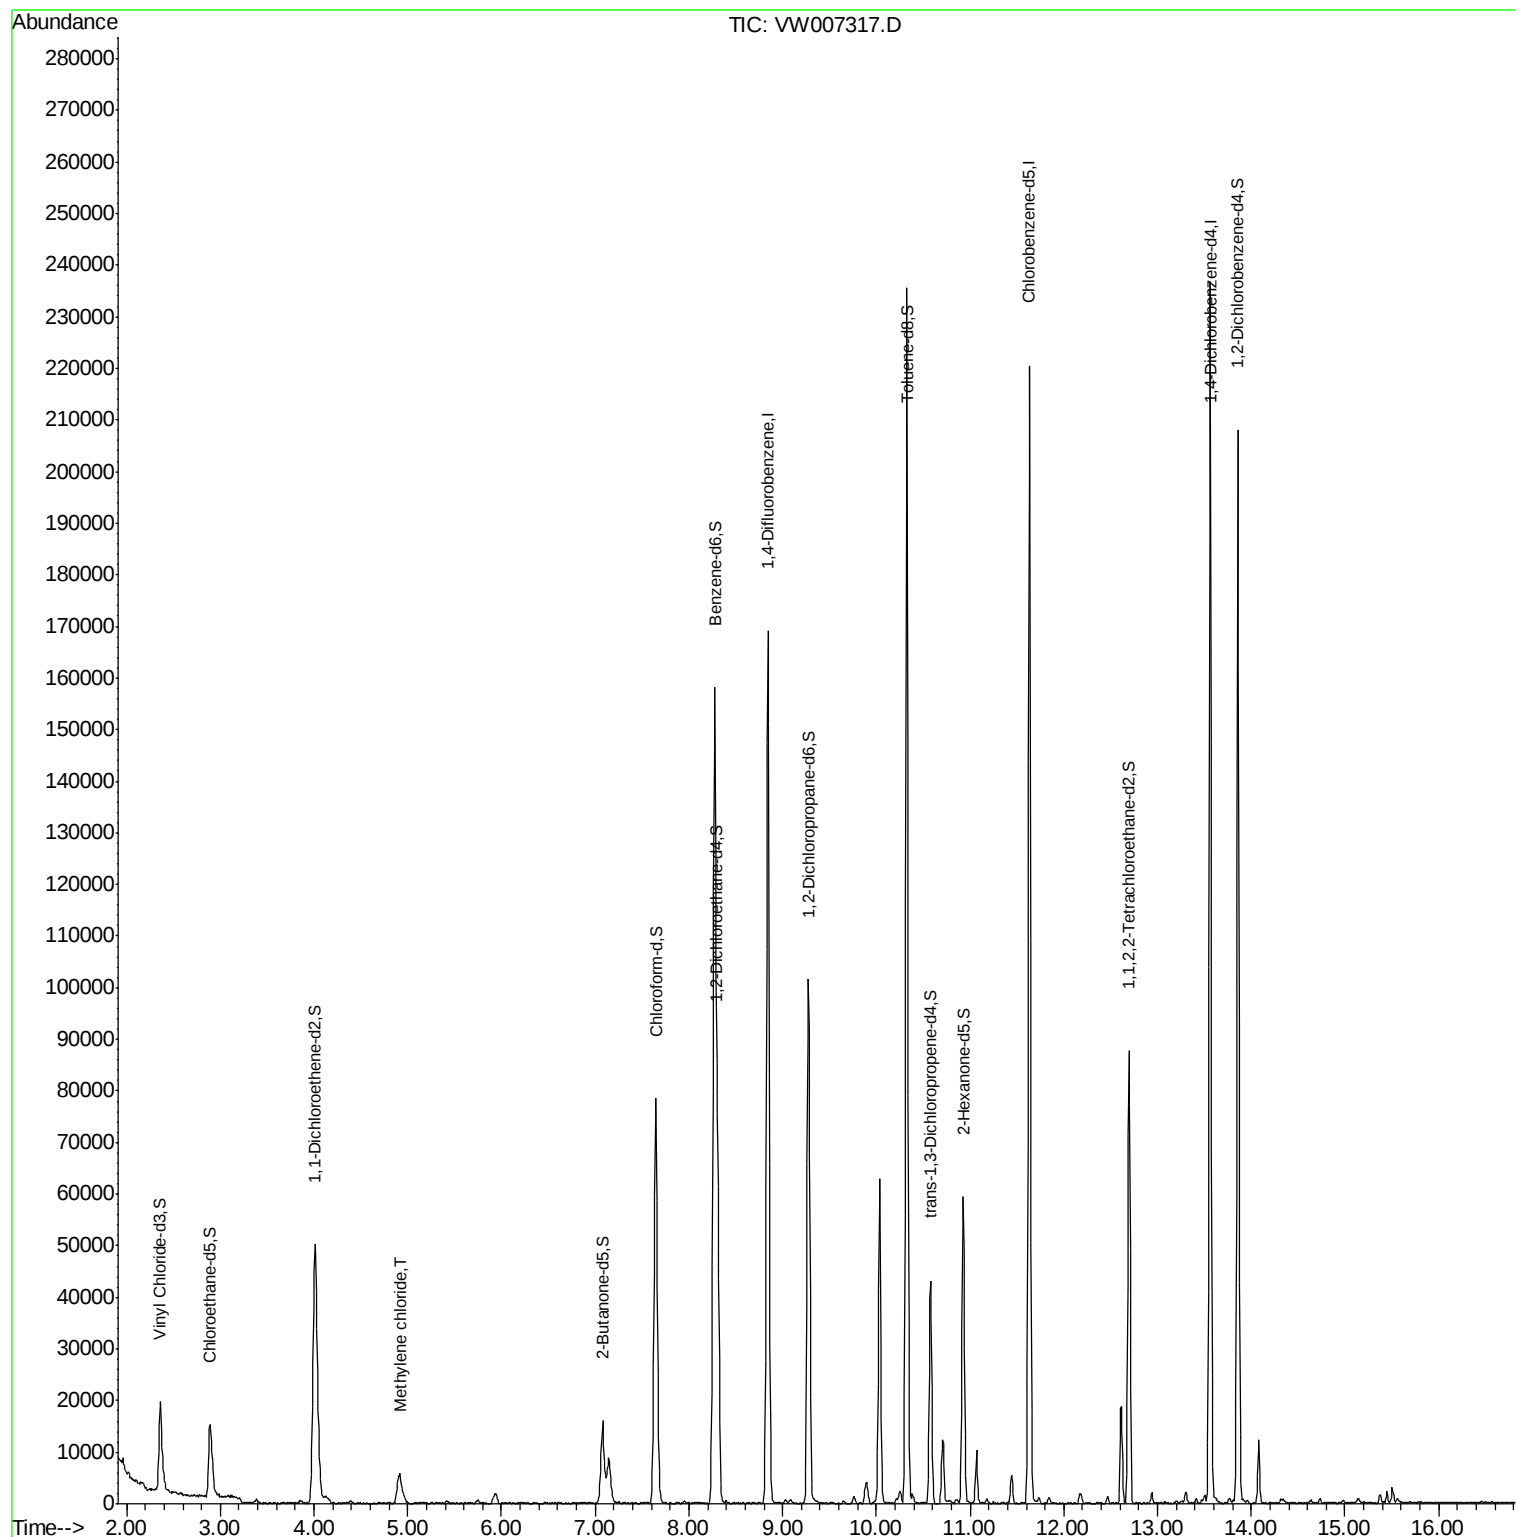

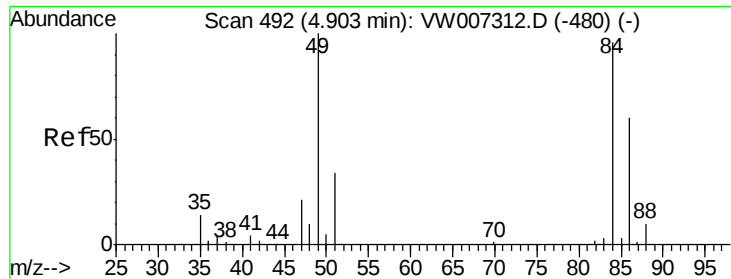

#16
Methylene chloride
Concen: 2.176 ug/L m
RT: 4.92 min Scan# 494
Delta R.T. 0.01 min
Lab File: VW007317.D
Acq: 07 Dec 2018 20:07

Instrument :
MSVOA_W
ClientSampleId :
VIBLK92

Tgt Ion:	84	Resp:	5051
Ion Ratio	Lower	Upper	
84	100		
49	125.3	80.8	150.2
86	74.8	45.8	85.2

Manual Integrations
APPROVED

MMDadoda
12/11/2018 4:08:57 PM

