

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW120718\
 Data File : VW007339.D
 Acq On : 08 Dec 2018 06:54
 Operator : SY/AP
 Sample : J6270-08
 Misc : 6.53G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F9E07

Quant Time: Dec 10 06:26:04 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Quant Title : VOC Analysis
 QLast Update : Mon Dec 10 05:52:22 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	131911	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	113584	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	51604	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	24049	27.99	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	111.96%
7) Chloroethane-d5	2.89	69	17790	24.45	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.80%
10) 1,1-Dichloroethene-d2	4.01	63	55079	18.59	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	74.36%
20) 2-Butanone-d5	7.08	46	17489	32.29	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	64.58%
24) Chloroform-d	7.65	84	72656	23.35	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	93.40%
26) 1,2-Dichloroethane-d4	8.31	65	41665	23.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.12%
29) Benzene-d6	8.27	84	147107	23.85	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.40%
33) 1,2-Dichloropropane-d6	9.27	67	40011	22.73	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	90.92%
37) Toluene-d8	10.32	98	137605	23.79	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.16%
38) trans-1,3-Dichloropropene-	10.58	79	18038	20.04	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.16%
39) 2-Hexanone-d5	10.93	63	12766	30.12	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	60.24%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	31227	19.47	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	77.88%
61) 1,2-Dichlorobenzene-d4	13.86	152	41219	22.71	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	90.84%


Target Compounds					Qvalue
13) Acetone	4.12	43	14625	23.223 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW120718\
Data File : VW007339.D
Acq On : 08 Dec 2018 06:54
Operator : SY/AP
Sample : J6270-08
Misc : 6.53G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F9E07

Quant Time: Dec 10 06:26:04 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
Quant Title : VOC Analysis
QLast Update : Mon Dec 10 05:52:22 2018
Response via : Initial Calibration

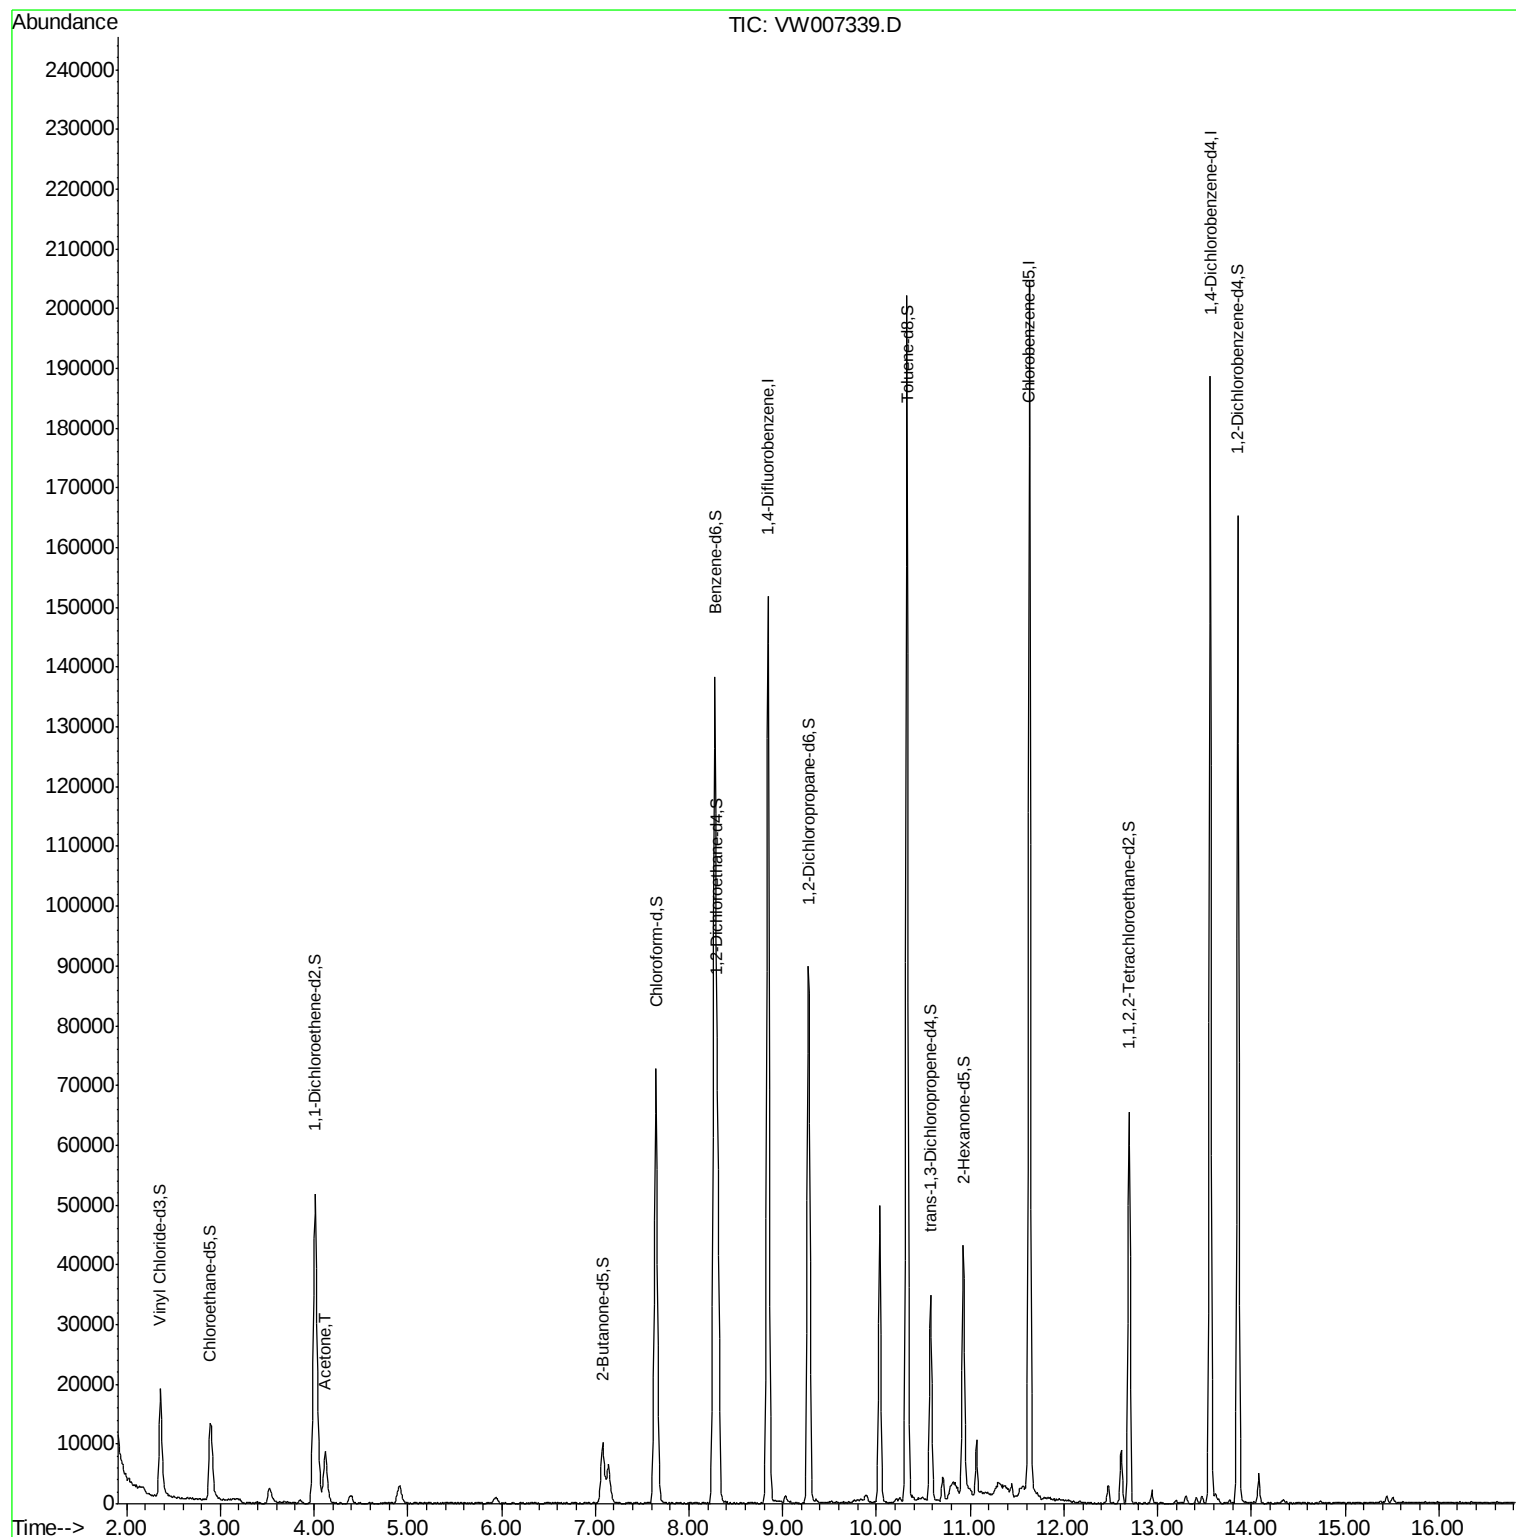

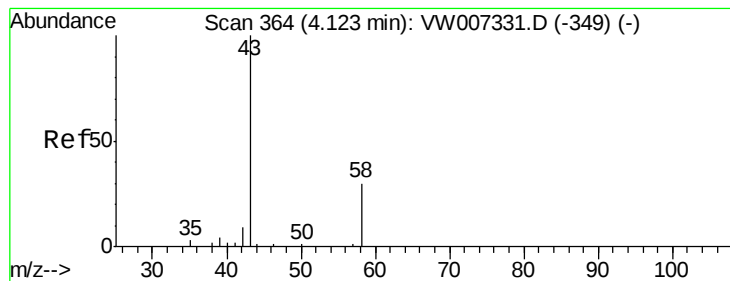

#13

Acetone

Concen: 23.223 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.00 min

Lab File: VW007339.D

Acq: 08 Dec 2018 06:54

Instrument :
MSVOA_W
ClientSampleId :
F9E07

Tgt Ion: 43 Resp: 14625

Ion Ratio Lower Upper

43 100

58 29.8 0.0 59.2

