


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW120718\
 Data File : VW007305.D
 Acq On : 07 Dec 2018 12:22
 Operator : SY/AP
 Sample : BFB83
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB83

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Title : VOC Analysis
 Last Update : Tue Dec 11 01:18:15 2018

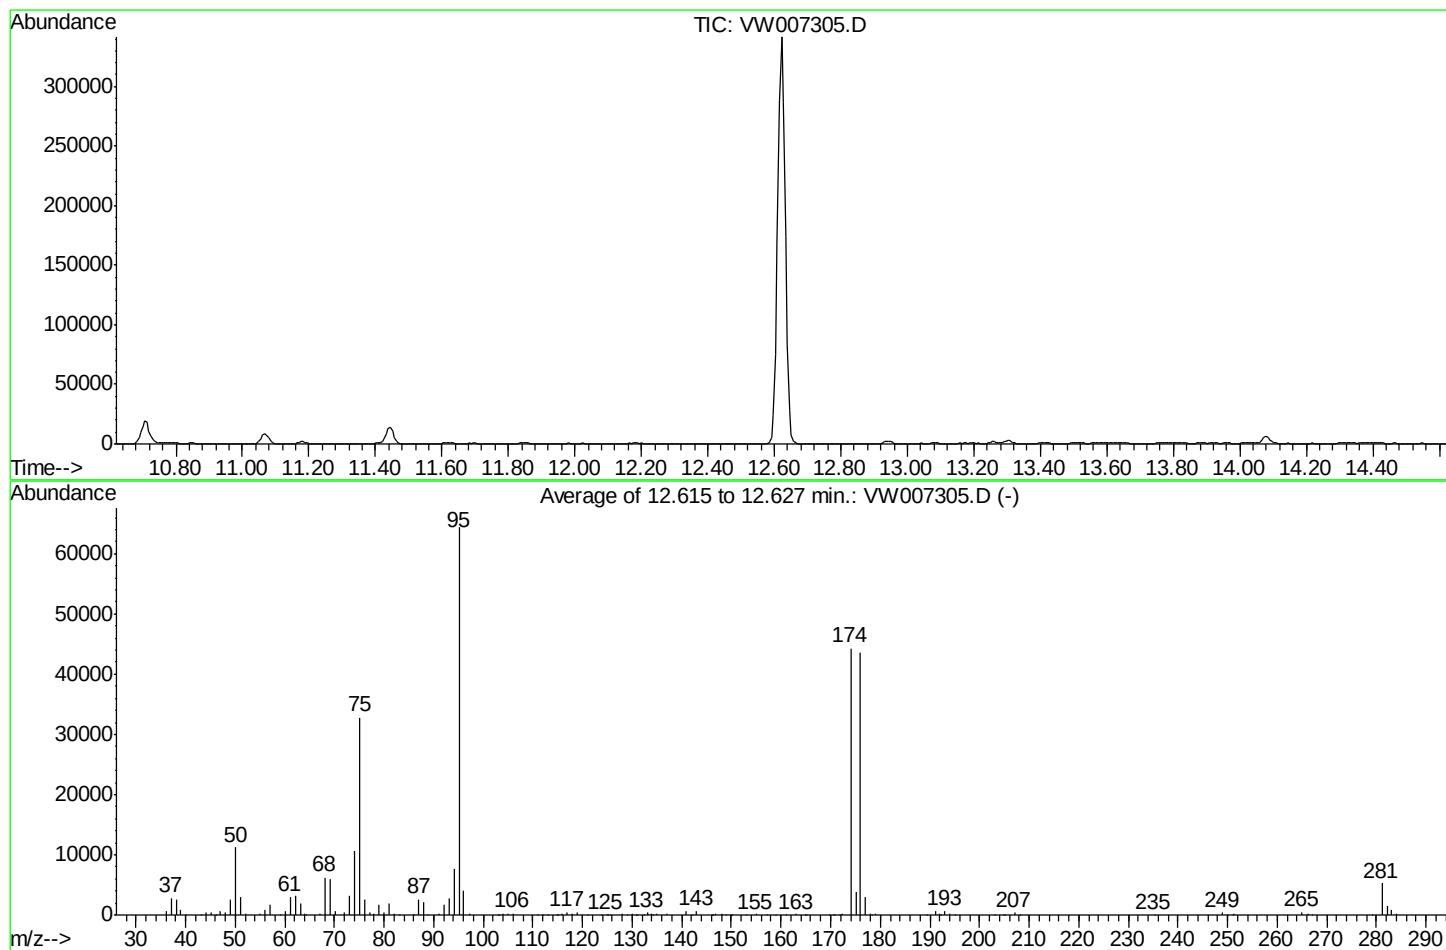

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.4	11215	PASS
75	95	30	80	51.0	32834	PASS
95	95	100	100	100.0	64392	PASS
96	95	5	9	6.4	4130	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	68.8	44285	PASS
175	174	5	9	8.8	3877	PASS
176	174	95	101	98.6	43658	PASS
177	176	5	9	6.9	3030	PASS

Scan 1750 (12.572 min): VW007305.D
BFB83

m/z	Abundance
40.00	99.0
41.00	71.0
55.00	64.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

m/z	Abundance
36.00	597.0
37.10	3184.0
38.10	2589.0
39.00	923.0
39.90	115.0
44.10	294.0
45.10	532.0
46.00	58.0
47.00	454.0
48.00	303.0
49.10	2601.0
50.10	10721.0
51.10	3024.0
52.20	165.0
55.00	271.0
56.00	896.0
57.10	1571.0
59.00	88.0
60.10	604.0
61.10	3043.0
62.10	3162.0
63.10	1939.0
64.00	204.0
67.10	175.0
68.00	5687.0
69.10	6070.0
70.00	561.0
72.10	243.0
73.10	2891.0
74.10	9856.0
75.10	31552.0
76.10	2540.0
77.00	511.0
77.90	156.0
79.00	1723.0
80.10	405.0
81.00	1648.0
81.90	256.0
85.80	78.0
87.10	2278.0
88.00	2376.0
88.80	116.0
91.00	277.0
92.10	1587.0
93.00	2504.0
94.10	6601.0
95.10	61640.0
96.00	4247.0
97.20	191.0
102.80	129.0
104.00	317.0
105.10	135.0
106.00	314.0
110.90	61.0
112.10	59.0
114.90	101.0
116.00	180.0
117.00	403.0
118.00	342.0
118.90	446.0
121.00	63.0
123.90	60.0
125.20	200.0
127.90	249.0
129.00	103.0
129.90	200.0
130.80	79.0
132.30	55.0
133.00	1004.0
133.90	219.0
134.90	222.0
137.10	129.0
140.90	617.0
143.00	618.0
146.90	138.0
148.00	160.0
148.90	94.0
153.00	52.0
155.00	122.0
157.00	92.0
159.00	75.0
160.90	109.0
163.10	219.0
164.90	114.0
170.60	78.0
172.30	184.0
174.00	39760.0
175.10	3617.0
176.00	36904.0
177.00	2556.0
178.00	134.0
179.10	187.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

189.30	73.0
191.10	709.0
192.10	227.0
193.00	966.0
194.10	122.0
194.90	136.0
203.20	107.0
204.90	198.0
207.10	521.0
208.10	119.0
235.20	53.0
249.00	466.0
250.00	96.0
251.00	164.0
265.10	592.0
266.10	192.0
267.10	113.0
279.20	94.0
281.10	6012.0
282.10	1777.0
283.10	905.0
284.20	297.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

m/z	Abundance
36.00	569.0
37.10	3321.0
38.10	2649.0
39.10	1124.0
40.00	112.0
43.00	52.0
44.10	454.0
45.10	529.0
46.10	75.0
47.10	770.0
48.00	515.0
49.10	2854.0
50.10	13799.0
51.10	3308.0
52.10	121.0
55.00	210.0
56.10	1030.0
57.10	1810.0
59.00	141.0
60.00	664.0
61.10	3398.0
62.00	3411.0
63.10	2228.0
64.20	165.0
66.90	219.0
68.00	7349.0
69.10	6445.0
70.10	598.0
72.00	437.0
73.10	3586.0
74.10	11958.0
75.10	36800.0
76.10	2922.0
77.00	375.0
77.90	286.0
78.90	1980.0
80.00	526.0
81.00	2139.0
82.00	359.0
83.10	54.0
86.00	91.0
87.00	2875.0
88.00	2243.0
91.00	304.0
92.00	1871.0
93.10	3036.0
94.10	9076.0
95.10	74920.0
96.10	4609.0
97.10	147.0
103.10	181.0
103.90	321.0
104.90	117.0
106.00	261.0
110.90	103.0
111.90	52.0
113.00	88.0
115.10	92.0
116.00	223.0
116.90	486.0
118.00	368.0
118.90	433.0
123.90	84.0
124.80	186.0
125.70	81.0
127.90	360.0
129.00	150.0
129.90	199.0
130.90	133.0
133.20	595.0
133.90	154.0
134.80	197.0
136.90	120.0
141.00	668.0
142.20	78.0
143.00	726.0
146.20	61.0
146.90	206.0
148.10	191.0
148.90	57.0
149.90	53.0
155.10	132.0
157.10	143.0
159.00	120.0
161.00	152.0
163.00	105.0
165.10	132.0
170.80	99.0
171.90	258.0
174.00	46856.0
175.10	4050.0
176.00	47952.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

177.00	3218.0
178.00	112.0
178.20	110.0
178.90	135.0
191.10	634.0
192.00	125.0
193.00	799.0
194.00	209.0
194.90	92.0
203.10	85.0
204.90	121.0
207.10	451.0
208.20	66.0
249.10	330.0
250.00	96.0
251.20	173.0
265.10	426.0
266.20	124.0
267.00	90.0
279.00	88.0
281.10	5751.0
282.20	1650.0
283.10	975.0
284.10	218.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

m/z	Abundance
36.10	569.0
37.10	2112.0
38.10	2209.0
39.10	676.0
40.10	107.0
44.10	277.0
45.00	424.0
46.10	81.0
47.00	653.0
48.10	379.0
49.10	2204.0
50.10	9126.0
51.10	2787.0
52.00	91.0
52.30	82.0
55.10	185.0
56.00	829.0
57.00	1658.0
58.90	58.0
60.00	530.0
61.10	2786.0
62.00	2796.0
63.10	1785.0
64.00	192.0
67.10	193.0
68.10	5733.0
69.00	5415.0
70.10	495.0
72.00	365.0
73.10	2962.0
74.10	10023.0
75.10	30152.0
76.10	2443.0
77.00	257.0
78.00	254.0
79.00	1589.0
80.00	423.0
81.00	1751.0
81.90	358.0
83.10	56.0
85.80	128.0
87.10	2544.0
88.00	2015.0
88.80	52.0
90.90	219.0
92.10	1701.0
93.00	2493.0
94.10	7470.0
95.10	56616.0
96.10	3535.0
97.10	162.0
102.90	80.0
104.00	209.0
105.10	126.0
105.90	274.0
110.90	61.0
114.90	72.0
115.80	231.0
116.90	504.0
118.00	258.0
119.00	321.0
124.90	78.0
128.00	149.0
129.00	94.0
129.90	229.0
131.10	94.0
133.10	292.0
133.70	59.0
134.10	58.0
134.80	209.0
136.80	105.0
137.10	87.0
141.00	604.0
142.00	80.0
142.90	681.0
145.90	81.0
147.00	106.0
148.00	179.0
149.00	81.0
150.10	54.0
152.90	53.0
154.90	112.0
157.00	79.0
158.90	75.0
161.10	76.0
163.10	147.0
165.10	94.0
169.80	76.0
170.80	106.0
172.10	219.0
174.00	46240.0
175.00	3965.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83

176.00	46120.0
177.00	3317.0
178.00	174.0
178.90	134.0
191.00	343.0
192.30	145.0
193.10	372.0
193.90	111.0
205.10	118.0
207.10	196.0
208.20	52.0
249.00	284.0
251.10	176.0
265.00	382.0
266.10	79.0
267.00	73.0
281.10	4101.0
282.10	1136.0
283.10	653.0
284.00	124.0

Instrument :
MSVOA_W
ClientSampleId :
BFB83