

Data File : VW014263.D
Acq On : 09 Dec 2019 14:32
Operator : SY/VA
Sample : K6172-11
Misc : 5.21G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BW7

Quant Time: Dec 10 07:36:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 10 07:34:10 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1243863	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1091296	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	431989	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	424308	22.53	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	90.12%
7) Chloroethane-d5	2.89	69	320717	22.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.60%
10) 1,1-Dichloroethene-d2	4.23	63	161	0.00	ug/L	0.21
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.00%#
20) 2-Butanone-d5	7.07	46	231798	47.23	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	94.46%
24) Chloroform-d	7.65	84	719400	22.72	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.88%
26) 1,2-Dichloroethane-d4	8.31	65	401470	24.18	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	96.72%
29) Benzene-d6	8.27	84	1530719	23.93	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.72%
33) 1,2-Dichloropropane-d6	9.27	67	476311	24.21	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	96.84%
37) Toluene-d8	10.32	98	1342643	23.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.88%
38) trans-1,3-Dichloropropene-	10.57	79	191704	23.22	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	92.88%
39) 2-Hexanone-d5	10.92	63	174181	44.52	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	89.04%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	366879	22.88	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	91.52%
61) 1,2-Dichlorobenzene-d4	13.85	152	386171	23.39	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	93.56%


Target Compounds						Qvalue
13) Acetone	4.12	43	78332	16.552	ug/L	98
21) 2-Butanone	7.17	43	32242	5.075	ug/L	92
59) 1,2,3-Trichloropropane	13.55	75	49389	4.026	ug/L	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014263.D
Acq On : 09 Dec 2019 14:32
Operator : SY/VA
Sample : K6172-11
Misc : 5.21G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0BW7

Quant Time: Dec 10 07:36:37 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 10 07:34:10 2019
Response via : Initial Calibration

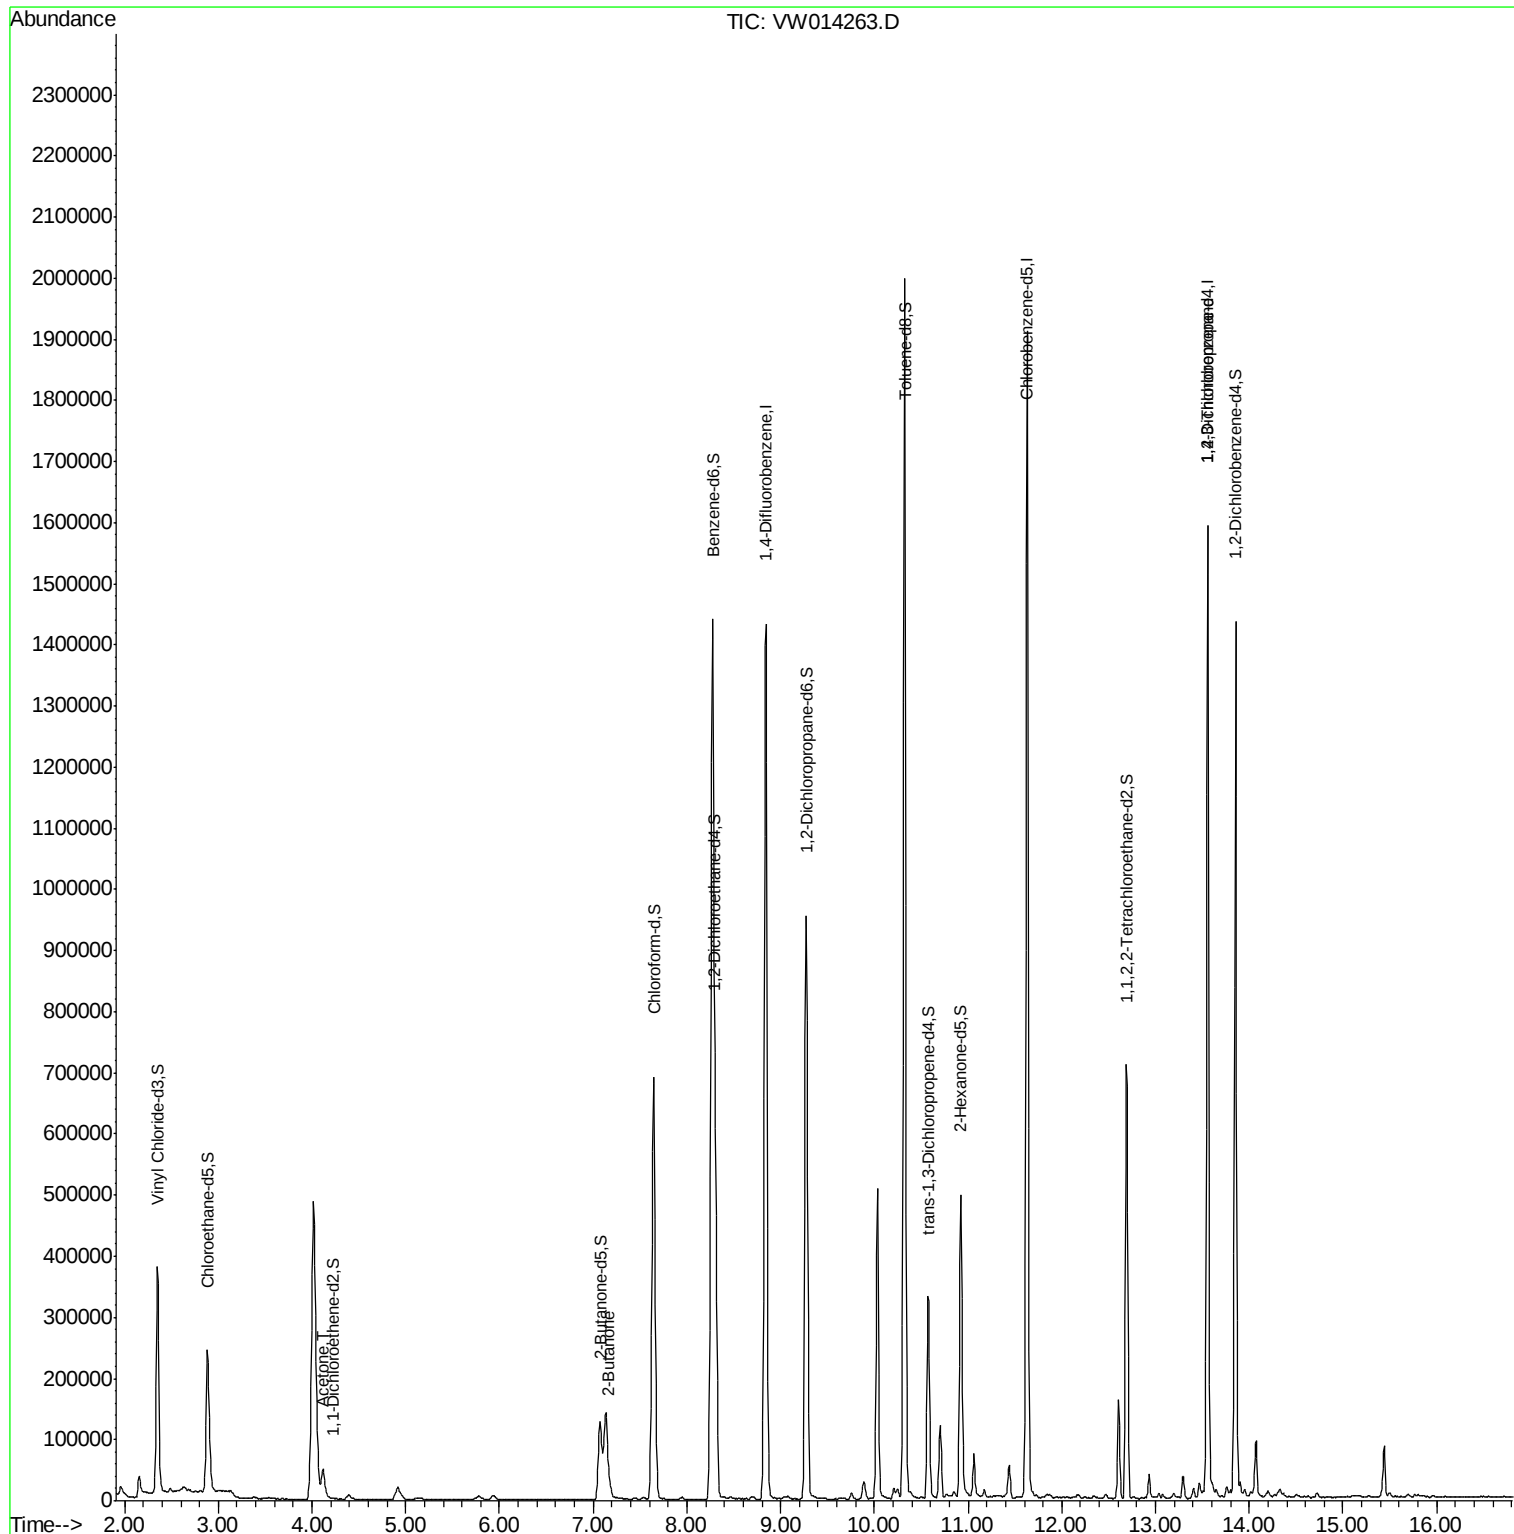

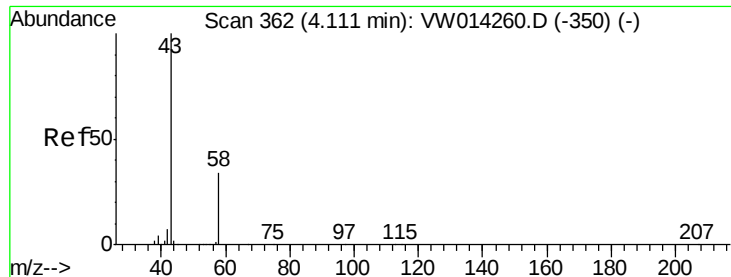

#13

Acetone

Concen: 16.552 ug/L

RT: 4.12 min Scan# 363

Delta R.T. 0.01 min

Lab File: VW014263.D

Acq: 09 Dec 2019 14:32

Instrument :

MSVOA_W

ClientSampleId :





C0BW7

Tgt Ion: 43 Resp: 78332

Ion Ratio Lower Upper

43 100

58 33.7 0.0 65.4

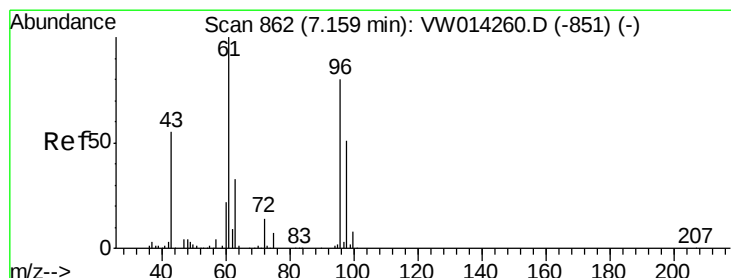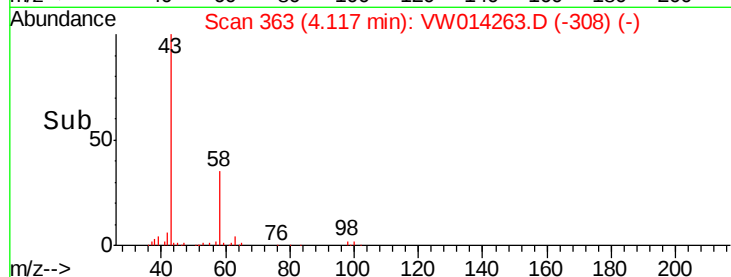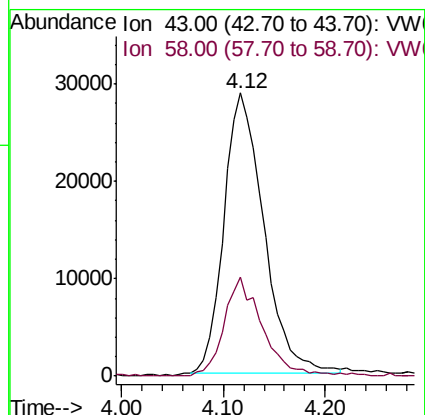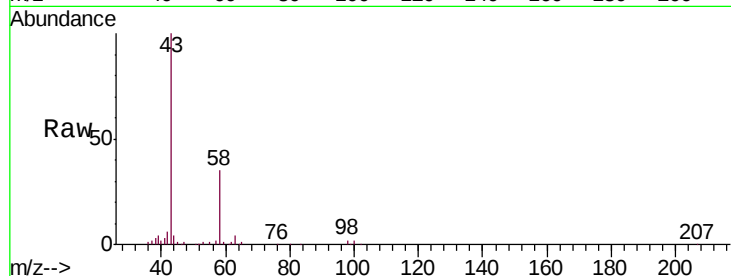

#21

2-Butanone

Concen: 5.075 ug/L

RT: 7.17 min Scan# 863

Delta R.T. 0.01 min

Lab File: VW014263.D




Acq: 09 Dec 2019 14:32


Tgt Ion: 43 Resp: 32242

Ion Ratio Lower Upper

43 100

72 23.7 14.1 42.2

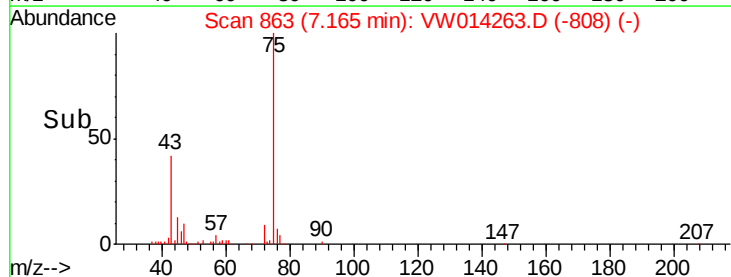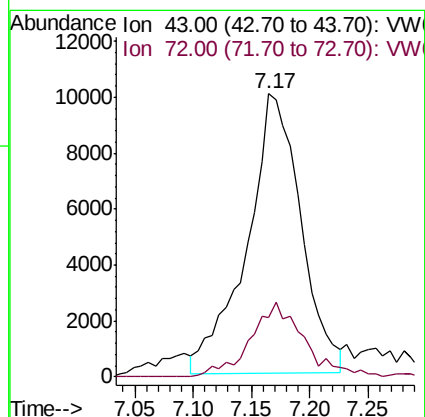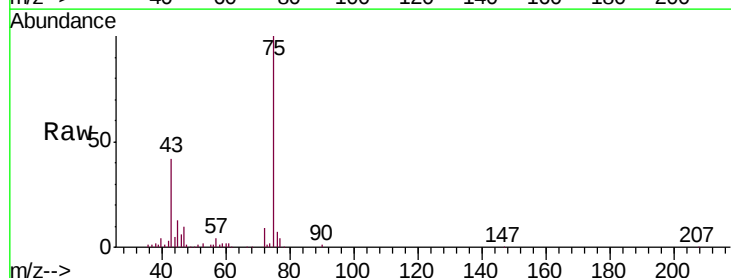

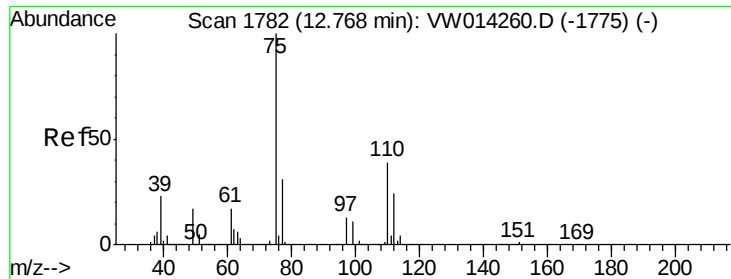

#59

1,2,3-Trichloropropane

Concen: 4.026 ug/L

RT: 13.55 min Scan# 1911

Delta R.T. 0.79 min

Lab File: VW014263.D

Acq: 09 Dec 2019 14:32

Instrument :

MSVOA_W

ClientSampleId :

C0BW7

Tgt Ion: 75 Resp: 49389

Ion Ratio Lower Upper

75 100

77 36.4 25.9 38.9

