

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
 Data File : VW021252.D
 Acq On : 09 Dec 2021 19:47
 Operator : SY/VA
 Sample : M4883-07RE
 Misc : 4.07g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9G3RE

Manual IntegrationsAPPROVED

Quant Time: Dec 10 00:47:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 00:28:10 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/10/2021
 Supervised By :Mahesh Dadoda 12/10/2021

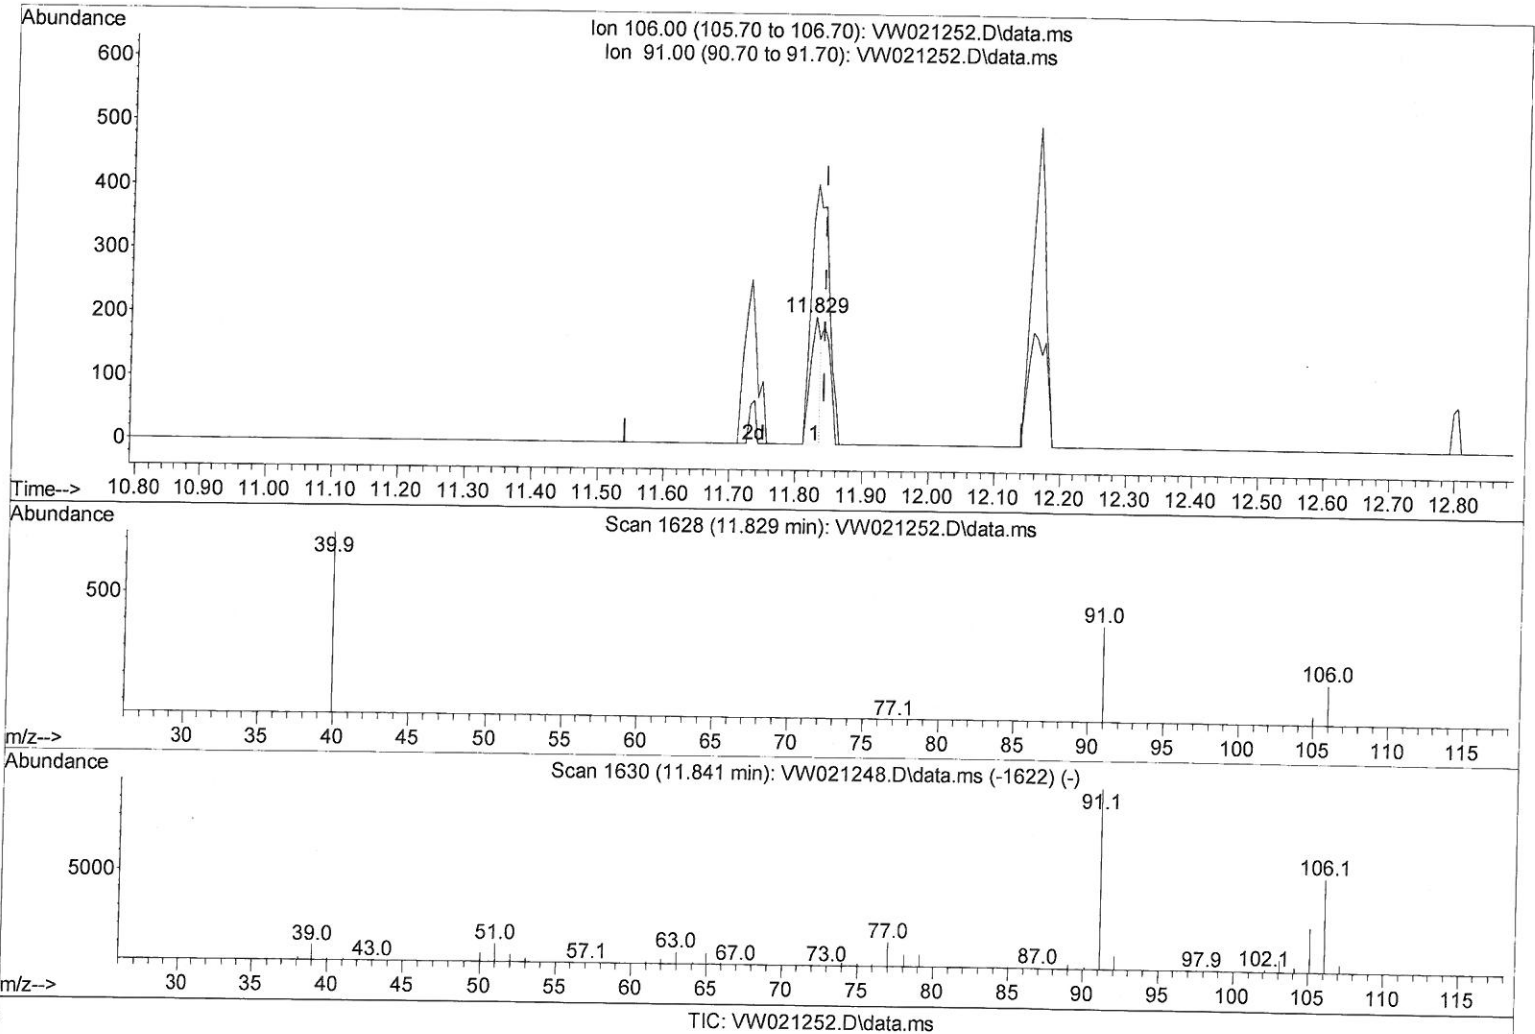

(53) m,p-Xylene (T)

11.829min (-0.012) 1.79 ug/L

response 210

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	214.10	203.50
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
 Data File : VW021252.D
 Acq On : 09 Dec 2021 19:47
 Operator : SY/VA
 Sample : M4883-07RE
 Misc : 4.07g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9G3RE

Manual IntegrationsAPPROVED

Quant Time: Dec 10 00:47:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 00:28:10 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/10/2021
 Supervised By :Mahesh Dadoda 12/10/2021

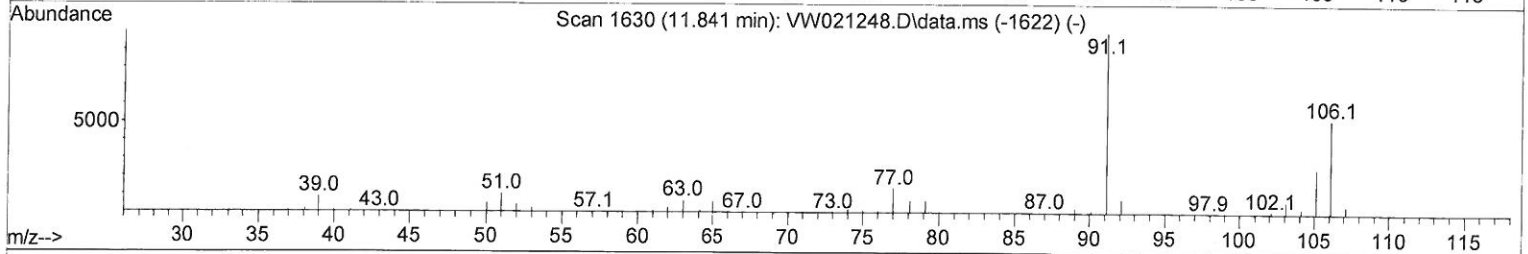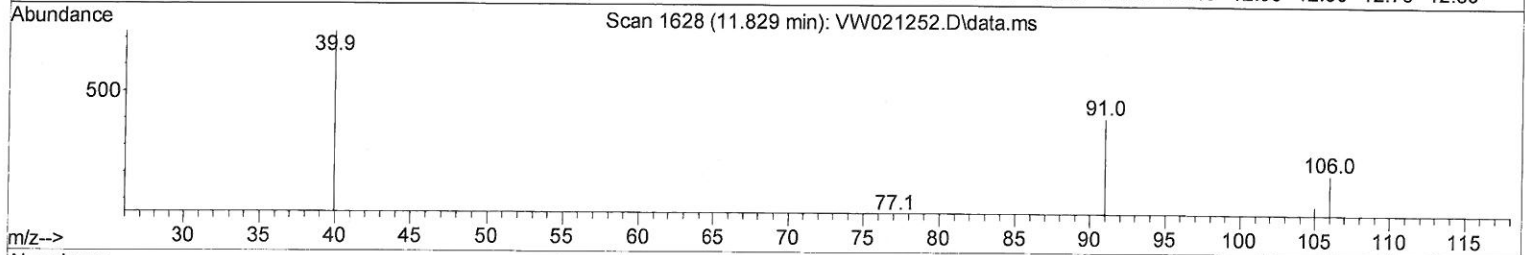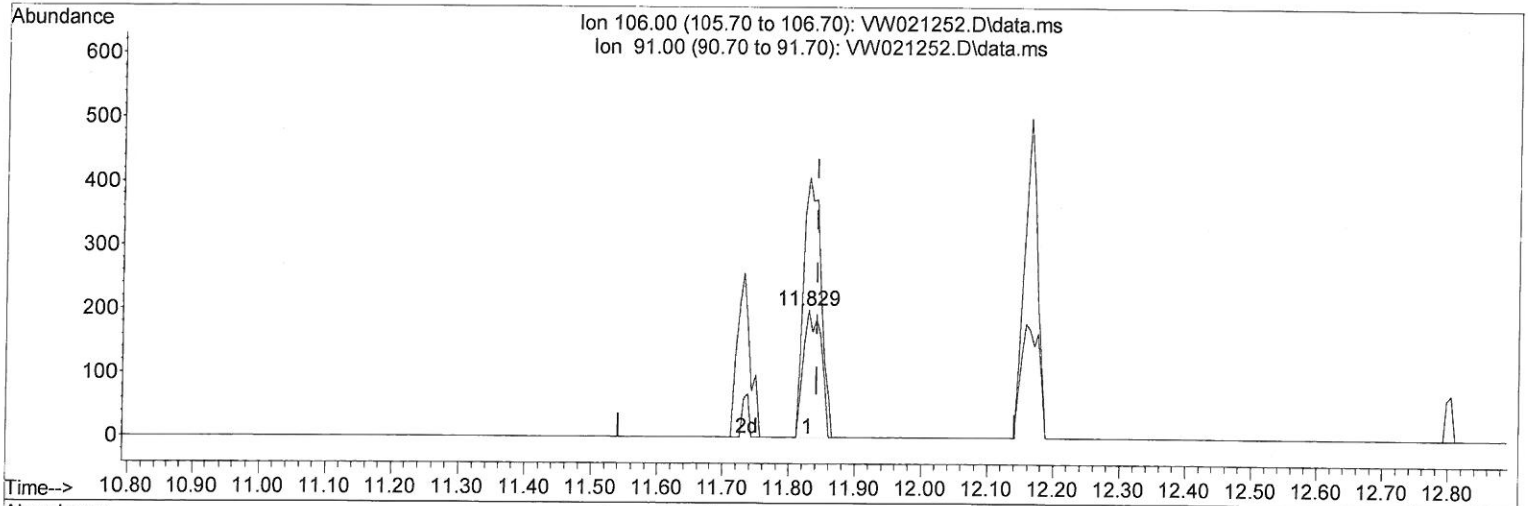

TIC: VW021252.D\data.ms

(53) m,p-Xylene (T)

11.829min (-0.012) 3.17 ug/L m

response 372

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	214.10	203.50
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
 Data File : VW021252.D
 Acq On : 09 Dec 2021 19:47
 Operator : SY/VA
 Sample : M4883-07RE
 Misc : 4.07g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9G3RE

Manual IntegrationsAPPROVED

Quant Time: Dec 10 00:47:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 00:28:10 2021
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/10/2021
 Supervised By :Mahesh Dadoda 12/10/2021

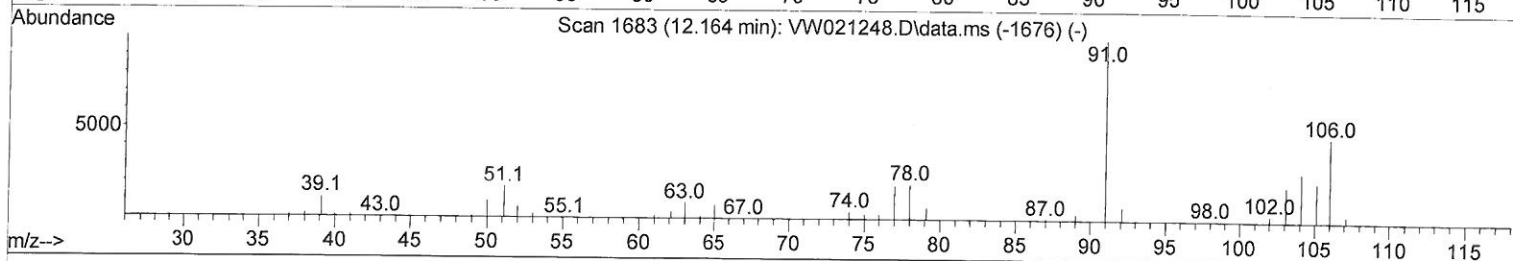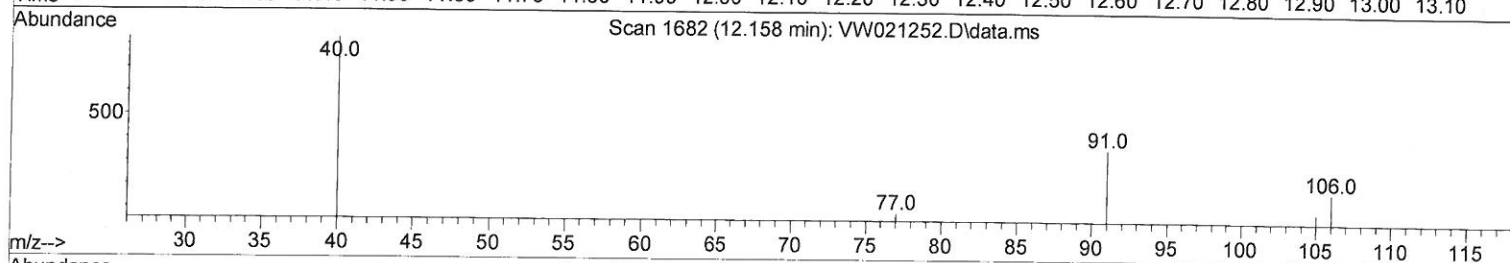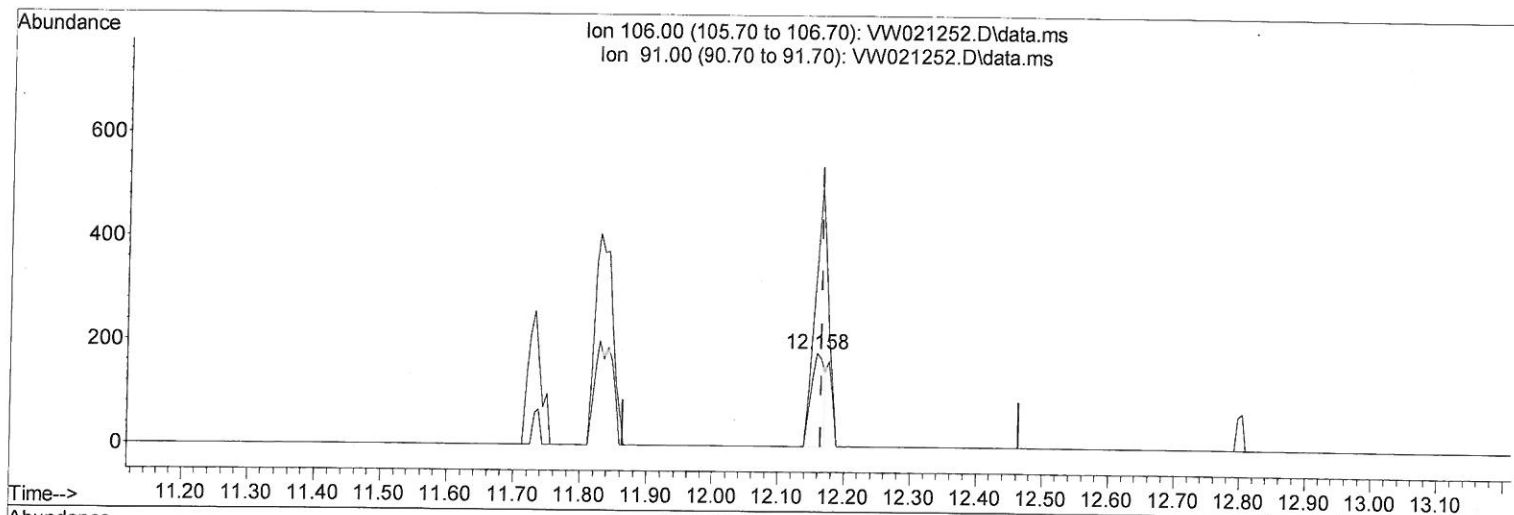

TIC: VW021252.D\data.ms

(54) o-Xylene (T)

12.158min (-0.006) 2.29 ug/L

response 255

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	219.50	201.11
0.00	0.00	0.00
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
Data File : VW021252.D
Acq On : 09 Dec 2021 19:47
Operator : SY/VA
Sample : M4883-07RE
Misc : 4.07g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW9G3RE

Manual IntegrationsAPPROVED

Quant Time: Dec 10 00:47:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 00:28:10 2021
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/10/2021
Supervised By :Mahesh Dadoda 12/10/2021

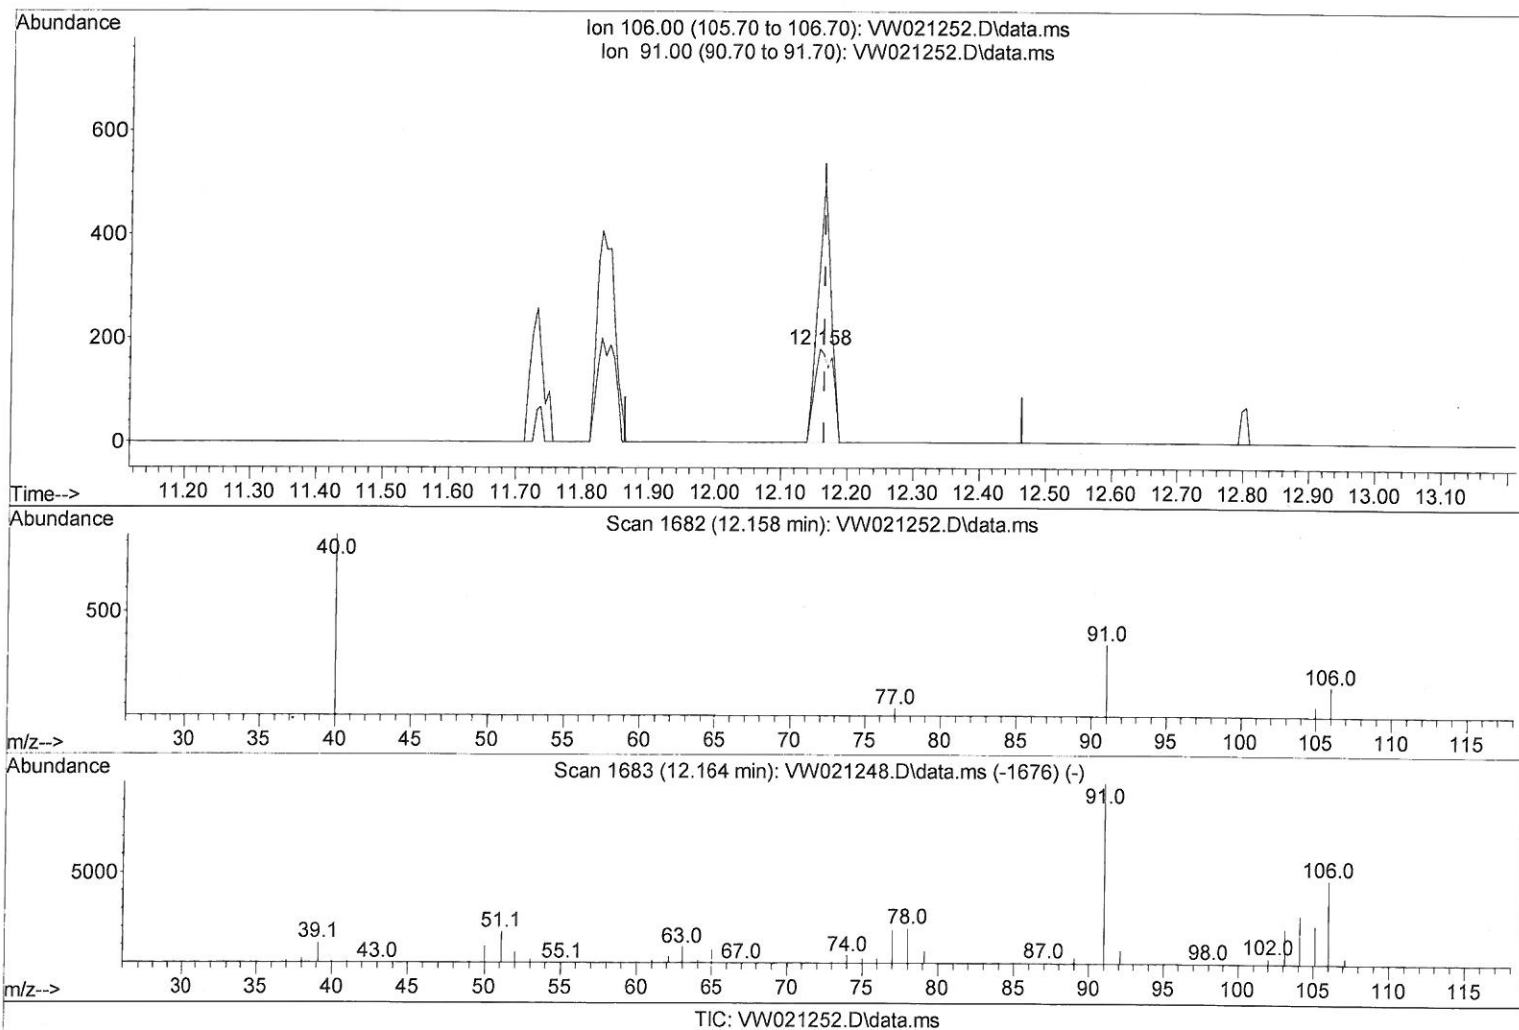

(54) o-Xylene (T)

12.158min (-0.006) 3.08 ug/L m

response 343

Ion	Exp%	Act%
106.00	100.00	100.00
91.00	219.50	201.11
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
 Data File : VW021252.D
 Acq On : 09 Dec 2021 19:47
 Operator : SY/VA
 Sample : M4883-07RE
 Misc : 4.07g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 EW9G3RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/10/2021
 Supervised By :Mahesh Dadoda 12/10/2021

Quant Time: Dec 10 00:47:03 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 00:28:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	9098	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	3996	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	875	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	4950	29.874	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	= 119.480%		
7) Chloroethane-d5	2.885	69	4974	45.408	ug/L	0.00
Spiked Amount	25.000	Range 30 - 150	Recovery	= 181.640%#		
11) 1,1-Dichloroethene-d2	4.019	63	5003	22.648	ug/L	0.00
Spiked Amount	25.000	Range 45 - 110	Recovery	= 90.600%		
21) 2-Butanone-d5	7.086	46	2039	87.298	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	= 174.600%#		
24) Chloroform-d	7.653	84	7753	30.579	ug/L	0.00
Spiked Amount	25.000	Range 40 - 150	Recovery	= 122.320%		
26) 1,2-Dichloroethane-d4	8.305	65	4292	31.824	ug/L	0.00
Spiked Amount	25.000	Range 70 - 130	Recovery	= 127.280%		
32) Benzene-d6	8.281	84	13449	61.401	ug/L	0.00
Spiked Amount	25.000	Range 20 - 135	Recovery	= 245.600%#		
36) 1,2-Dichloropropane-d6	9.274	67	4251	72.367	ug/L	0.00
Spiked Amount	25.000	Range 70 - 120	Recovery	= 289.480%#		
41) Toluene-d8	10.329	98	8273	36.967	ug/L	0.00
Spiked Amount	25.000	Range 30 - 130	Recovery	= 147.880%#		
43) trans-1,3-Dichloroprop...	10.579	79	613	22.664	ug/L	0.00
Spiked Amount	25.000	Range 30 - 135	Recovery	= 90.640%		
47) 2-Hexanone-d5	10.927	63	933	107.409	ug/L	0.00
Spiked Amount	50.000	Range 20 - 135	Recovery	= 214.820%#		
56) 1,1,2,2-Tetrachloroeth...	12.688	84	1918	37.982	ug/L	0.00
Spiked Amount	25.000	Range 45 - 120	Recovery	= 151.920%#		
66) 1,2-Dichlorobenzene-d4	13.853	152	742	21.881	ug/L	0.00
Spiked Amount	25.000	Range 75 - 120	Recovery	= 87.520%		
Target Compounds						
16) Methylene chloride	4.909	84	975	6.486	ug/L	# 63
34) Trichloroethene	9.091	95	27487	449.819	ug/L	93
35) Methylcyclohexane	9.335	83	212	2.103	ug/L	# 83
42) Toluene	10.390	91	2030	7.974	ug/L	86
46) Tetrachloroethene	10.866	164	218	3.755	ug/L	80
52) Ethylbenzene	11.731	91	345	1.186	ug/L	87
53) m,p-Xylene	11.829	106	372m	3.170	ug/L	
54) o-Xylene	12.158	106	343m	3.079	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
Data File : VW021252.D
Acq On : 09 Dec 2021 19:47
Operator : SY/VA
Sample : M4883-07RE
Misc : 4.07g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
EW9G3RE

Manual IntegrationsAPPROVED

Quant Time: Dec 10 00:47:03 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 00:28:10 2021
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/10/2021
Supervised By :Mahesh Dadoda 12/10/2021

