

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
 Data File : VW021253.D
 Acq On : 09 Dec 2021 20:11
 Operator : SY/VA
 Sample : VIBLK520
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK520

Quant Time: Dec 10 00:33:07 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 00:28:10 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	96516	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	94614	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.560	152	50606	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.355	65	44200	25.145	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.560%
7) Chloroethane-d5	2.885	69	28464	24.495	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	97.960%
11) 1,1-Dichloroethene-d2	4.013	63	42104	17.966	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.880%
21) 2-Butanone-d5	7.080	46	12703	51.267	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.540%
24) Chloroform-d	7.653	84	59285	22.042	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	88.160%
26) 1,2-Dichloroethane-d4	8.305	65	33311	23.283	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.120%
32) Benzene-d6	8.274	84	118060	22.765	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.040%
36) 1,2-Dichloropropane-d6	9.274	67	31857	22.905	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	91.600%
41) Toluene-d8	10.323	98	116859	22.054	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.200%
43) trans-1,3-Dichloroprop...	10.579	79	13646	21.308	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.240%
47) 2-Hexanone-d5	10.920	63	10394	50.537	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.080%
56) 1,1,2,2-Tetrachloroeth...	12.688	84	26992	22.575	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.320%
66) 1,2-Dichlorobenzene-d4	13.853	152	45052	22.971	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.880%
Target Compounds						Qvalue
16) Methylene chloride	4.915	84	6470	4.057	ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
Data File : VW021253.D
Acq On : 09 Dec 2021 20:11
Operator : SY/VA
Sample : VIBLK520
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK520


Quant Time: Dec 10 00:33:07 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 00:28:10 2021
Response via : Initial Calibration

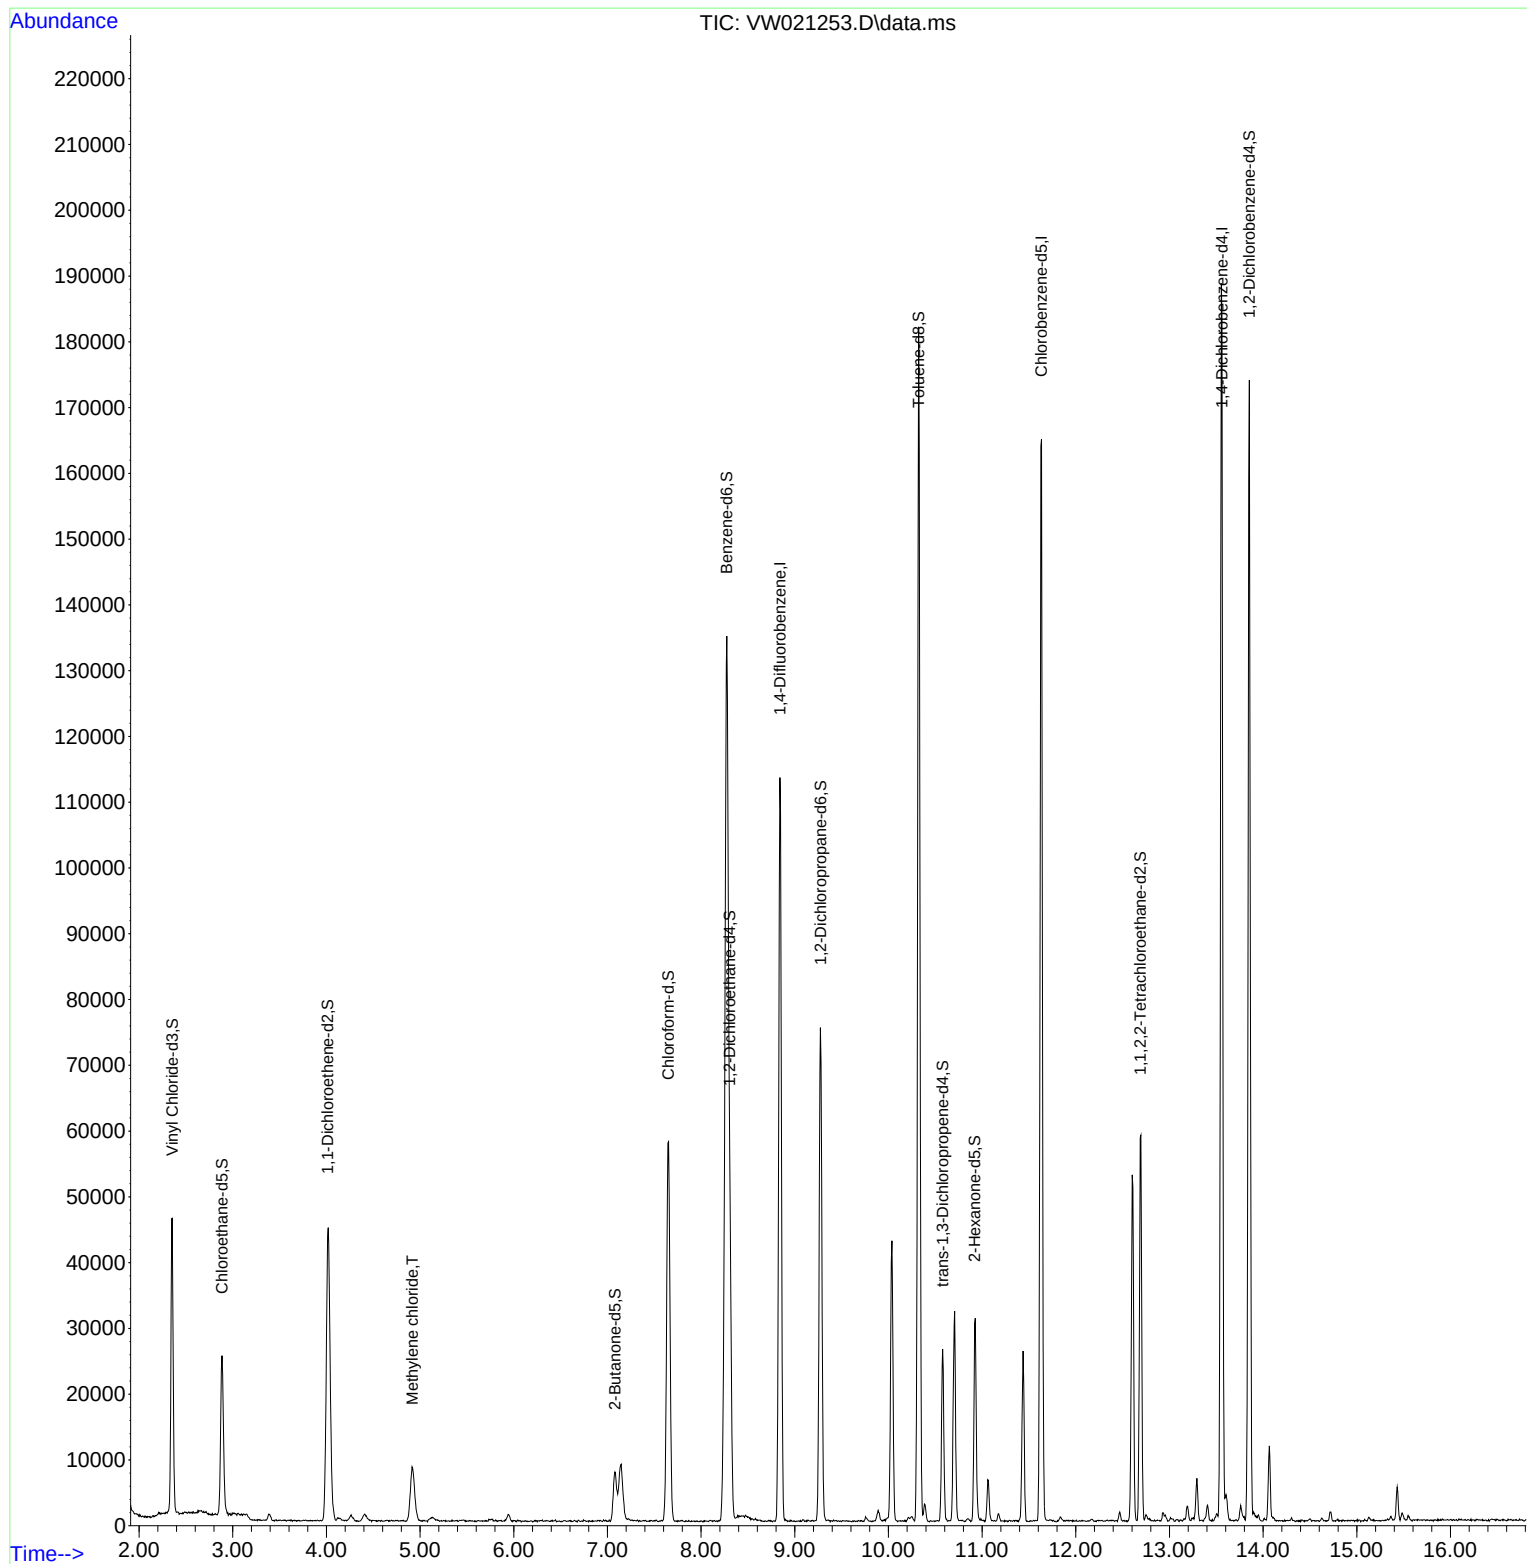

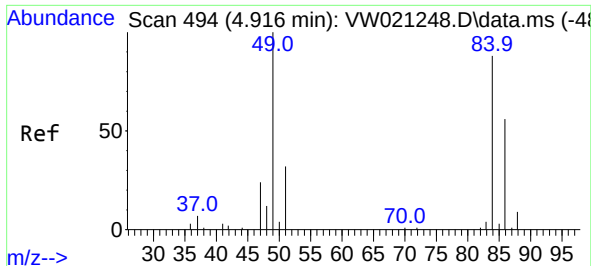

#16
Methylene chloride
Concen: 4.057 ug/L
RT: 4.915 min Scan# 49
Delta R.T. -0.000 min
Lab File: VW021253.D
Acq: 09 Dec 2021 20:11

Instrument :
MSVOA_W
ClientSampleId :
VIBLK520

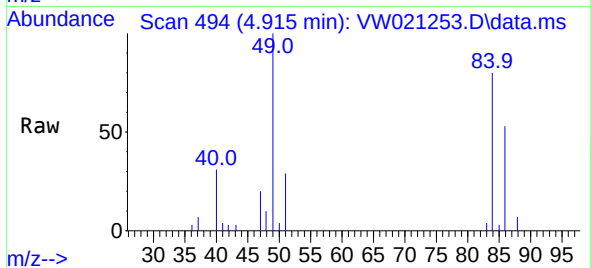

Tgt Ion: 84 Resp: 6470

Ion	Ratio	Lower	Upper
84	100		
86	65.8	45.5	84.5
49	124.7	100.5	186.7

