
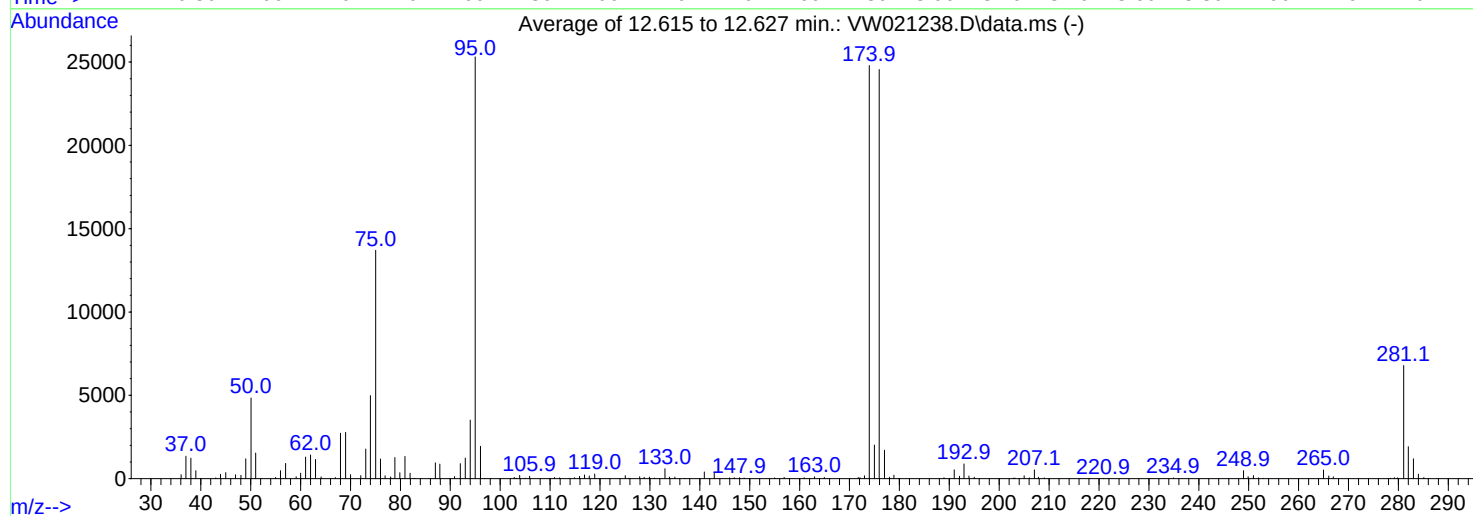


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120921\
 Data File : VW021238.D
 Acq On : 09 Dec 2021 07:44
 Operator : SY/VA
 Sample : BFB475
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB475

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Title : SFAM01.0
 Last Update : Fri Dec 10 00:28:10 2021

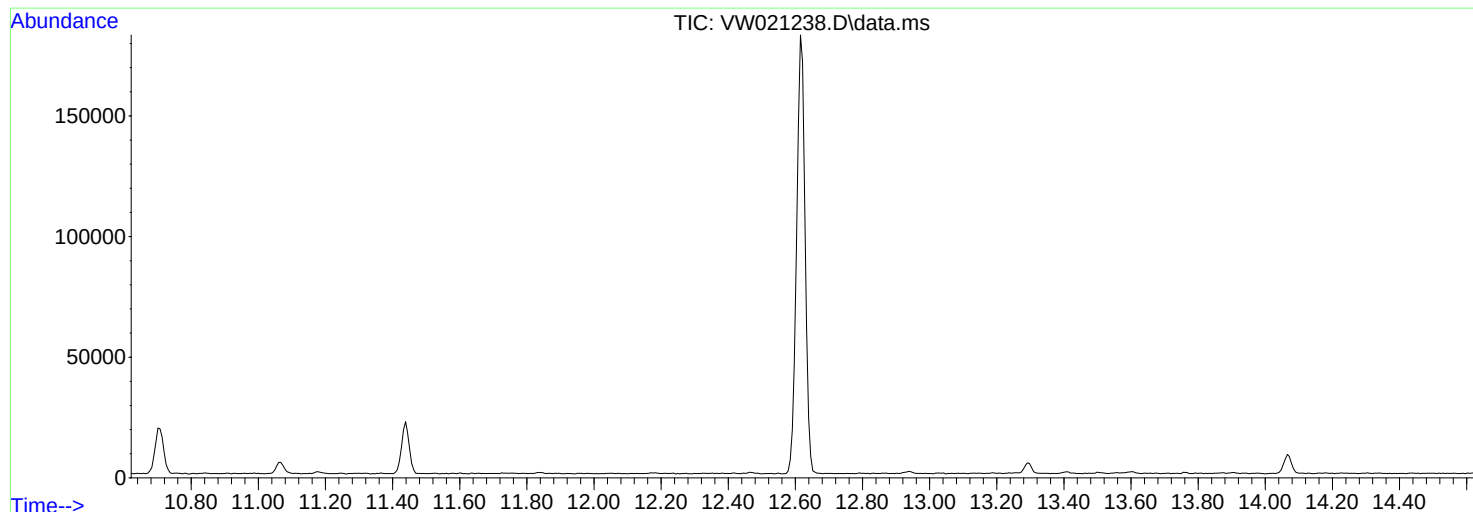

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	4842	PASS
75	95	30	80	54.1	13699	PASS
95	95	100	100	100.0	25312	PASS
96	95	5	9	7.6	1936	PASS
173	174	0.00	2	0.7	173	PASS
174	95	50	120	98.0	24795	PASS
175	174	5	9	8.1	2015	PASS
176	174	95	105	99.0	24557	PASS
177	176	5	10	7.0	1710	PASS

m/z	Abundance
36.00	321.0
37.00	1473.0
38.00	1447.0
39.00	567.0
40.00	1857.0
43.00	81.0
44.00	286.0
45.00	355.0
47.00	229.0
48.10	193.0
49.00	1262.0
50.00	5259.0
51.00	1677.0
55.00	131.0
55.90	544.0
57.00	940.0
59.10	108.0
60.00	369.0
61.00	1415.0
62.00	1480.0
63.00	1230.0
64.10	97.0
66.90	68.0
68.00	2948.0
69.00	3042.0
70.00	235.0
72.00	225.0
73.10	1838.0
74.00	5449.0
75.10	15694.0
76.00	1309.0
77.00	235.0
78.00	146.0
78.90	1522.0
79.90	362.0
80.90	1406.0
81.90	342.0
87.00	991.0
87.90	989.0
90.90	155.0
92.00	1017.0
93.00	1417.0
94.00	4088.0
95.00	28400.0
96.00	2118.0
103.20	99.0
103.90	206.0
105.90	181.0
110.90	76.0
111.90	78.0
114.90	108.0
115.90	163.0
116.90	237.0
117.80	159.0
119.00	322.0
125.00	185.0
127.90	115.0
128.90	105.0
129.90	120.0
130.80	55.0
133.00	531.0
135.00	95.0
140.90	572.0
142.90	450.0
146.00	69.0
146.90	71.0
147.90	84.0
155.00	75.0
156.80	75.0
160.90	58.0
162.90	69.0
164.90	69.0
171.70	88.0
173.00	518.0
174.00	26184.0
175.00	2423.0
175.90	28896.0
177.00	1763.0
178.00	97.0
178.90	141.0
189.00	73.0
191.00	382.0
192.00	127.0
193.00	896.0
193.80	159.0
195.00	103.0
203.10	71.0
205.00	168.0
206.10	56.0
207.00	453.0
207.80	84.0
208.90	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB475

249.00	402.0
249.90	101.0
250.90	156.0
252.00	55.0
265.00	367.0
266.00	126.0
267.00	95.0
279.80	141.0
281.00	5511.0
282.00	1731.0
283.00	752.0
284.00	228.0
285.10	107.0

Instrument :
MSVOA_W
ClientSampleId :
BFB475

m/z	Abundance
36.10	193.0
37.00	937.0
38.00	914.0
39.00	365.0
40.00	1864.0
43.90	228.0
45.00	264.0
47.00	213.0
48.10	162.0
49.00	757.0
50.00	3616.0
51.00	1279.0
56.00	409.0
57.00	736.0
59.00	52.0
59.90	239.0
61.00	954.0
62.00	1161.0
63.00	951.0
64.10	76.0
67.00	62.0
68.00	2111.0
69.00	2146.0
70.00	193.0
72.10	146.0
73.00	1191.0
74.00	3949.0
75.00	10095.0
76.00	911.0
76.90	158.0
78.10	67.0
78.90	847.0
79.90	252.0
80.90	1195.0
81.90	277.0
87.00	794.0
87.90	713.0
90.90	115.0
92.10	669.0
93.00	888.0
94.00	2728.0
95.00	20368.0
96.10	1469.0
104.00	133.0
105.90	122.0
116.00	73.0
116.80	166.0
117.90	104.0
118.90	229.0
125.10	121.0
128.00	116.0
128.80	55.0
129.90	63.0
133.00	218.0
133.90	76.0
135.00	69.0
140.90	236.0
143.00	262.0
155.00	82.0
157.00	60.0
163.00	51.0
171.80	108.0
173.90	21584.0
175.00	1631.0
175.90	19792.0
177.00	1529.0
178.00	74.0
179.00	65.0
191.00	204.0
191.90	65.0
193.00	332.0
193.80	54.0
203.20	58.0
205.10	92.0
207.00	86.0
249.00	199.0
249.90	50.0
250.90	90.0
264.90	224.0
265.90	60.0
267.00	85.0
281.10	3292.0
282.00	797.0
283.00	460.0
283.90	140.0

Instrument :
MSVOA_W
ClientSampleId :
BFB475

m/z	Abundance
40.00	1791.0

Instrument :
MSVOA_W
ClientSampleId :
BFB475

m/z	Abundance
36.00	195.0
37.00	1609.0
38.00	1338.0
39.00	512.0
40.00	1711.0
43.00	62.0
44.00	264.0
45.00	486.0
46.90	257.0
48.00	242.0
49.00	1546.0
50.10	5652.0
51.00	1657.0
52.10	53.0
55.00	98.0
56.00	502.0
57.00	1047.0
59.10	201.0
60.00	380.0
61.00	1524.0
62.00	1636.0
63.00	1263.0
64.10	154.0
67.00	65.0
68.00	3134.0
69.00	3149.0
70.00	287.0
72.10	168.0
73.00	2310.0
74.00	5549.0
75.00	15309.0
76.00	1321.0
77.00	132.0
78.10	101.0
78.90	1430.0
79.90	452.0
80.90	1407.0
82.00	347.0
82.90	55.0
87.00	1073.0
87.90	930.0
90.80	117.0
92.00	1026.0
93.00	1408.0
94.00	3741.0
95.00	27168.0
96.00	2222.0
96.90	60.0
102.80	222.0
103.90	243.0
105.00	79.0
105.90	134.0
109.80	66.0
110.90	119.0
111.90	68.0
114.90	74.0
115.90	175.0
117.00	255.0
117.90	229.0
119.00	276.0
125.10	255.0
125.80	77.0
127.90	108.0
128.80	80.0
129.90	120.0
131.00	67.0
133.00	1030.0
133.90	207.0
135.00	130.0
137.00	58.0
140.90	411.0
142.90	407.0
145.90	64.0
146.90	113.0
148.00	103.0
148.90	104.0
149.90	52.0
156.90	87.0
160.90	107.0
163.00	240.0
165.00	155.0
172.10	169.0
173.90	26616.0
175.00	1990.0
176.00	24984.0
177.00	1838.0
178.00	89.0
178.90	433.0
179.90	66.0
188.90	104.0
190.10	68.0
191.00	985.0

Instrument :
MSVOA_W
ClientSampleId :
BFB475

192.10	236.0
192.90	1425.0
194.00	286.0
195.00	159.0
202.90	96.0
205.00	261.0
206.00	91.0
207.10	1036.0
207.90	166.0
209.10	98.0
220.90	57.0
234.90	145.0
248.90	840.0
249.90	203.0
251.00	299.0
251.90	91.0
252.90	63.0
265.00	957.0
266.10	297.0
266.90	154.0
278.40	91.0
279.20	165.0
281.10	11565.0
282.00	3239.0
283.00	2361.0
284.10	432.0
285.10	105.0

Instrument :
MSVOA_W
ClientSampleId :
BFB475