




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120924\
 Data File : VW031169.D
 Acq On : 09 Dec 2024 18:15
 Operator : SY/MD
 Sample : P5153-02
 Misc : 6.54g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28P0

Manual IntegrationsAPPROVED

Quant Time: Dec 10 01:15:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 10 01:12:15 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/17/2024
 Supervised By :Mahesh Dadoda 12/17/2024

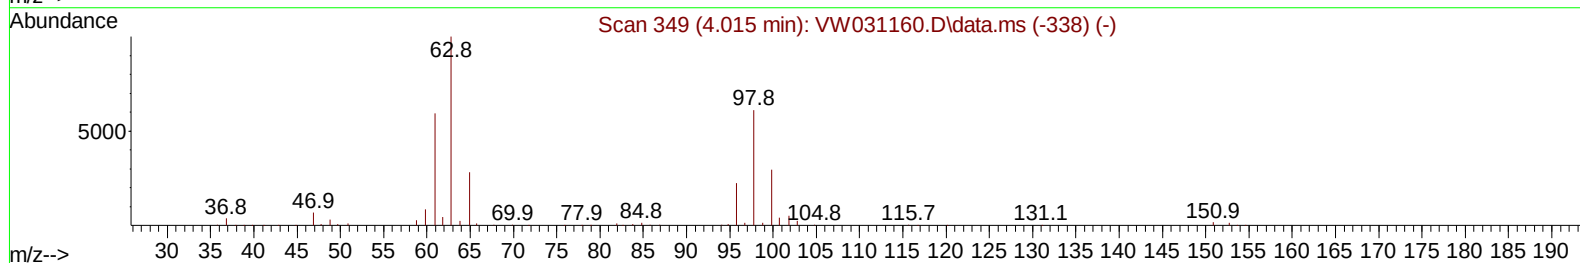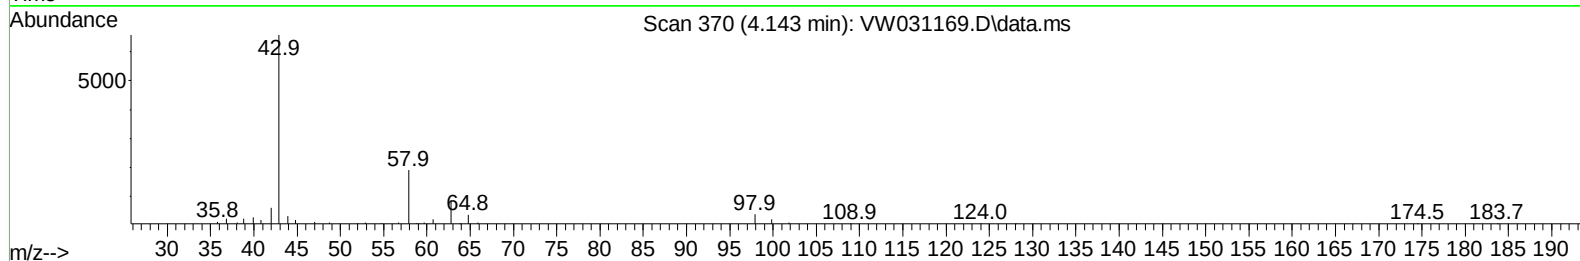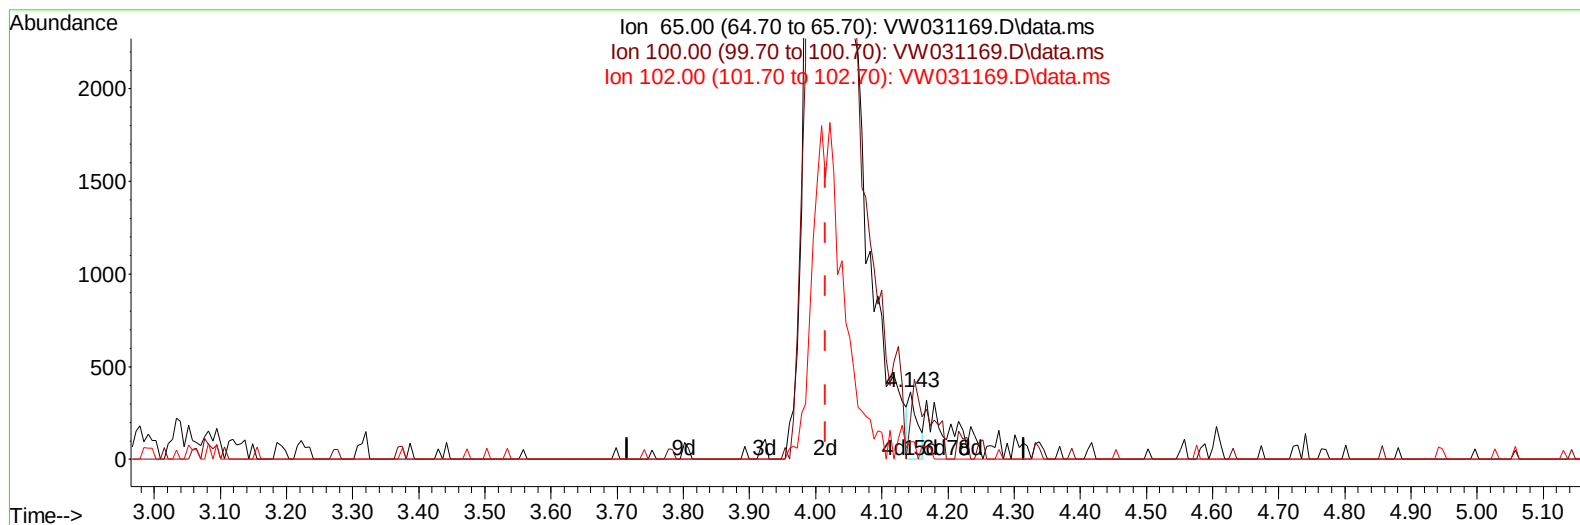

TIC: VW031169.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.143min (+ 0.128) 0.12 ug/L

response 342

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.20	177.49
102.00	21.00	20.47
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120924\
Data File : VW031169.D
Acq On : 09 Dec 2024 18:15
Operator : SY/MD
Sample : P5153-02
Misc : 6.54g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28P0

Manual IntegrationsAPPROVED

Quant Time: Dec 10 01:15:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 10 01:12:15 2024
Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/17/2024
Supervised By :Mahesh Dadoda 12/17/2024

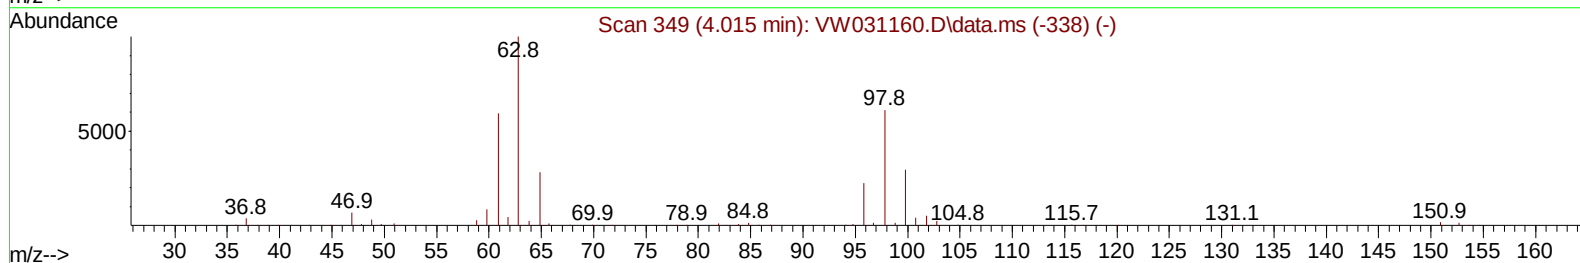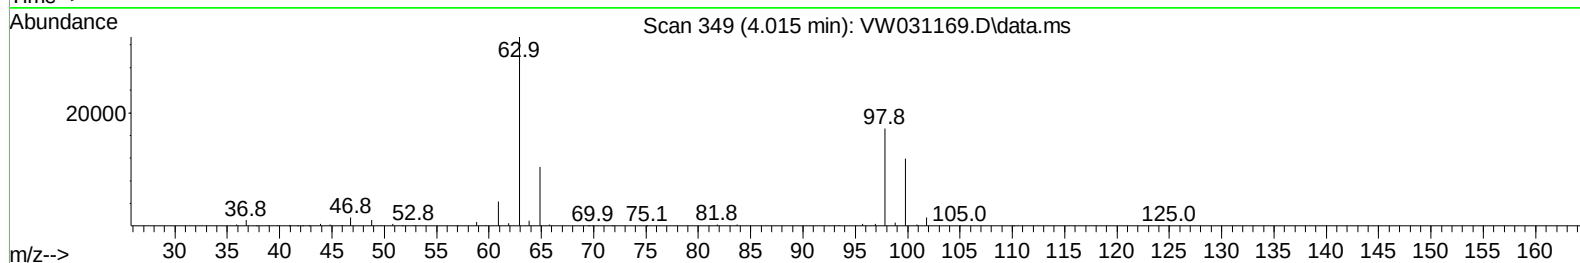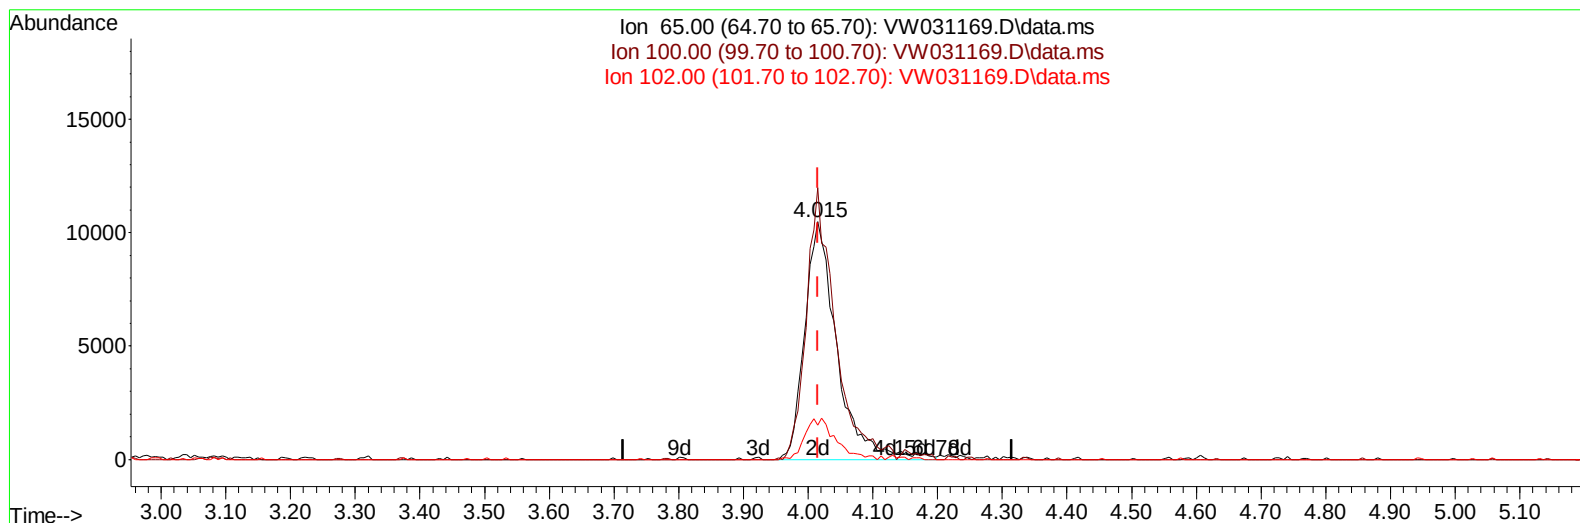

TIC: VW031169.D\data.ms

(11) 1,1-Dichloroethene-d2 (S)

4.015min (+ 0.000) 12.79 ug/L m

response 36231

Ion	Exp%	Act%
65.00	100.00	100.00
100.00	143.20	1.68#
102.00	21.00	0.19#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw120924\
 Data File : VW031169.D
 Acq On : 09 Dec 2024 18:15
 Operator : SY/MD
 Sample : P5153-02
 Misc : 6.54g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28P0

Manual IntegrationsAPPROVED

Quant Time: Dec 10 01:15:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
 Quant Title : SFAM01.0
 QLast Update : Tue Dec 10 01:12:15 2024
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/17/2024
 Supervised By :Mahesh Dadoda 12/17/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	403603	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.629	117	353993	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	114479	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	73462	11.828	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	47.320%	
7) Chloroethane-d5	2.899	69	66346	13.768	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	55.080%	
11) 1,1-Dichloroethene-d2	4.015	65	36231m	12.786	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	51.160%	
21) 2-Butanone-d5	7.100	46	45057	41.480	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	82.960%	
24) Chloroform-d	7.648	84	196459	16.619	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	66.480%	
26) 1,2-Dichloroethane-d4	8.301	65	107321	18.450	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	73.800%	
32) Benzene-d6	8.270	84	320605	14.736	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	58.960%	
36) 1,2-Dichloropropane-d6	9.270	67	114595	17.981	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	71.920%	
41) Toluene-d8	10.319	98	263505	13.420	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	53.680%	
43) trans-1,3-Dichloroprop...	10.575	79	43346	16.894	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	67.560%	
47) 2-Hexanone-d5	10.922	63	32258	43.202	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	86.400%	
56) 1,1,2,2-Tetrachloroeth...	12.684	84	81447	18.936	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	75.760%	
66) 1,2-Dichlorobenzene-d4	13.849	152	62475	15.365	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	61.440%#	
Target Compounds						
13) Acetone	4.167	43	52299	26.743	ug/L	Qvalue 90

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW120924\
Data File : VW031169.D
Acq On : 09 Dec 2024 18:15
Operator : SY/MD
Sample : P5153-02
Misc : 6.54g/10mL/MSVOA_W/SOIL/A
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28P0

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/17/2024
Supervised By :Mahesh Dadoda 12/17/2024

Quant Time: Dec 10 01:15:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120424SMA.M
Quant Title : SFAM01.0
QLast Update : Tue Dec 10 01:12:15 2024
Response via : Initial Calibration

