

Quantitation Report (Qedit)


Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121019\
 Data File : VW014276.D
 Acq On : 10 Dec 2019 12:04
 Operator : SY/VA
 Sample : VW1210SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampleId :
 VBLK07

Manual Integrations
APPROVED

MMDadoda
 12/11/2019 12:55:11 PM

Ouant Time: Dec 11 04:10:47 2019
 Ouant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 04:05:19 2019
 Response via : Initial Calibration

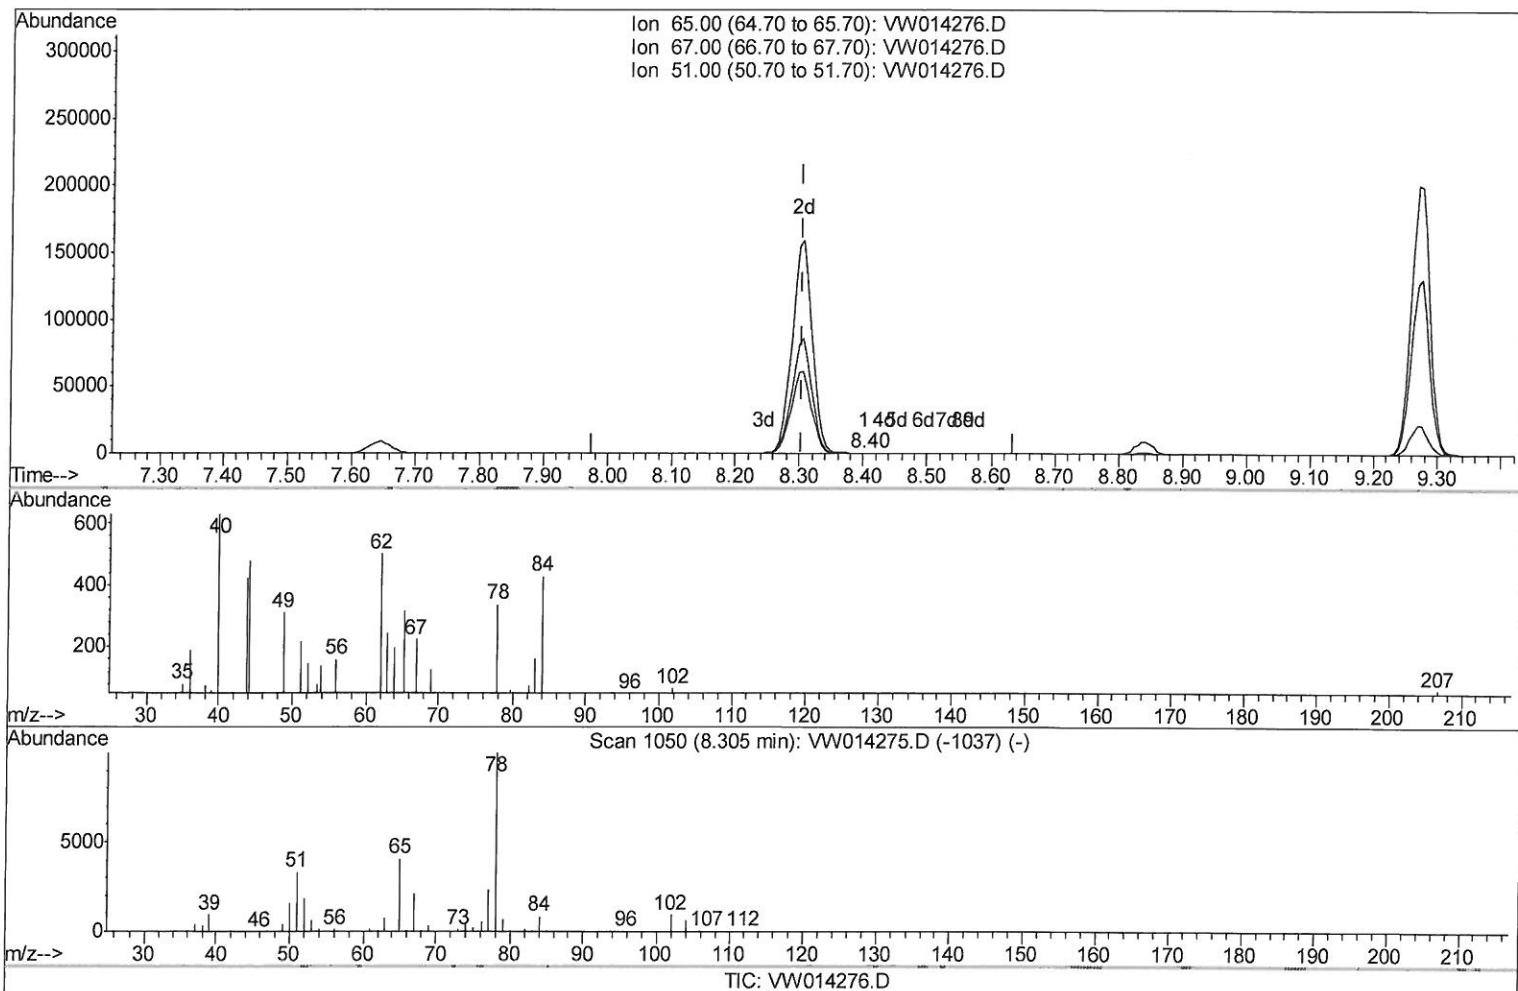

(26) 1,2-Dichloroethane-d4 (S)

8.403min (+0.098) 0.02ug/L

response 313

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	58.79
51.00	107.20	86.26
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121019\
 Data File : VW014276.D
 Acq On : 10 Dec 2019 12:04
 Operator : SY/VA
 Sample : VW1210SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampled :
 VBLK07

Manual Integrations
 APPROVED

MMDadoda
 12/11/2019 12:55:11 PM

Quant Time: Dec 11 04:10:47 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 04:05:19 2019
 Response via : Initial Calibration

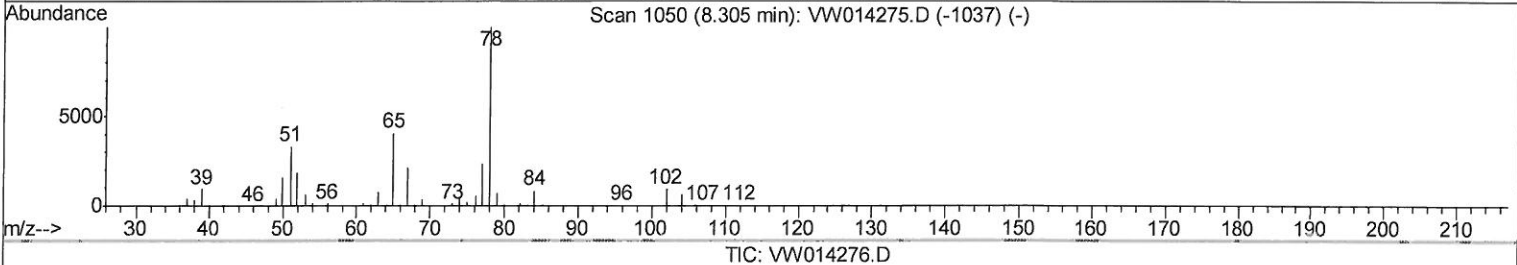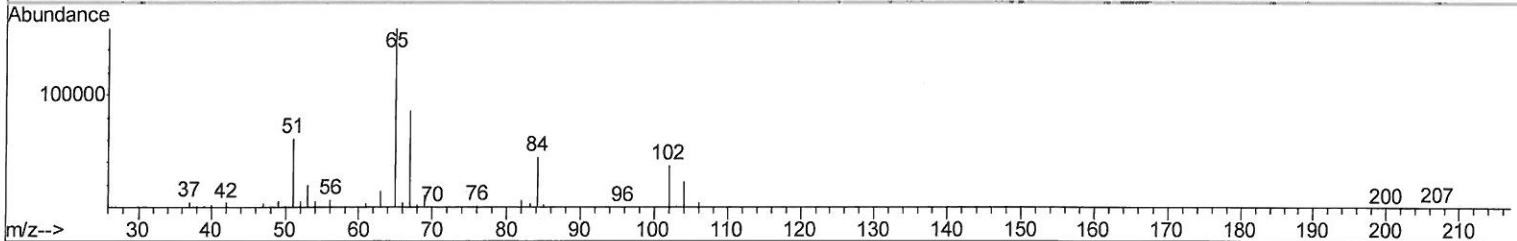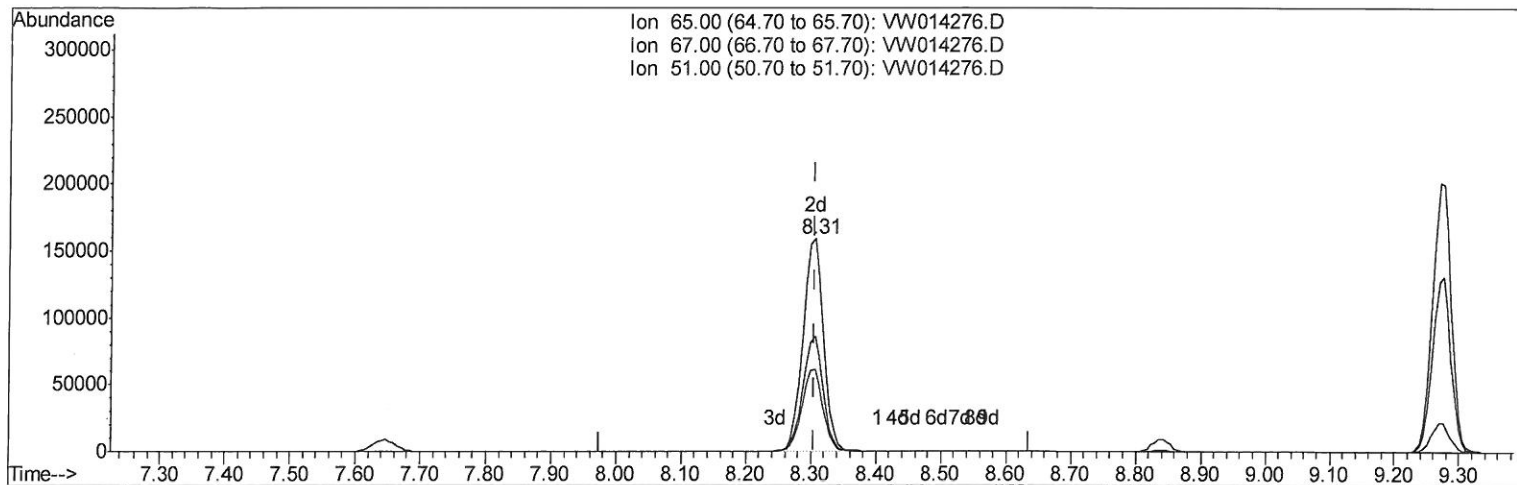

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.000) 25.36ug/L m

response 348419

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.05#
51.00	107.20	0.08#
0.00	0.00	0.00

12/11/19 SY

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121019\
 Data File : VW014276.D
 Acq On : 10 Dec 2019 12:04
 Operator : SY/VA
 Sample : VW1210SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK07

Manual Integrations
 APPROVED

MMDadoda
 12/11/2019 12:55:11 PM

Quant Time: Dec 11 04:15:25 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 04:05:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1029302	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	936330	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	393634	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	354699	22.76	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.04%		
7) Chloroethane-d5	2.89	69	272976	23.55	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	94.20%		
10) 1,1-Dichloroethene-d2	4.01	63	484680	17.61	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	70.44%		
20) 2-Butanone-d5	7.07	46	233918	57.59	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	115.18%		
24) Chloroform-d	7.64	84	614975	23.47	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	93.88%		
26) 1,2-Dichloroethane-d4	8.31	65	348419m	25.36	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	101.44%		
29) Benzene-d6	8.27	84	1297502	23.64	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	94.56%		
33) 1,2-Dichloropropane-d6	9.27	67	404381	23.95	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	95.80%		
37) Toluene-d8	10.32	98	1151195	23.20	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	92.80%		
38) trans-1,3-Dichloropropene-	10.58	79	161558	22.81	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	91.24%		
39) 2-Hexanone-d5	10.92	63	175152	52.18	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	104.36%		
48) 1,1,2,2-Tetrachloroethane-	12.69	84	353683	25.71	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	102.84%		
61) 1,2-Dichlorobenzene-d4	13.85	152	374478	24.90	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	99.60%		

12/11/19 SG

Target Compounds					Ovalue	
13) Acetone	4.12	43	27426	7.003	ug/L	74

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121019\
Data File : VW014276.D
Acq On : 10 Dec 2019 12:04
Operator : SY/VA
Sample : VW1210SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK07

Manual Integrations
APPROVED

MMDadoda
12/11/2019 12:55:11 PM

Quant Time: Dec 11 04:15:25 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 11 04:05:19 2019
Response via : Initial Calibration

