

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121019\
 Data File : VW014286.D
 Acq On : 10 Dec 2019 17:09
 Operator : SY/VA
 Sample : K6172-15
 Misc : 5.82G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 C0C11

Quant Time: Dec 11 05:25:14 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 11 04:05:19 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1248168	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1131054	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	475106	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	433154	22.92	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.68%
7) Chloroethane-d5	2.89	69	328082	23.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.40%
10) 1,1-Dichloroethene-d2	4.02	63	588519	17.63	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	70.52%
20) 2-Butanone-d5	7.07	46	180908	36.73	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	73.46%
24) Chloroform-d	7.65	84	749582	23.59	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	94.36%
26) 1,2-Dichloroethane-d4	8.30	65	380251	22.82	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	91.28%
29) Benzene-d6	8.27	84	1580075	23.84	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	95.36%
33) 1,2-Dichloropropane-d6	9.27	67	486693	23.86	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.44%
37) Toluene-d8	10.32	98	1406965	23.47	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	93.88%
38) trans-1,3-Dichloropropene-	10.58	79	182329	21.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	85.24%
39) 2-Hexanone-d5	10.92	63	140161	34.56	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	69.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	332325	20.00	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.00%
61) 1,2-Dichlorobenzene-d4	13.85	152	436264	24.03	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	96.12%


Target Compounds					Ovalue
13) Acetone	4.12	43	43130	9.082 ug/L	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW121019\
Data File : VW014286.D
Acq On : 10 Dec 2019 17:09
Operator : SY/VA
Sample : K6172-15
Misc : 5.82G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
C0C11

Quant Time: Dec 11 05:25:14 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 11 04:05:19 2019
Response via : Initial Calibration

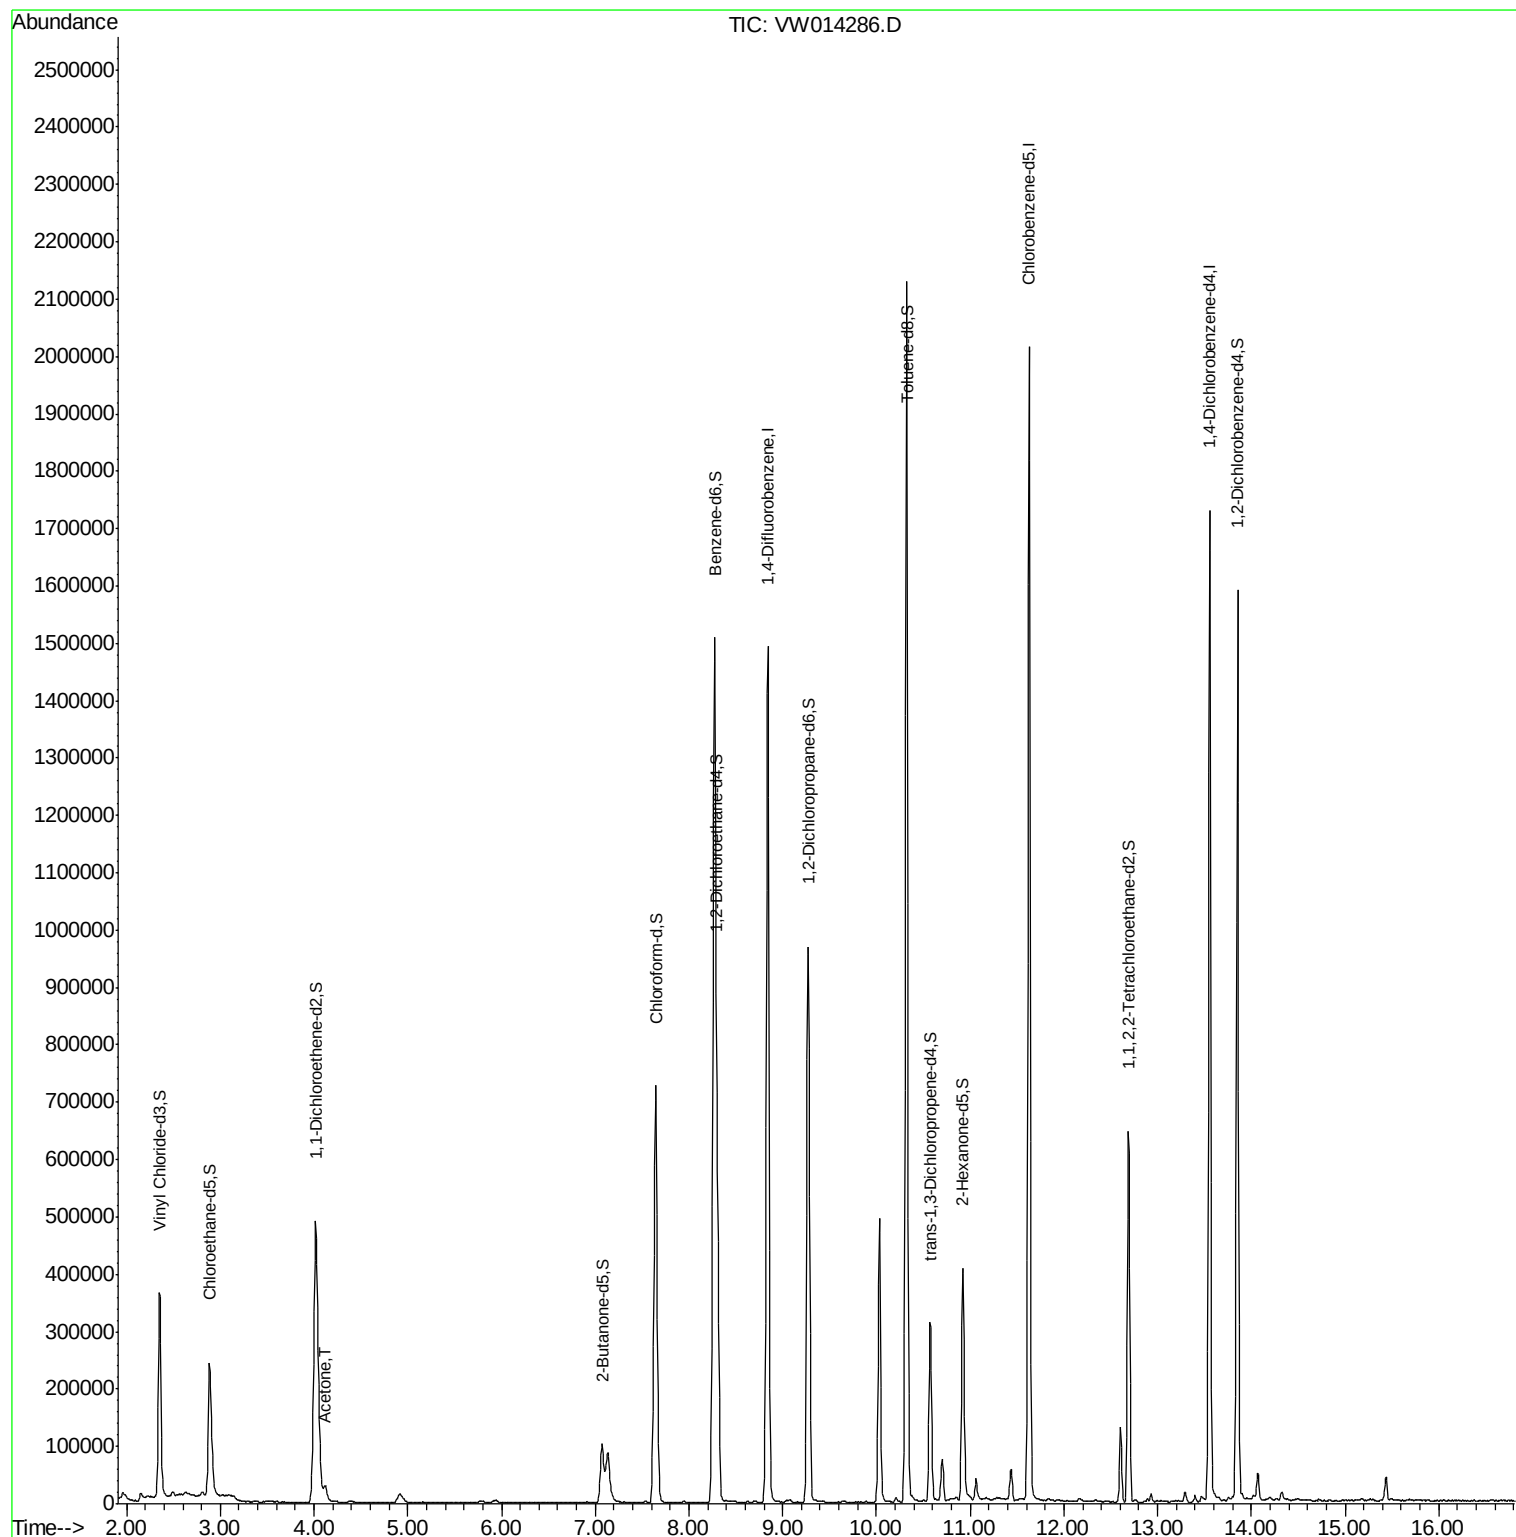

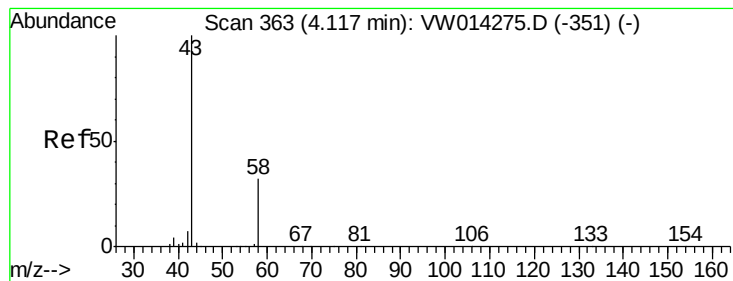

#13

Acetone

Concen: 9.082 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW014286.D

Acq: 10 Dec 2019 17:09

Instrument :

MSVOA_W

ClientSampleId :

C0C11

Tot Ion: 43 Resp: 43130

Ion Ratio Lower Upper

43 100

58 32.5 0.0 65.4

