




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
Data File : VW021306.D
Acq On : 11 Dec 2021 01:37
Operator : SY/VA
Sample : M5023-01
Misc : 6.27g/10.0mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGKX7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/12/2021
Supervised By :Mahesh Dadoda 12/15/2021

Quant Time: Dec 11 03:28:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 23:12:45 2021
Response via : Initial Calibration

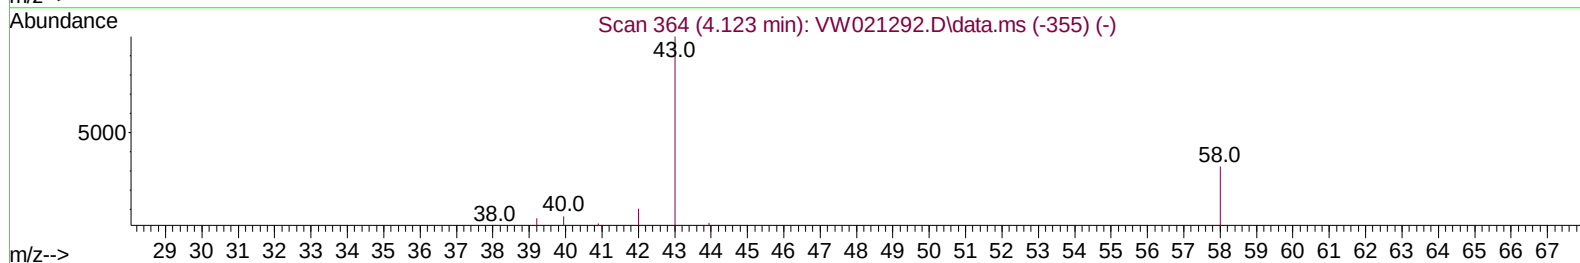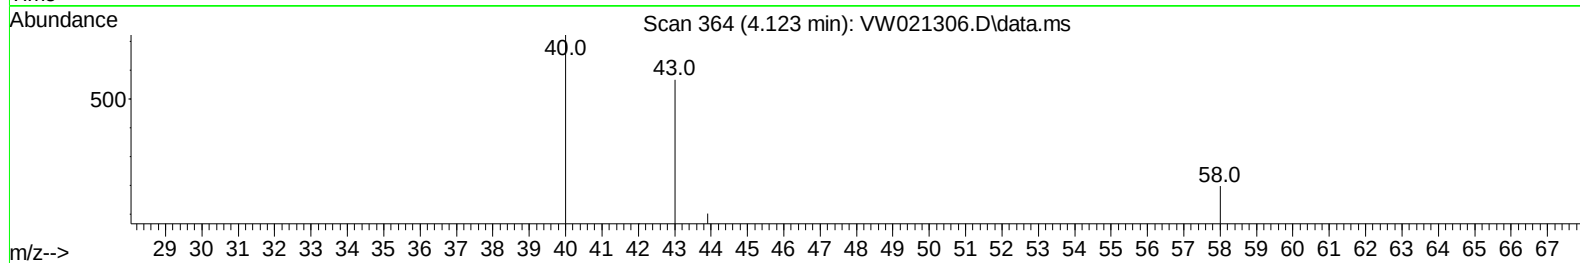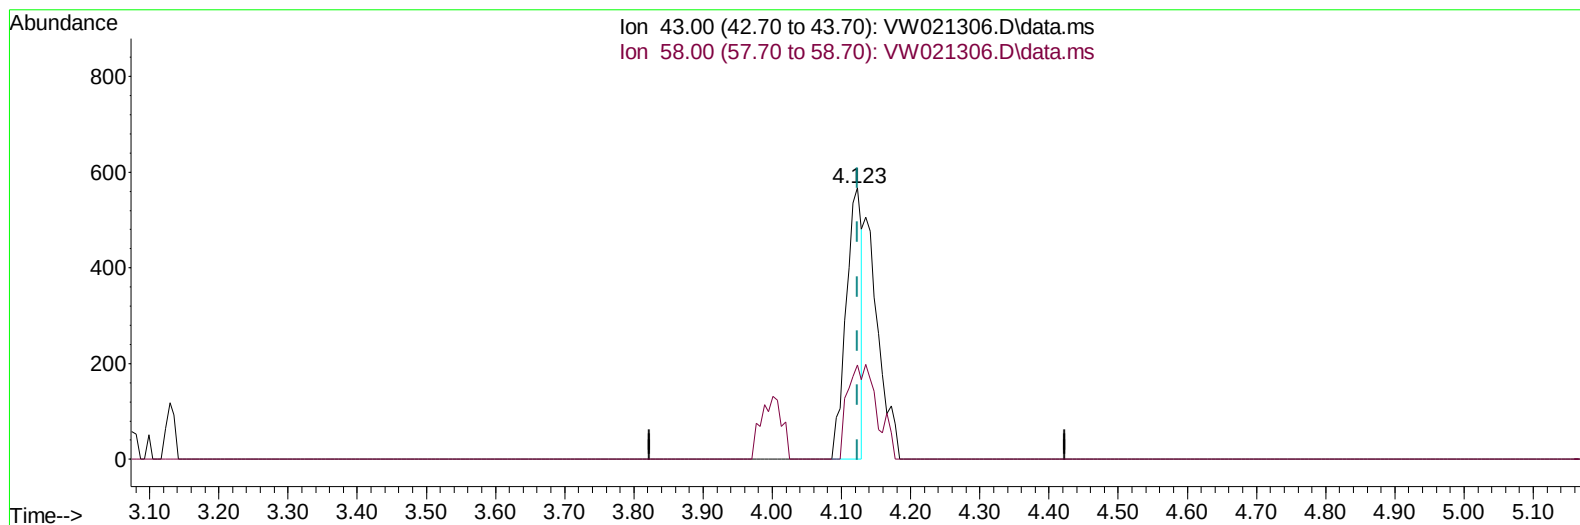

TIC: VW021306.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 7.99 ug/L

response 902

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	32.93
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
 Data File : VW021306.D
 Acq On : 11 Dec 2021 01:37
 Operator : SY/VA
 Sample : M5023-01
 Misc : 6.27g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGKX7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/12/2021
 Supervised By :Mahesh Dadoda 12/15/2021

Quant Time: Dec 11 03:28:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration

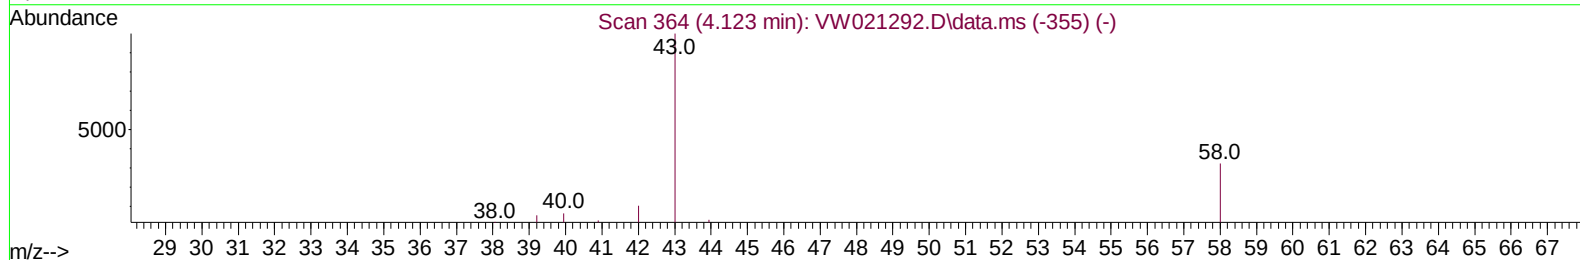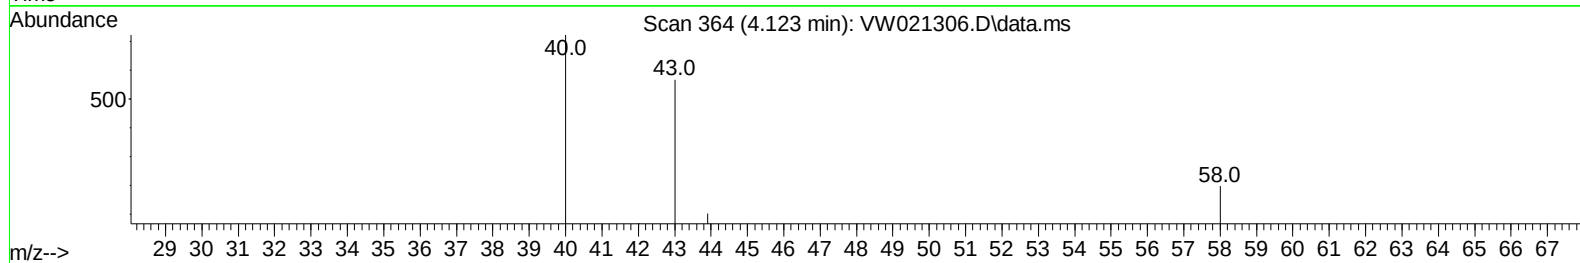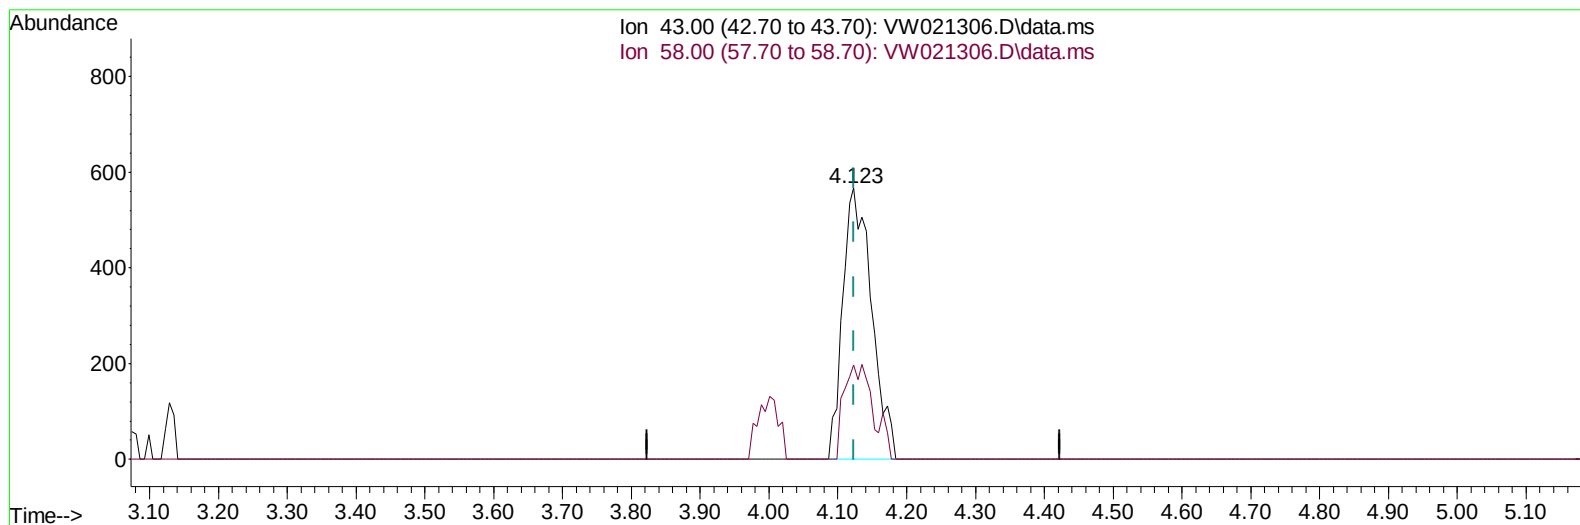

TIC: VW021306.D\data.ms

(13) Acetone (T)

4.123min (-0.000) 14.60 ug/L m

response 1649

Ion	Exp%	Act%
43.00	100.00	100.00
58.00	26.40	18.01
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121021\
 Data File : VW021306.D
 Acq On : 11 Dec 2021 01:37
 Operator : SY/VA
 Sample : M5023-01
 Misc : 6.27g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGKX7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/12/2021
 Supervised By :Mahesh Dadoda 12/15/2021

Quant Time: Dec 11 03:28:39 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.841	114	49075	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.634	117	36549	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	12880	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	24354	27.248	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	109.000%	
7) Chloroethane-d5	2.879	69	19149	32.409	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	129.640%	
11) 1,1-Dichloroethene-d2	4.019	63	23849	20.015	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	80.040%	
21) 2-Butanone-d5	7.074	46	11125	88.302	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	176.600%#	
24) Chloroform-d	7.647	84	42358	30.972	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	123.880%	
26) 1,2-Dichloroethane-d4	8.305	65	22500	30.929	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	123.720%	
32) Benzene-d6	8.275	84	71609	35.744	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	142.960%#	
36) 1,2-Dichloropropane-d6	9.274	67	21159	39.382	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	157.520%#	
41) Toluene-d8	10.323	98	56288	27.499	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	110.000%	
43) trans-1,3-Dichloroprop...	10.579	79	6953	28.105	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	112.440%	
47) 2-Hexanone-d5	10.920	63	6849	86.206	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	172.420%#	
56) 1,1,2,2-Tetrachloroeth...	12.694	84	15333	33.198	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	132.800%#	
66) 1,2-Dichlorobenzene-d4	13.853	152	10694	21.423	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	85.680%	
Target Compounds						Qvalue
13) Acetone	4.123	43	1649m	14.600	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
Data File : VW021306.D
Acq On : 11 Dec 2021 01:37
Operator : SY/VA
Sample : M5023-01
Misc : 6.27g/10.0mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGKX7

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/12/2021
Supervised By :Mahesh Dadoda 12/15/2021

Quant Time: Dec 11 03:28:39 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 23:12:45 2021
Response via : Initial Calibration

