

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
 Data File : VW021309.D
 Acq On : 11 Dec 2021 02:49
 Operator : SY/VA
 Sample : VIBLK526
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK526

Quant Time: Dec 11 03:29:15 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.842	114	81731	25.000	ug/L	# 0.00
28) Chlorobenzene-d5	11.628	117	79999	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.554	152	42010	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.349	65	36865	24.766	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	99.080%
7) Chloroethane-d5	2.885	69	25104	25.511	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	102.040%
11) 1,1-Dichloroethene-d2	4.019	63	35473	17.875	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	71.520%
21) 2-Butanone-d5	7.080	46	11863	56.538	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	113.080%
24) Chloroform-d	7.647	84	56169	24.661	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	98.640%
26) 1,2-Dichloroethane-d4	8.305	65	30184	24.913	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	99.640%
32) Benzene-d6	8.275	84	109815	25.043	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.160%
36) 1,2-Dichloropropane-d6	9.275	67	29962	25.478	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.920%
41) Toluene-d8	10.323	98	106472	23.764	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.040%
43) trans-1,3-Dichloroprop...	10.579	79	12772	23.587	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.360%
47) 2-Hexanone-d5	10.921	63	8919	51.288	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.580%
56) 1,1,2,2-Tetrachloroeth...	12.689	84	25840	25.560	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.240%
66) 1,2-Dichlorobenzene-d4	13.853	152	39053	23.987	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.960%
Target Compounds						
13) Acetone	4.135	43	828	4.402	ug/L	Qvalue 91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
Data File : VW021309.D
Acq On : 11 Dec 2021 02:49
Operator : SY/VA
Sample : VIBLK526
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK526

Quant Time: Dec 11 03:29:15 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 23:12:45 2021
Response via : Initial Calibration

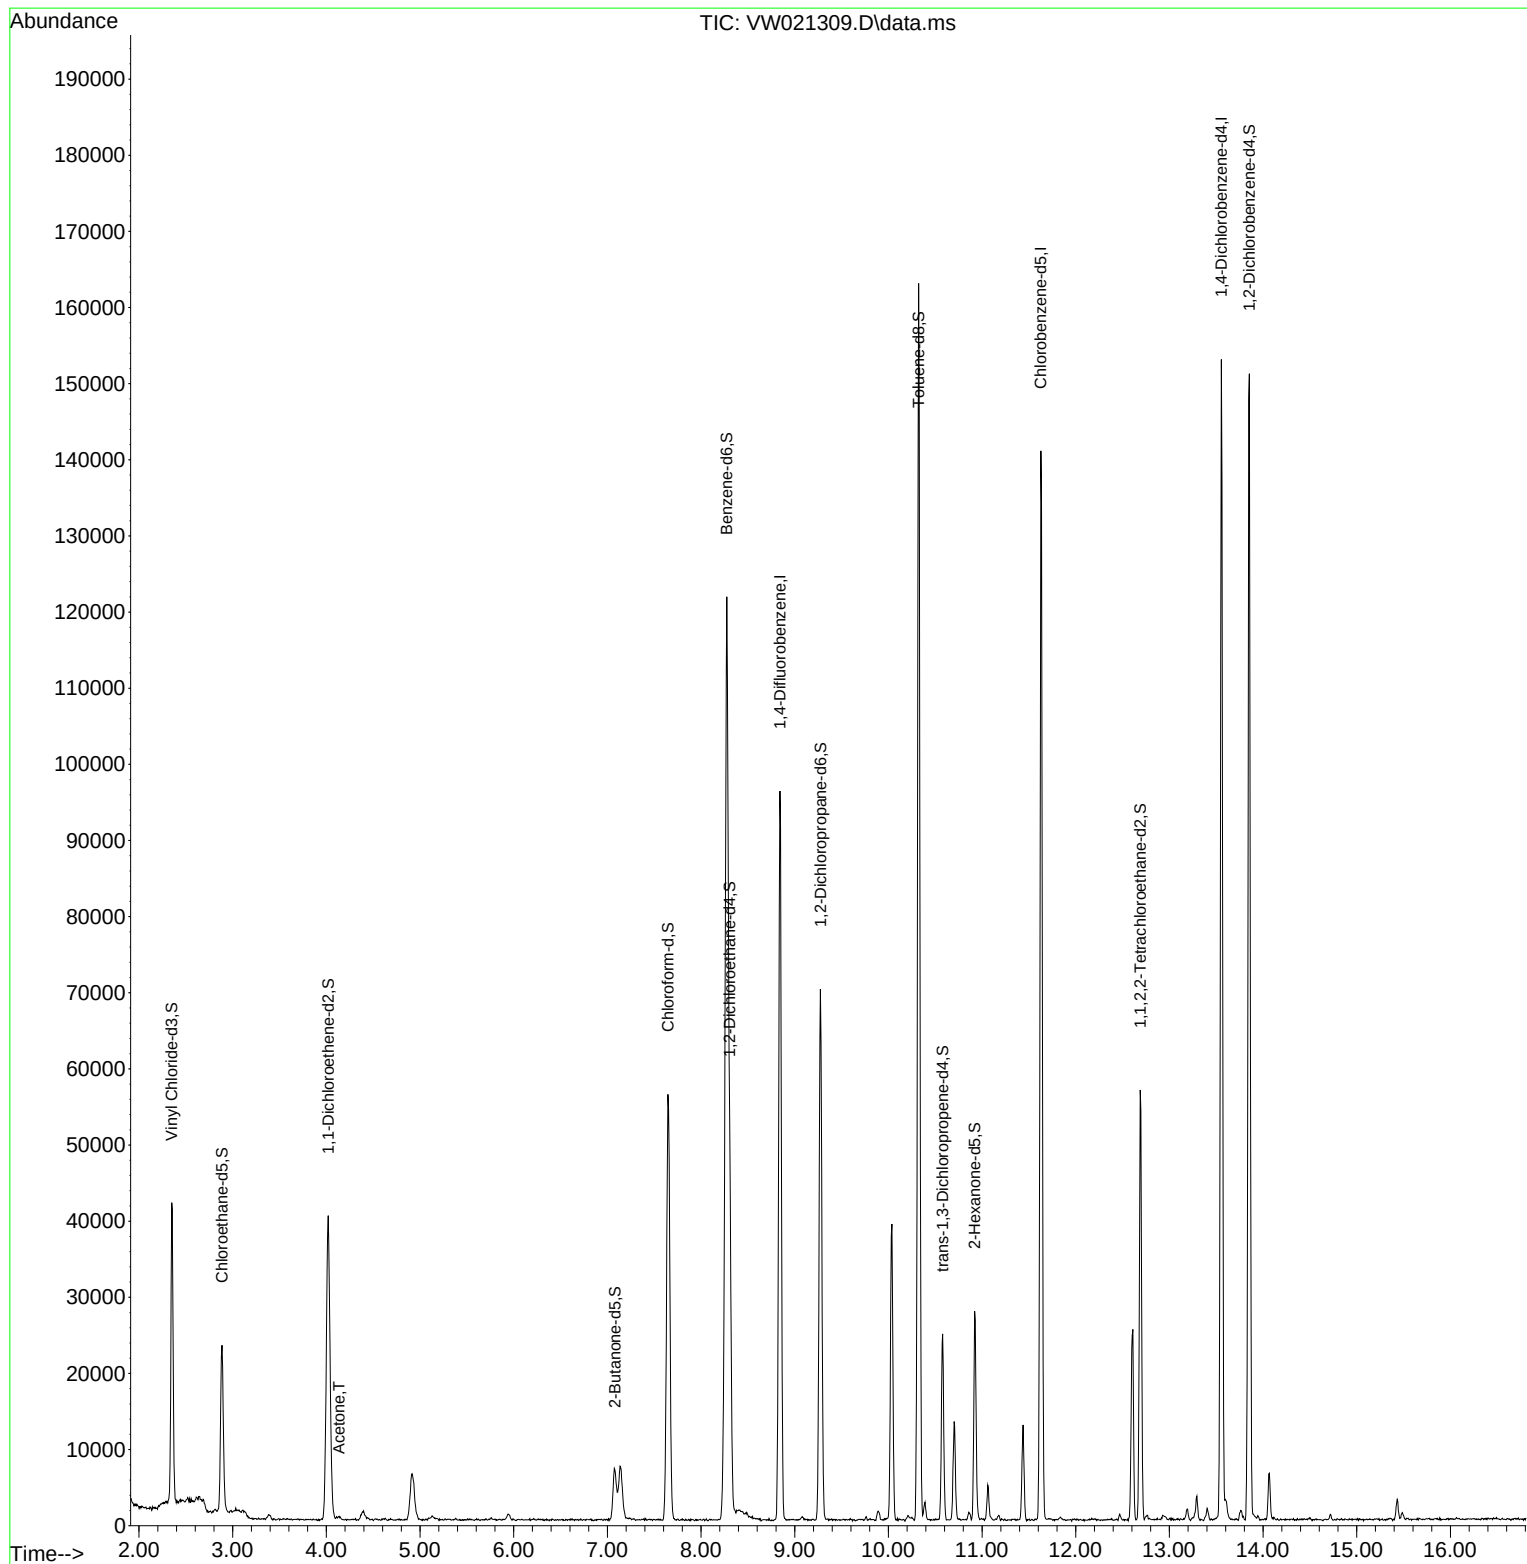

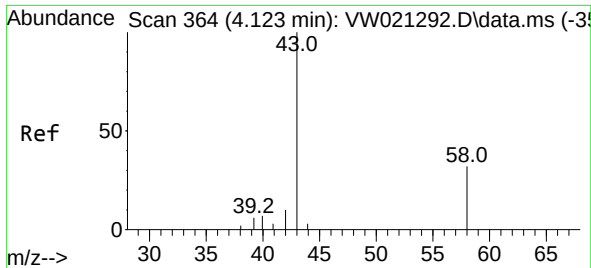

#13
 Acetone
 Concen: 4.402 ug/L
 RT: 4.135 min Scan# 30
 Delta R.T. 0.012 min
 Lab File: VW021309.D
 Acq: 11 Dec 2021 02:49

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK526

Tgt Ion: 43 Resp: 828
 Ion Ratio Lower Upper
 43 100
 58 21.9 0.0 52.8

