

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
 Data File : VW021314.D
 Acq On : 11 Dec 2021 04:48
 Operator : SY/VA
 Sample : VIBLK527
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK527

Quant Time: Dec 11 05:18:06 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 10 23:12:45 2021
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.842	114	72880	25.000	ug/L	# 0.00
28) Chlorobenzene-d5		11.634	117	69128	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.560	152	35255	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.355	65	36020	27.137	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 108.560%		
7) Chloroethane-d5		2.885	69	25024	28.518	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	= 114.080%		
11) 1,1-Dichloroethene-d2		4.019	63	33551	18.960	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	= 75.840%		
21) 2-Butanone-d5		7.080	46	11661	62.324	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 124.640%		
24) Chloroform-d		7.653	84	51770	25.490	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	= 101.960%		
26) 1,2-Dichloroethane-d4		8.305	65	28551	26.428	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	= 105.720%		
32) Benzene-d6		8.275	84	101161	26.698	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	= 106.800%		
36) 1,2-Dichloropropane-d6		9.275	67	27837	27.393	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	= 109.560%		
41) Toluene-d8		10.323	98	97477	25.178	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	= 100.720%		
43) trans-1,3-Dichloroprop...		10.579	79	12293	26.272	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	= 105.080%		
47) 2-Hexanone-d5		10.921	63	9056	60.265	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	= 120.540%		
56) 1,1,2,2-Tetrachloroeth...		12.689	84	25024	28.646	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	= 114.600%		
66) 1,2-Dichlorobenzene-d4		13.853	152	37503	27.448	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	= 109.800%		
Target Compounds							
13) Acetone		4.123	43	652	3.887	ug/L	Qvalue 73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
Data File : VW021314.D
Acq On : 11 Dec 2021 04:48
Operator : SY/VA
Sample : VIBLK527
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VIBLK527

Quant Time: Dec 11 05:18:06 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 10 23:12:45 2021
Response via : Initial Calibration

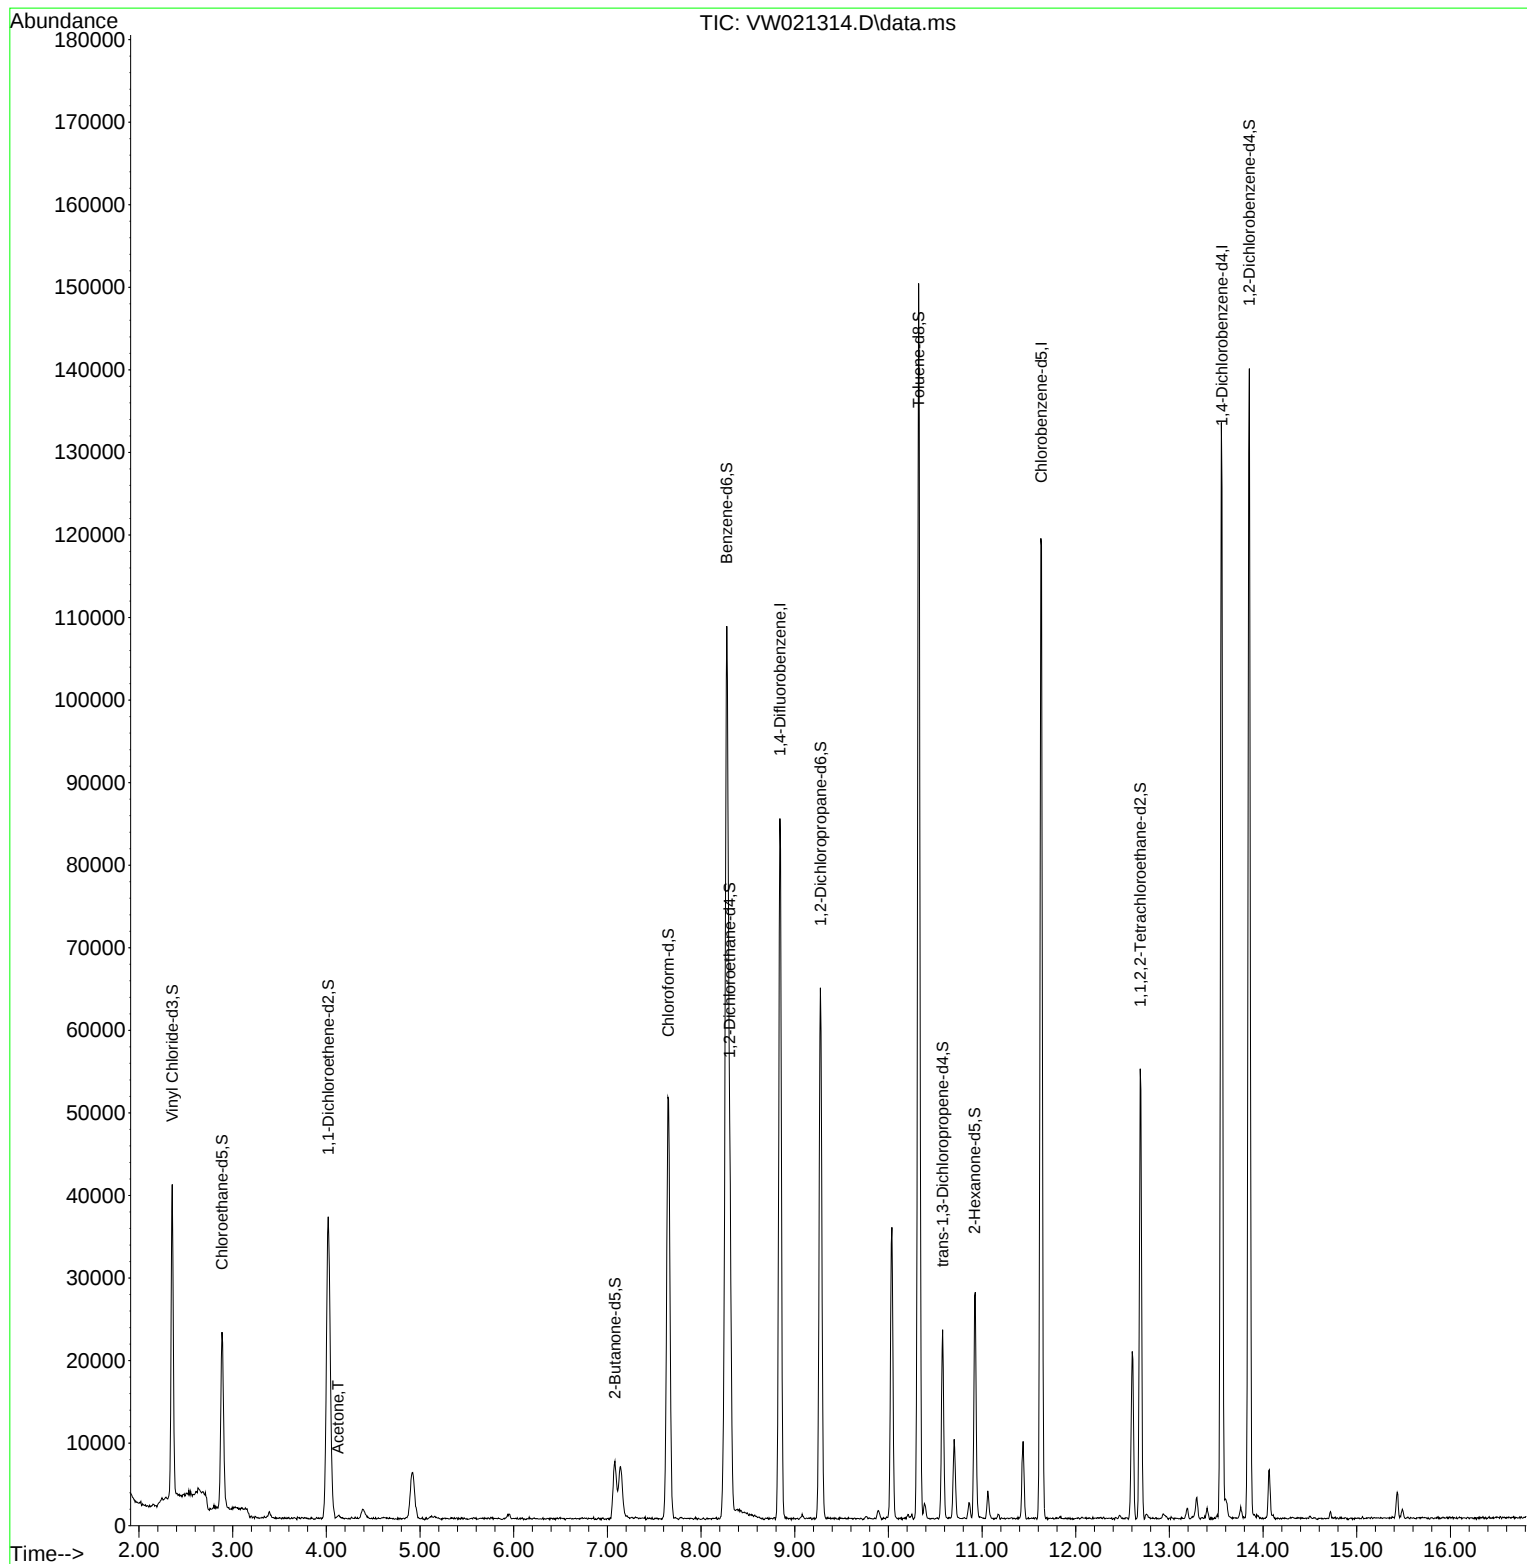

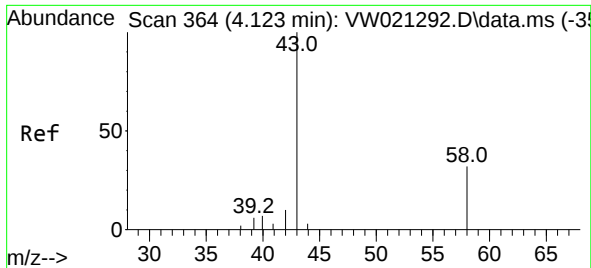

#13
 Acetone
 Concen: 3.887 ug/L
 RT: 4.123 min Scan# 30
 Delta R.T. 0.000 min
 Lab File: VW021314.D
 Acq: 11 Dec 2021 04:48

Instrument :
 MSVOA_W
 ClientSampleId :
 VIBLK527

Tgt Ion:	43	Resp:	652
Ion	Ratio	Lower	Upper
43	100		
58	12.6	0.0	52.8

