
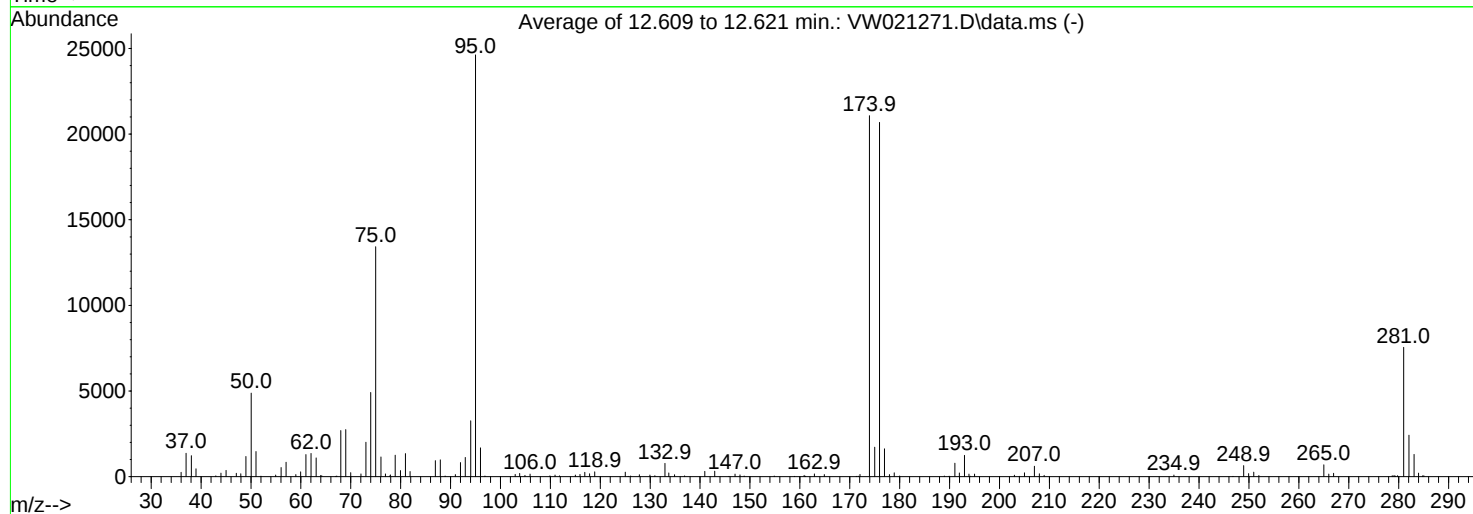


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121021\
Data File : VW021271.D
Acq On : 10 Dec 2021 07:51
Operator : SY/VA
Sample : BFB476
Misc : 5.00g/10.0mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB476

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
Title : SFAM01.0
Last Update : Wed Dec 15 00:46:16 2021

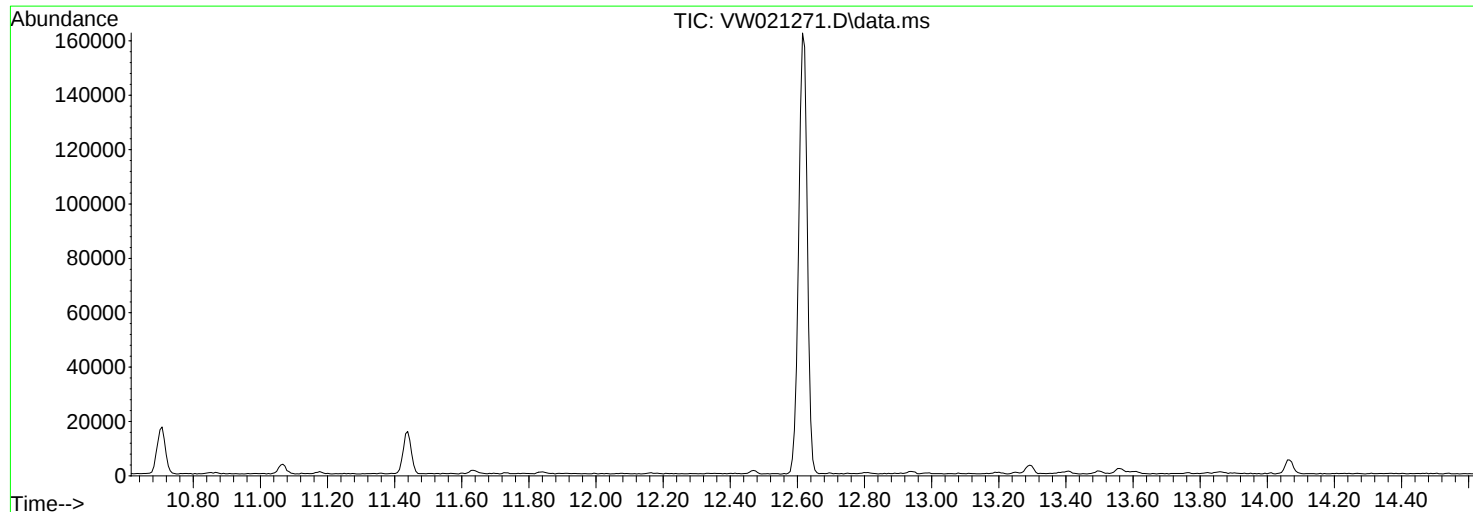

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.8	4876	PASS
75	95	30	80	54.5	13428	PASS
95	95	100	100	100.0	24629	PASS
96	95	5	9	6.8	1685	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	85.6	21078	PASS
175	174	5	9	8.1	1717	PASS
176	174	95	105	98.1	20688	PASS
177	176	5	10	7.9	1628	PASS

Scan 1750 (12.573 min): VW021271.D\data.ms
BFB476

m/z	Abundance
40.00	866.0
44.00	86.0
280.90	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

m/z	Abundance
36.00	237.0
37.00	1178.0
38.00	1042.0
39.00	399.0
40.00	747.0
43.00	78.0
44.10	237.0
45.00	395.0
47.00	225.0
47.90	177.0
49.00	946.0
50.00	4314.0
51.00	1161.0
55.00	79.0
56.10	458.0
57.10	721.0
59.00	228.0
59.90	266.0
61.00	1226.0
62.10	1183.0
63.00	923.0
64.00	99.0
67.00	69.0
68.00	2158.0
69.00	2332.0
70.00	157.0
72.10	117.0
73.00	2210.0
74.00	4144.0
75.00	10887.0
76.00	1061.0
77.00	159.0
77.80	121.0
78.90	1086.0
79.90	327.0
81.00	1047.0
81.90	283.0
87.00	763.0
88.00	852.0
88.90	64.0
90.90	91.0
92.00	674.0
93.00	883.0
94.00	2564.0
95.00	19584.0
96.00	1276.0
102.90	216.0
103.90	191.0
104.90	82.0
105.90	117.0
109.90	81.0
111.00	99.0
111.90	61.0
115.00	117.0
116.00	152.0
117.00	186.0
117.80	199.0
119.00	281.0
125.10	415.0
126.10	122.0
127.90	56.0
130.00	58.0
131.00	106.0
133.00	1167.0
133.80	285.0
134.90	165.0
140.90	245.0
143.00	267.0
147.00	231.0
148.00	98.0
148.90	52.0
154.90	55.0
160.80	67.0
162.90	267.0
164.90	198.0
171.70	80.0
172.20	123.0
174.00	15433.0
175.00	1459.0
175.90	14992.0
177.00	1416.0
178.10	140.0
178.90	315.0
180.00	62.0
188.90	58.0
189.90	73.0
191.00	1065.0
192.00	384.0
193.00	1704.0
193.90	297.0
195.00	250.0
203.10	150.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

204.00	60.0
205.00	328.0
207.00	847.0
208.00	221.0
209.00	164.0
234.90	115.0
246.80	55.0
248.90	934.0
249.90	241.0
251.00	286.0
252.00	132.0
265.00	953.0
266.00	180.0
266.90	279.0
278.70	133.0
279.20	155.0
281.00	10097.0
282.10	3571.0
283.10	1810.0
283.90	202.0
284.80	152.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

m/z	Abundance
36.00	271.0
37.00	1527.0
38.10	1350.0
39.00	502.0
40.00	873.0
42.90	50.0
44.00	300.0
45.00	428.0
47.10	196.0
47.90	180.0
49.00	1430.0
50.00	5308.0
51.00	1645.0
52.00	72.0
55.00	117.0
56.00	578.0
57.10	1005.0
59.00	132.0
60.00	292.0
61.00	1443.0
62.00	1435.0
63.10	1215.0
63.90	91.0
64.20	95.0
68.00	3003.0
69.00	3009.0
70.00	253.0
72.00	199.0
73.00	2124.0
74.00	5331.0
75.00	15138.0
76.00	1182.0
77.00	157.0
78.00	170.0
78.90	1421.0
79.90	372.0
81.00	1462.0
81.90	303.0
86.90	1008.0
88.00	1013.0
90.90	137.0
92.00	862.0
92.90	1244.0
94.10	3539.0
95.00	27760.0
96.00	1895.0
96.90	63.0
103.00	179.0
103.80	197.0
104.90	80.0
106.00	191.0
109.90	60.0
111.00	117.0
111.80	75.0
114.90	116.0
115.90	112.0
116.80	257.0
117.90	172.0
118.90	328.0
124.90	231.0
127.80	127.0
129.90	118.0
130.90	76.0
132.90	740.0
133.70	247.0
134.90	116.0
136.90	67.0
140.90	302.0
143.00	367.0
145.80	58.0
147.00	132.0
148.00	121.0
148.80	51.0
158.90	63.0
160.90	156.0
162.90	130.0
165.00	115.0
172.00	121.0
174.00	22048.0
175.00	2130.0
176.00	20968.0
176.90	1740.0
177.90	133.0
178.90	244.0
180.00	65.0
191.10	909.0
191.90	183.0
193.00	1307.0
193.90	145.0
195.00	122.0
202.90	102.0
205.00	198.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

207.00	702.0
208.00	227.0
208.90	55.0
235.00	102.0
249.00	626.0
250.00	190.0
250.90	318.0
252.00	61.0
265.00	704.0
266.00	181.0
267.00	202.0
278.90	114.0
279.80	160.0
281.10	7404.0
282.00	2227.0
283.10	1593.0
284.00	236.0
285.00	102.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

m/z	Abundance
36.00	239.0
37.00	1385.0
38.10	1289.0
39.00	473.0
40.00	795.0
44.10	342.0
45.00	282.0
47.10	181.0
48.00	137.0
49.00	1165.0
50.10	5005.0
51.00	1583.0
54.90	89.0
56.00	554.0
57.00	804.0
60.00	270.0
61.00	1201.0
62.00	1442.0
63.10	1132.0
64.20	65.0
67.20	110.0
68.00	2922.0
69.00	2890.0
70.00	304.0
72.00	157.0
73.10	1695.0
74.00	5282.0
75.00	14258.0
76.10	1198.0
76.80	163.0
77.90	152.0
78.90	1242.0
80.00	378.0
80.90	1530.0
81.90	316.0
86.90	1044.0
87.90	1085.0
88.90	50.0
91.00	145.0
92.00	931.0
93.00	1239.0
94.00	3693.0
95.00	26544.0
96.00	1884.0
96.90	54.0
103.90	177.0
104.90	67.0
106.00	142.0
110.80	73.0
115.10	56.0
115.90	137.0
116.90	300.0
117.90	126.0
118.80	246.0
124.90	134.0
125.60	54.0
127.90	151.0
129.90	94.0
133.00	409.0
133.80	119.0
135.00	69.0
136.90	64.0
141.00	372.0
142.90	324.0
147.00	84.0
148.00	97.0
154.80	63.0
161.10	75.0
162.90	89.0
164.80	63.0
171.30	59.0
171.90	137.0
173.90	25752.0
175.00	1561.0
175.90	26104.0
176.90	1729.0
177.90	93.0
178.90	120.0
189.00	59.0
191.00	380.0
191.90	90.0
193.00	723.0
194.10	97.0
194.90	88.0
205.00	134.0
207.10	278.0
208.00	60.0
234.90	58.0
249.00	384.0
250.00	97.0
251.00	179.0
264.90	430.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476

265.90	86.0
266.90	107.0
278.90	55.0
279.40	90.0
281.10	5302.0
282.10	1452.0
283.10	498.0
284.10	171.0
285.10	69.0

Instrument :
MSVOA_W
ClientSampleId :
BFB476