

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121119\
 Data File : VW014307.D
 Acq On : 11 Dec 2019 16:47
 Operator : SY/VA
 Sample : K6238-01
 Misc : 4.77G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFPZ6

Manual Integrations
 APPROVED

apatel
 12/12/2019 4:21:16 PM

Quant Time: Dec 12 05:00:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 12 04:57:07 2019
 Response via : Initial Calibration

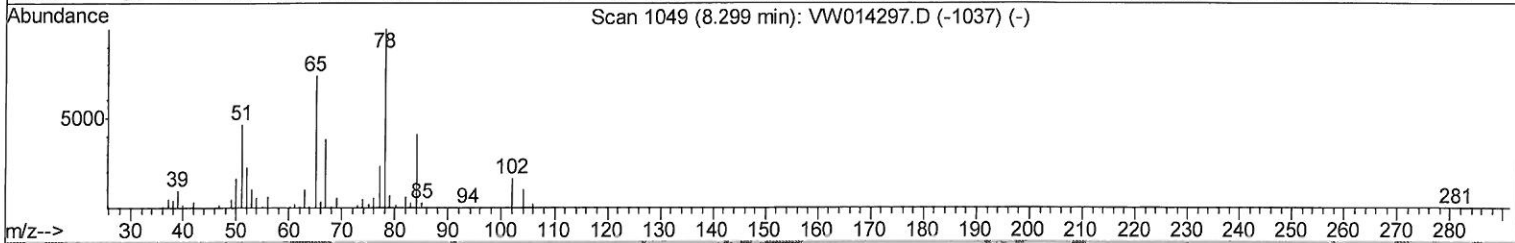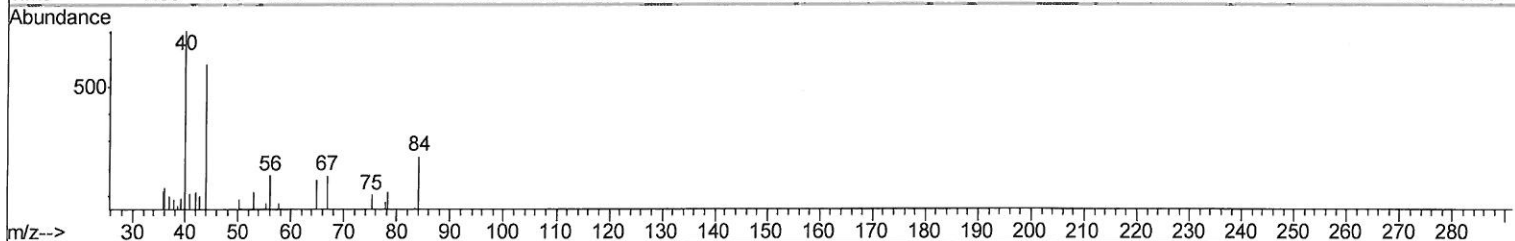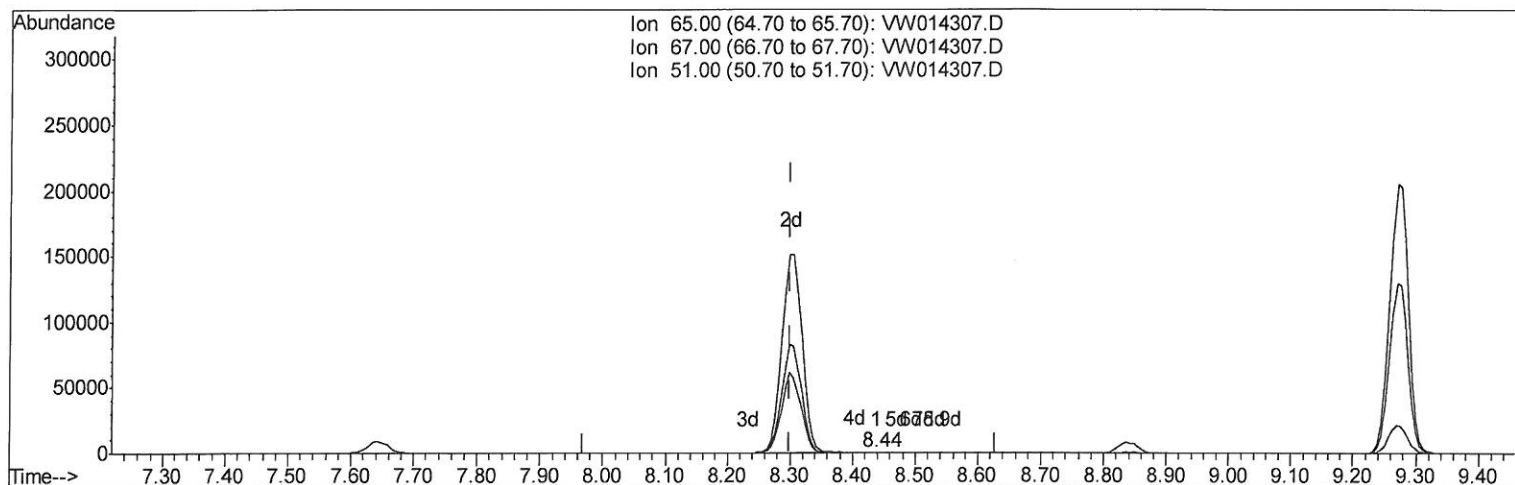

(26) 1,2-Dichloroethane-d4 (S)

8.439min (+0.141) 0.02ug/L

response 233

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	51.93
51.00	107.20	86.70
0.00	0.00	0.00

Quantitation Report (Qedit)




Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121119\
 Data File : VW014307.D
 Acq On : 11 Dec 2019 16:47
 Operator : SY/VA
 Sample : K6238-01
 Misc : 4.77G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
ClientSampled :
 BFPZ6

Manual Integrations
APPROVED

apatel
 12/12/2019 4:21:16 PM

Quant Time: Dec 12 05:00:13 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 12 04:57:07 2019
 Response via : Initial Calibration

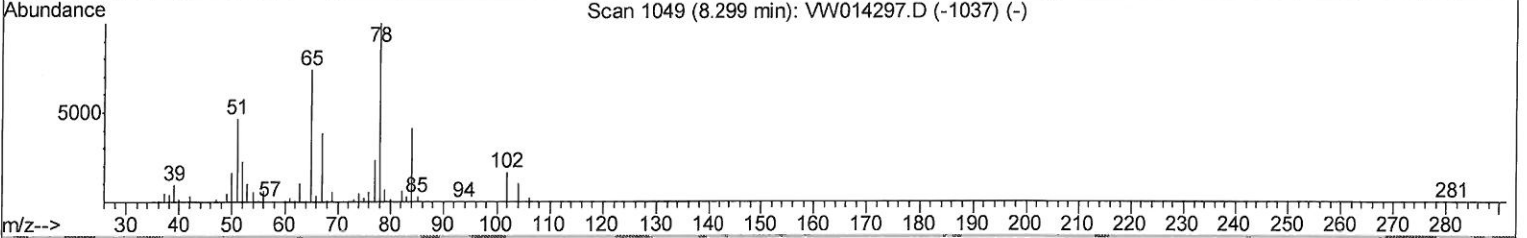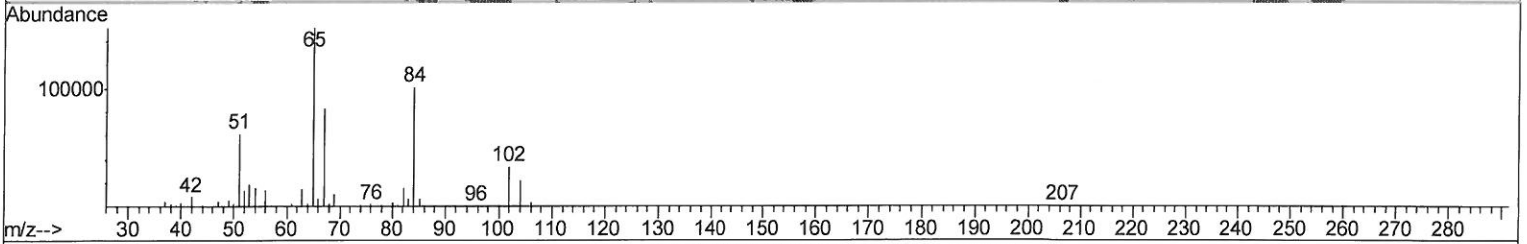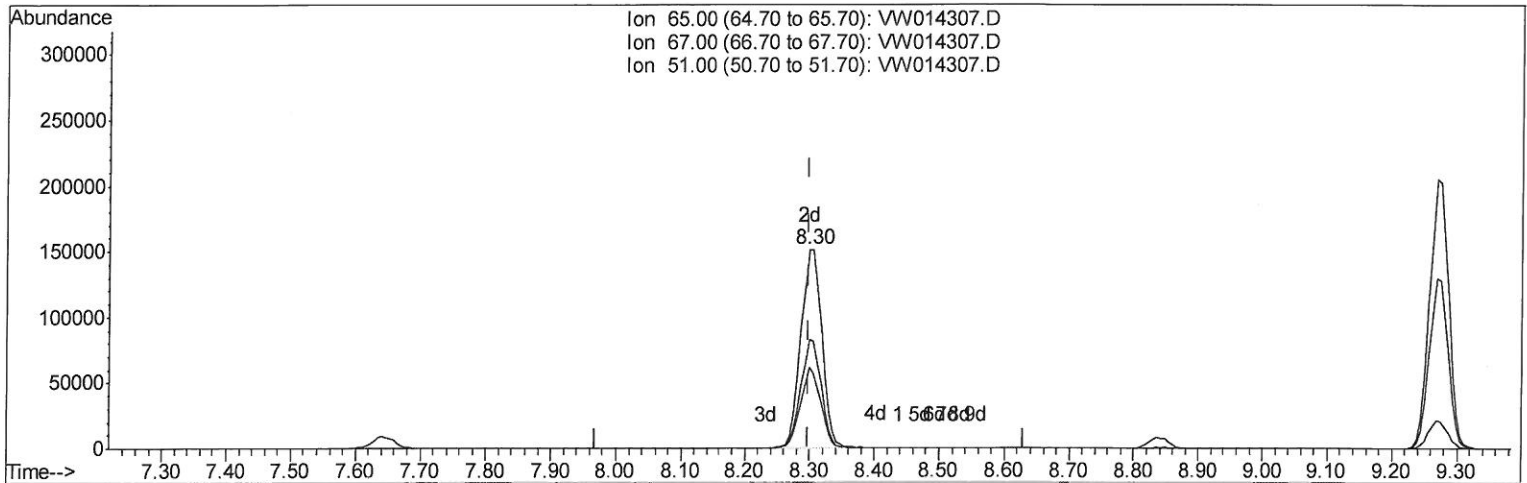

TIC: VW014307.D

(26) 1,2-Dichloroethane-d4 (S)

8.299min (+0.000) 25.80ug/L m

response 341304

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.04#
51.00	107.20	0.06#
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121119\
 Data File : VW014307.D
 Acq On : 11 Dec 2019 16:47
 Operator : SY/VA
 Sample : K6238-01
 Misc : 4.77G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFPZ6

Manual Integrations
 APPROVED

apatel
 12/12/2019 4:21:16 PM

Quant Time: Dec 12 06:09:29 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Thu Dec 12 04:57:07 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	990877	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	705602	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	160570	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	357152	23.80	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	95.20%
7) Chloroethane-d5	2.89	69	306899	27.51	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	110.04%
10) 1,1-Dichloroethene-d2	4.01	63	520074	19.62	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.48%
20) 2-Butanone-d5	7.08	46	124038	31.72	ug/L	0.01
Spiked Amount	50.000	Range	20 - 135	Recovery	=	63.44%
24) Chloroform-d	7.64	84	652930	25.88	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.52%
26) 1,2-Dichloroethane-d4	8.30	65	341304m	25.80	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	103.20%
29) Benzene-d6	8.27	84	1333630	32.25	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	129.00%
33) 1,2-Dichloropropane-d6	9.27	67	416063	32.70	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	130.80%#
37) Toluene-d8	10.32	98	1060983	28.37	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	113.48%
38) trans-1,3-Dichloropropene-	10.57	79	125806	23.57	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	94.28%
39) 2-Hexanone-d5	10.92	63	90189	35.65	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	71.30%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	208037	20.07	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	80.28%
61) 1,2-Dichlorobenzene-d4	13.85	152	146719	23.91	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.64%

Target Compounds					Ovalue
13) Acetone	4.12	43	632725	167.837	ug/L 98

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121119\
Data File : VW014307.D
Acq On : 11 Dec 2019 16:47
Operator : SY/VA
Sample : K6238-01
Misc : 4.77G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFPZ6

Manual Integrations
APPROVED

apatel
12/12/2019 4:21:16 PM

Quant Time: Dec 12 06:09:29 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 12 04:57:07 2019
Response via : Initial Calibration

