

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121218\
 Data File : VW007398.D
 Acq On : 11 Dec 2018 15:50
 Operator : SY/AP
 Sample : J6271-11
 Misc : 6.50G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F9E26

Quant Time: Dec 12 03:34:50 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 11 01:18:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	128868	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	116724	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	51763	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	22637	26.97	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	107.88%
7) Chloroethane-d5	2.89	69	16606	23.36	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	93.44%
10) 1,1-Dichloroethene-d2	4.01	63	56869	19.64	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	78.56%
20) 2-Butanone-d5	7.08	46	22897	43.28	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	86.56%
24) Chloroform-d	7.65	84	79260	26.08	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	104.32%
26) 1,2-Dichloroethane-d4	8.31	65	47595	27.51	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	110.04%
29) Benzene-d6	8.27	84	155464	24.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.08%
33) 1,2-Dichloropropane-d6	9.27	67	45053	24.90	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	99.60%
37) Toluene-d8	10.32	98	149557	25.16	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	100.64%
38) trans-1,3-Dichloropropene-	10.58	79	22291	24.10	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	96.40%
39) 2-Hexanone-d5	10.93	63	18687	42.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	85.82%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	40213	24.40	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	97.60%
61) 1,2-Dichlorobenzene-d4	13.86	152	49277	27.06	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	108.24%


Target Compounds					Ovalue
13) Acetone	4.12	43	1751	2.846 ug/L	73


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW121218\
Data File : VW007398.D
Acq On : 11 Dec 2018 15:50
Operator : SY/AP
Sample : J6271-11
Misc : 6.50G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F9E26

Quant Time: Dec 12 03:34:50 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 11 01:18:15 2018
Response via : Initial Calibration

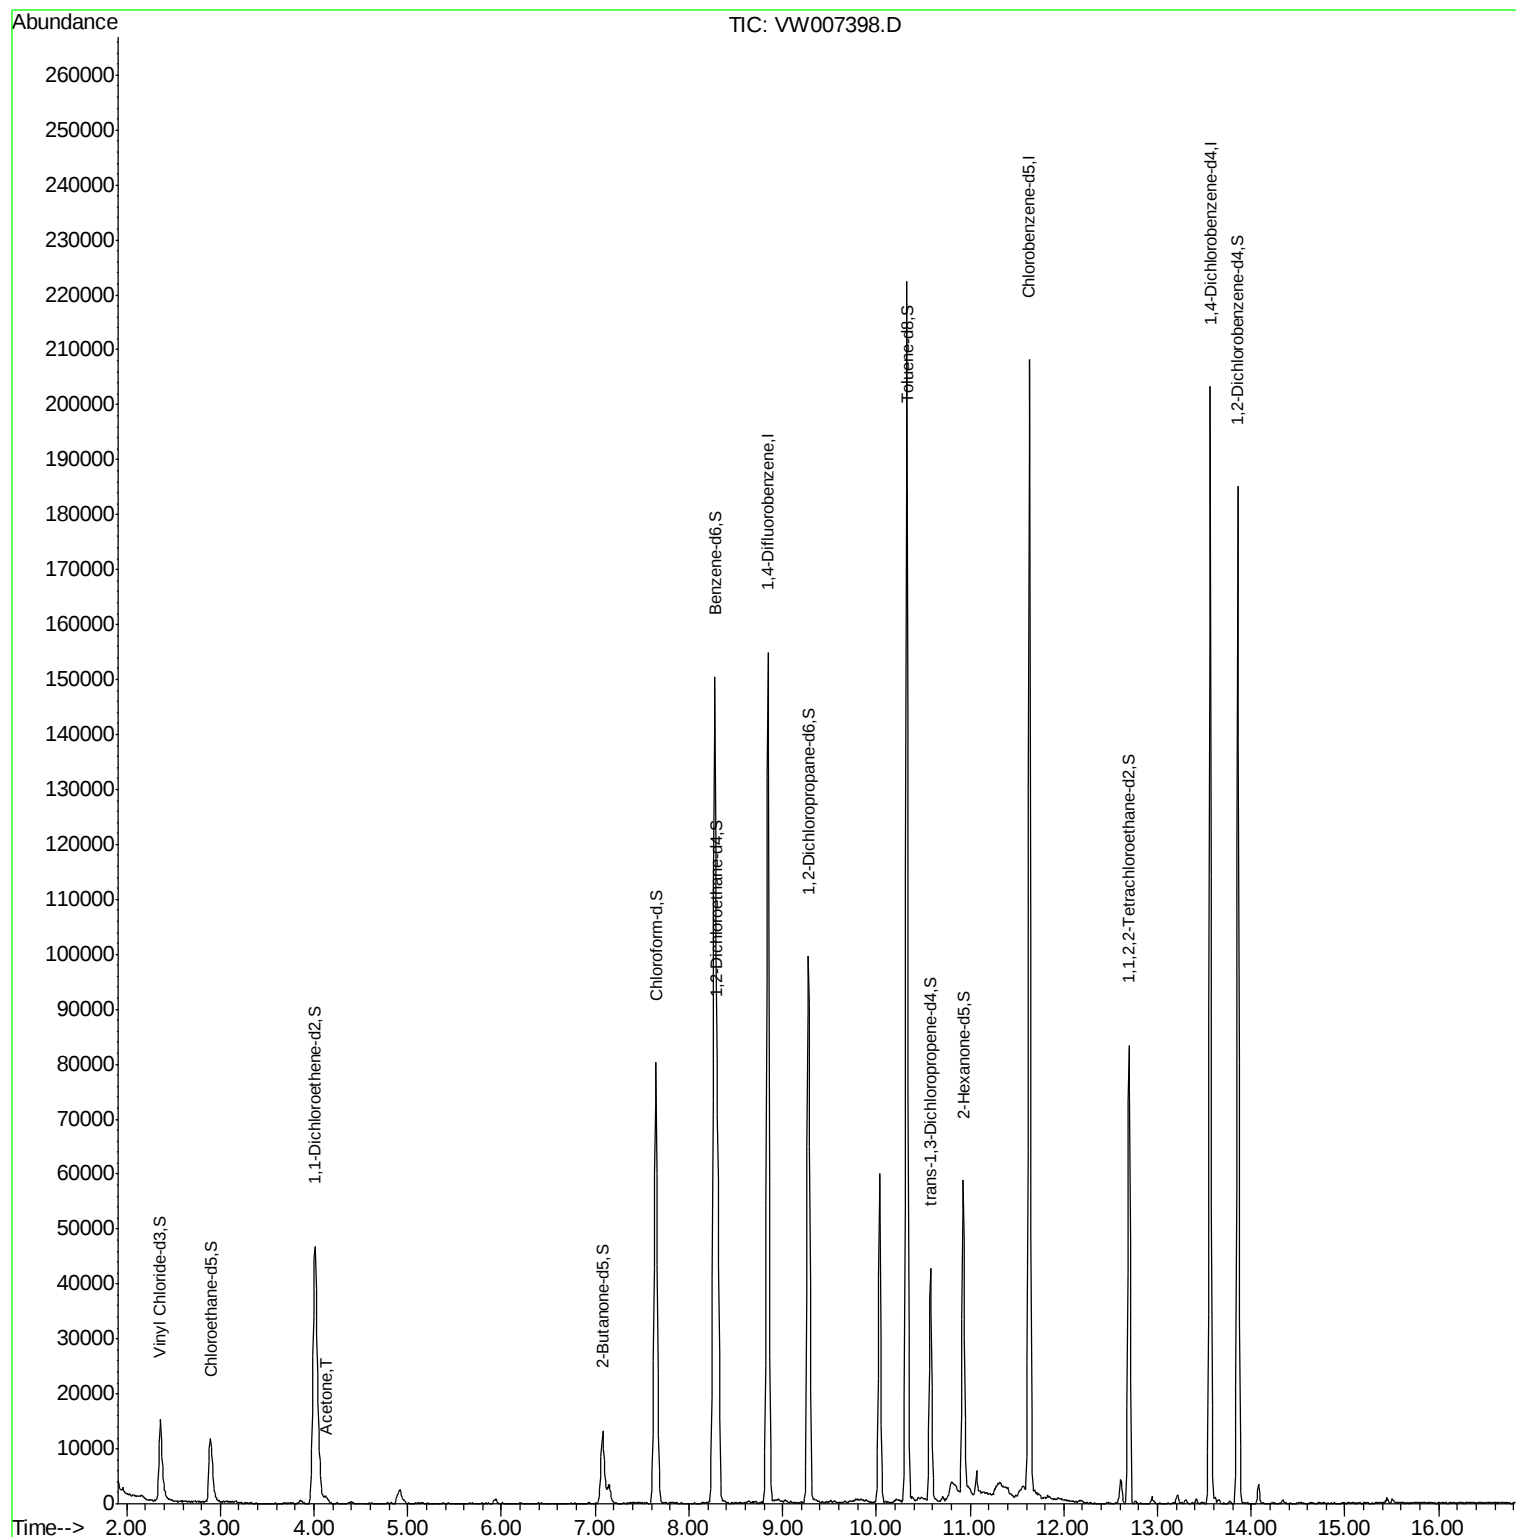

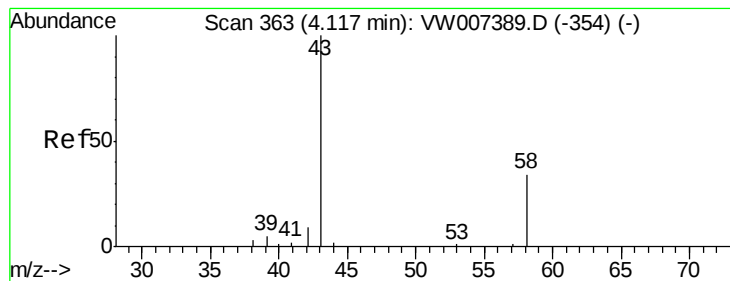

#13

Acetone

Concen: 2.846 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW007398.D

Acq: 11 Dec 2018 15:50

Instrument :
MSVOA_W
ClientSampleId :
F9E26

Tot Ion: 43 Resp: 1751

Ion Ratio Lower Upper

43 100

58 14.9 0.0 59.2

