

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121218\
 Data File : VW007400.D
 Acq On : 11 Dec 2018 16:42
 Operator : SY/AP
 Sample : J6271-13
 Misc : 5.90G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 F9E28

Quant Time: Dec 12 03:42:43 2018
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 11 01:18:15 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	105477	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	89017	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	34817	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.36	65	20070	29.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	116.84%
7) Chloroethane-d5	2.90	69	14750	25.35	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	101.40%
10) 1,1-Dichloroethene-d2	4.01	63	48576	20.50	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	82.00%
20) 2-Butanone-d5	7.08	46	20231	46.72	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	93.44%
24) Chloroform-d	7.65	84	68139	27.39	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	109.56%
26) 1,2-Dichloroethane-d4	8.31	65	42466	29.99	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	119.96%
29) Benzene-d6	8.27	84	130583	27.01	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	108.04%
33) 1,2-Dichloropropane-d6	9.27	67	38405	27.84	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	111.36%
37) Toluene-d8	10.32	98	118474	26.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	104.56%
38) trans-1,3-Dichloropropene-	10.58	79	18022	25.55	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	102.20%
39) 2-Hexanone-d5	10.93	63	16006	48.19	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	96.38%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	34721	27.62	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	110.48%
61) 1,2-Dichlorobenzene-d4	13.86	152	32521	26.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.20%


Target Compounds				Ovalue
16) Methylene chloride	4.92	84	3536	2.075 ug/L 96


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW121218\
Data File : VW007400.D
Acq On : 11 Dec 2018 16:42
Operator : SY/AP
Sample : J6271-13
Misc : 5.90G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
F9E28

Quant Time: Dec 12 03:42:43 2018
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 11 01:18:15 2018
Response via : Initial Calibration

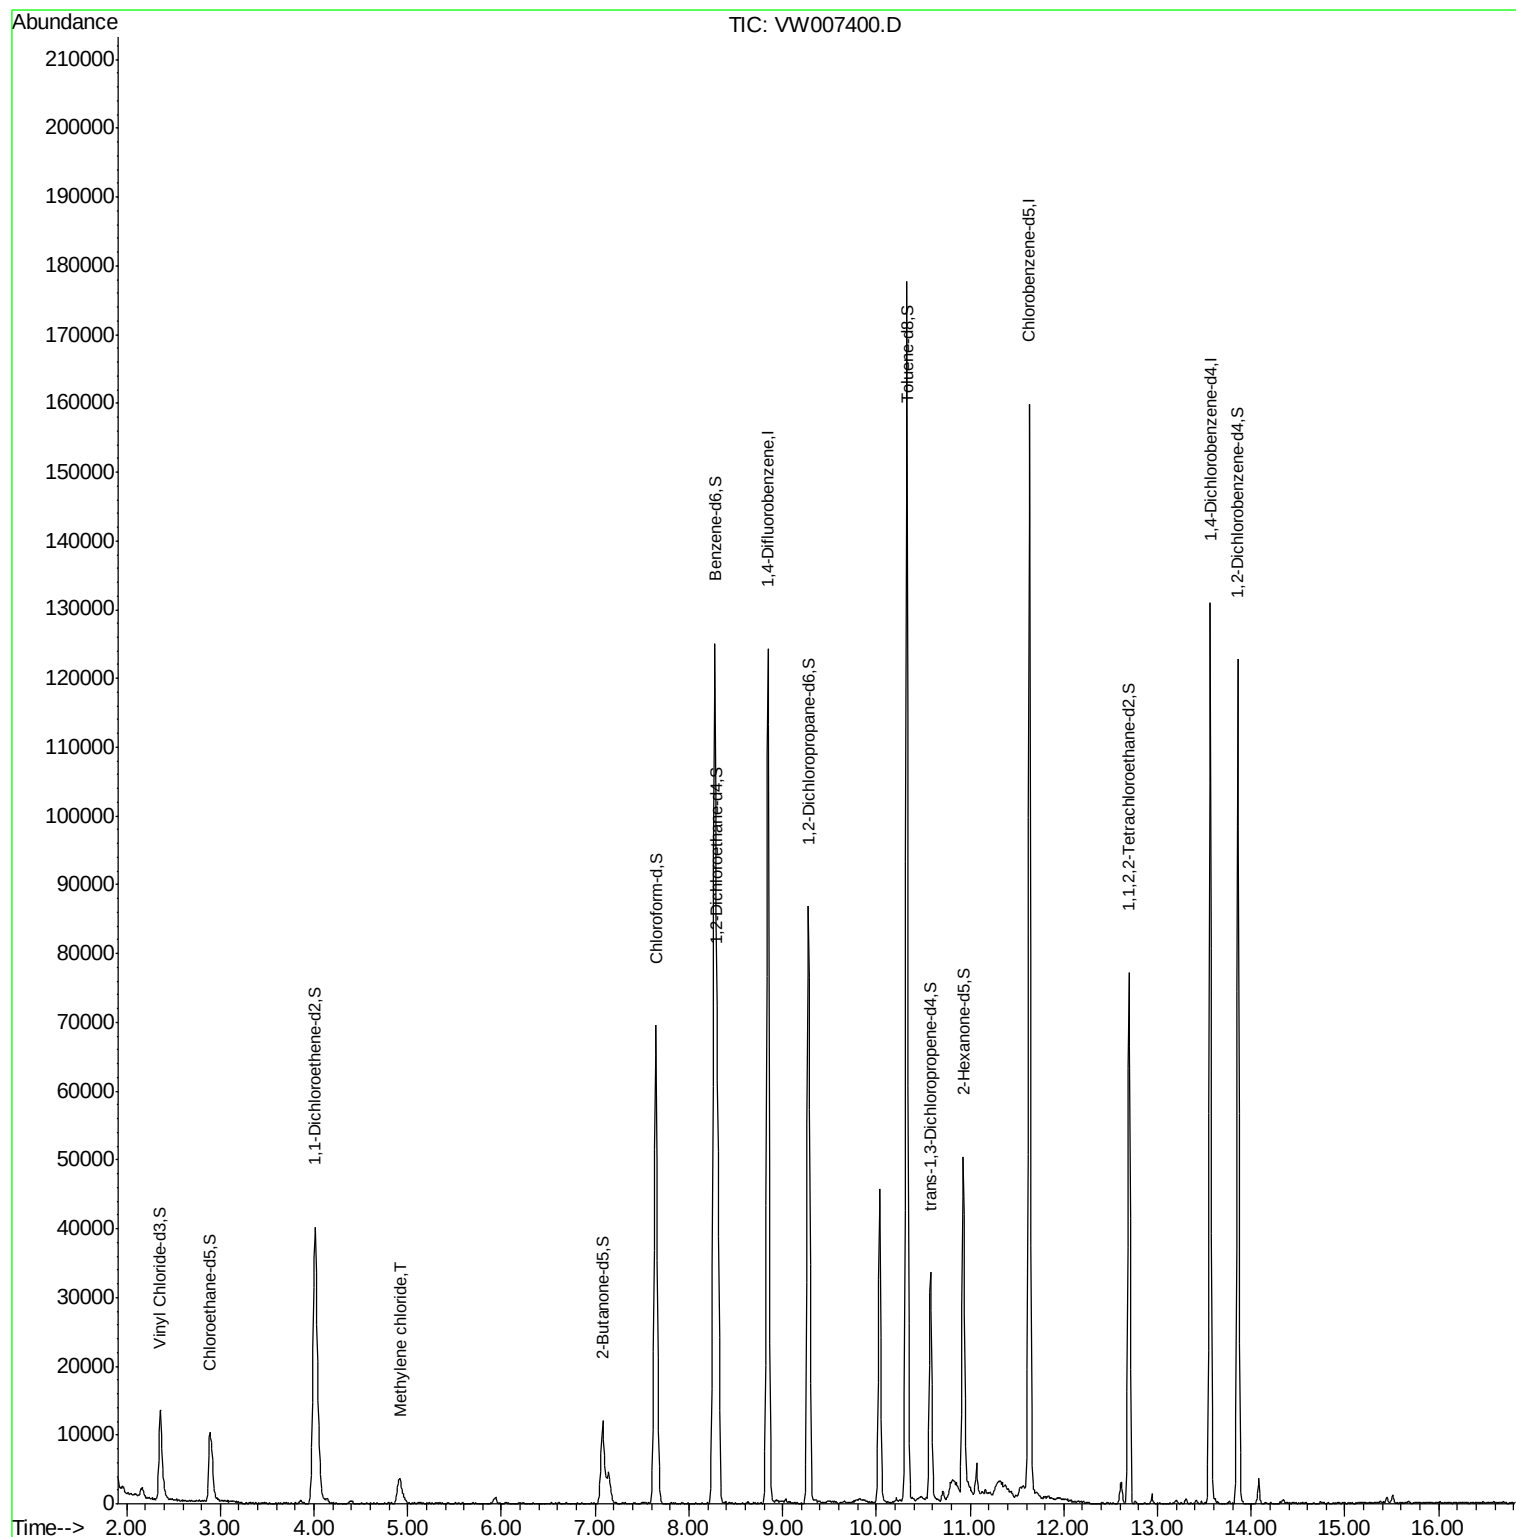

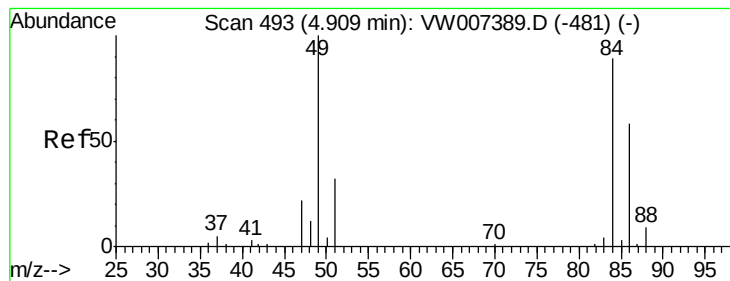

#16
Methylene chloride
Concen: 2.075 ug/L
RT: 4.92 min Scan# 494
Delta R.T. 0.00 min
Lab File: VW007400.D
Acq: 11 Dec 2018 16:42

Instrument :
MSVOA_W
ClientSampleId :
F9E28

Tot Ion	Ratio	Lower	Upper
84	100		
49	117.1	80.8	150.2
86	73.1	45.8	85.2

