


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121218\
 Data File : VW007388.D
 Acq On : 11 Dec 2018 09:30
 Operator : SY/AP
 Sample : BFB85
 Misc : 5.00G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB85

Integration File: LSCINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120718S.M
 Title : VOC Analysis
 Last Update : Tue Dec 11 01:18:15 2018

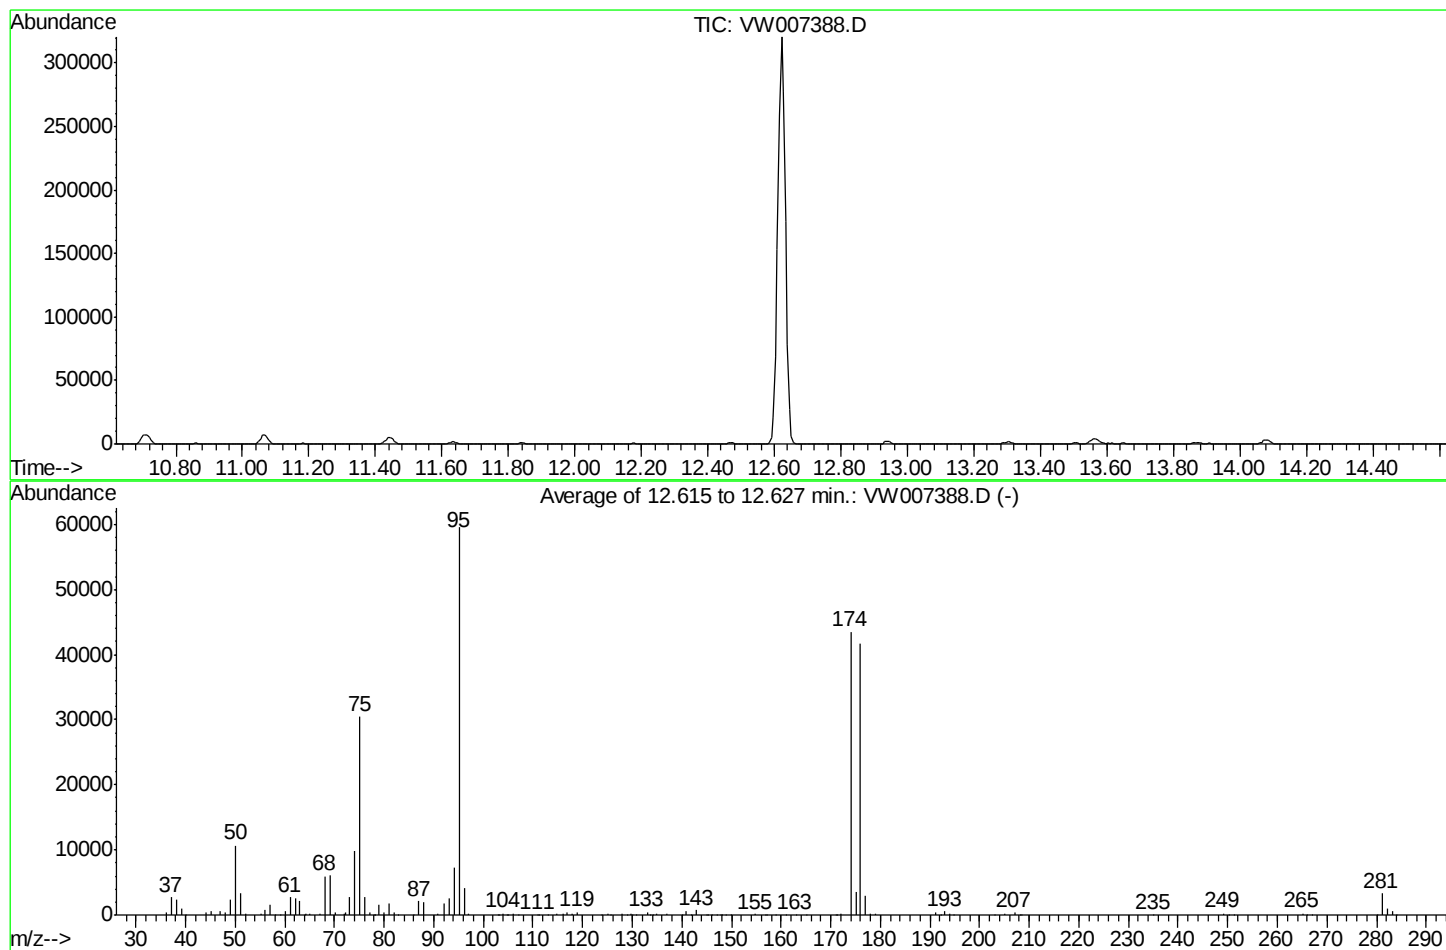

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1750

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.0	10709	PASS
75	95	30	80	51.0	30392	PASS
95	95	100	100	100.0	59554	PASS
96	95	5	9	6.9	4134	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	73.1	43552	PASS
175	174	5	9	8.3	3600	PASS
176	174	95	101	95.6	41642	PASS
177	176	5	9	7.1	2942	PASS

m/z	Abundance
36.10	354.0
37.10	2704.0
38.10	2325.0
39.10	899.0
40.00	67.0
44.10	387.0
45.00	492.0
47.00	532.0
48.00	359.0
49.10	2058.0
50.10	10442.0
51.10	3145.0
52.00	175.0
55.10	159.0
56.00	807.0
57.00	1551.0
58.00	62.0
59.00	107.0
60.10	554.0
61.10	2587.0
62.10	2426.0
63.00	1814.0
64.20	177.0
65.10	91.0
66.90	146.0
68.00	5804.0
69.00	5530.0
70.00	460.0
71.90	199.0
72.10	197.0
73.10	2767.0
74.10	8967.0
75.10	27672.0
76.10	2509.0
77.10	400.0
77.80	198.0
78.90	1534.0
79.90	438.0
81.00	1719.0
81.90	390.0
85.90	72.0
87.00	1868.0
88.00	1860.0
90.80	217.0
92.00	1724.0
93.00	2422.0
94.00	6562.0
95.10	55176.0
96.10	4012.0
97.10	149.0
102.80	68.0
103.20	77.0
104.00	225.0
105.10	90.0
106.00	247.0
111.10	83.0
112.90	57.0
114.90	136.0
116.00	169.0
116.90	327.0
117.90	271.0
119.00	502.0
123.70	72.0
125.00	193.0
125.60	56.0
128.00	256.0
129.00	61.0
129.80	134.0
130.90	101.0
133.10	626.0
134.10	116.0
135.00	133.0
136.90	185.0
140.10	92.0
141.00	483.0
141.90	68.0
143.00	726.0
145.90	80.0
147.00	112.0
147.80	96.0
148.10	98.0
154.80	121.0
156.80	111.0
162.90	102.0
165.10	92.0
170.80	97.0
171.30	79.0
172.20	265.0
174.00	36592.0
175.10	2855.0
176.00	33856.0

Instrument :
MSVOA_W
ClientSampleId :
BFB85

177.00	2488.0
178.00	136.0
179.00	159.0
191.10	422.0
192.20	141.0
193.00	635.0
194.10	154.0
194.90	75.0
205.10	213.0
207.00	371.0
208.10	80.0
235.00	63.0
249.10	292.0
250.20	59.0
251.10	115.0
265.10	307.0
266.00	106.0
267.00	68.0
281.20	3802.0
282.20	1182.0
283.10	771.0
284.00	155.0

Instrument :
MSVOA_W
ClientSampleId :
BFB85

m/z	Abundance
36.10	441.0
37.10	3104.0
38.10	2560.0
39.10	1074.0
40.10	80.0
44.10	397.0
45.10	504.0
47.00	488.0
48.00	405.0
49.10	2921.0
50.10	12171.0
51.10	3902.0
52.10	160.0
55.10	198.0
56.00	986.0
57.00	1942.0
58.00	91.0
60.00	587.0
61.00	2974.0
62.10	3030.0
63.00	2430.0
64.10	324.0
65.00	118.0
67.00	131.0
68.00	6717.0
69.10	6932.0
70.00	567.0
72.00	381.0
73.10	3043.0
74.10	11288.0
75.10	34184.0
76.10	3087.0
77.00	410.0
78.10	221.0
78.90	2045.0
80.00	540.0
81.00	1830.0
82.00	379.0
82.90	53.0
85.90	87.0
87.00	2204.0
88.00	2496.0
90.90	258.0
92.10	1932.0
93.00	2772.0
94.10	8481.0
95.10	66392.0
96.10	4670.0
97.10	83.0
102.90	143.0
104.00	369.0
105.10	111.0
106.00	287.0
107.10	67.0
110.80	68.0
111.10	74.0
114.80	137.0
115.90	188.0
117.00	490.0
117.80	299.0
119.00	476.0
125.10	199.0
125.70	86.0
128.00	186.0
129.00	66.0
130.10	267.0
130.80	62.0
133.00	502.0
133.70	132.0
135.00	173.0
137.00	133.0
140.10	69.0
141.00	717.0
141.90	85.0
142.90	807.0
144.90	82.0
146.00	95.0
147.00	114.0
147.80	162.0
148.90	53.0
149.90	58.0
154.90	186.0
157.10	134.0
159.00	110.0
161.00	84.0
162.90	54.0
170.90	105.0
171.30	111.0
172.00	263.0
174.00	48224.0
175.00	4012.0

Instrument :
MSVOA_W
ClientSampleId :
BFB85

176.00	46896.0
177.00	3165.0
178.00	176.0
179.10	108.0
191.10	411.0
192.10	119.0
193.00	605.0
194.00	176.0
194.80	53.0
202.90	59.0
205.00	92.0
207.10	367.0
208.30	86.0
249.20	259.0
250.10	77.0
251.10	87.0
265.10	309.0
265.90	60.0
267.10	92.0
281.10	3596.0
282.10	1001.0
283.10	472.0
284.10	85.0

Instrument :
MSVOA_W
ClientSampleId :
BFB85

m/z	Abundance
36.00	425.0
37.10	2363.0
38.10	1954.0
39.10	834.0
40.00	74.0
44.00	361.0
45.10	546.0
47.10	647.0
48.10	328.0
49.00	2072.0
50.10	9514.0
51.10	3009.0
52.00	111.0
55.10	190.0
56.00	855.0
57.10	1353.0
60.00	582.0
61.00	2631.0
62.10	2419.0
63.10	1996.0
63.90	251.0
64.90	77.0
65.10	81.0
67.00	200.0
68.10	5420.0
69.10	5761.0
70.10	399.0
71.90	271.0
72.20	359.0
73.10	2453.0
74.10	9249.0
75.10	29320.0
76.10	2420.0
77.10	292.0
79.00	1454.0
80.00	446.0
80.90	1539.0
81.90	425.0
87.00	2313.0
88.00	1812.0
91.00	219.0
92.00	1756.0
93.00	2631.0
94.10	6923.0
95.10	57096.0
96.10	3722.0
96.90	120.0
102.80	75.0
104.00	266.0
104.70	81.0
106.00	303.0
114.90	88.0
116.00	251.0
117.00	422.0
118.00	316.0
118.90	358.0
125.10	76.0
127.90	211.0
128.90	69.0
129.90	211.0
130.90	84.0
133.10	147.0
133.60	96.0
134.80	109.0
136.90	88.0
140.90	627.0
141.90	100.0
143.00	729.0
144.80	55.0
145.20	67.0
146.00	58.0
148.10	143.0
149.90	104.0
154.80	195.0
156.80	132.0
159.00	111.0
160.90	109.0
171.00	67.0
174.00	45840.0
175.10	3933.0
176.00	44176.0
177.00	3175.0
178.00	79.0
178.90	72.0
191.10	157.0
193.00	294.0
193.90	66.0
205.00	83.0
207.10	255.0
249.20	173.0
250.00	51.0

Instrument :
MSVOA_W
ClientSampleId :
BFB85

251.10	84.0
265.20	254.0
280.00	107.0
281.20	2380.0
282.10	625.0
283.20	438.0

Instrument :
MSVOA_W
ClientSampleId :
BFB85

m/z Abundance

Instrument :
MSVOA_W
ClientSampleId :
BFB85