


Data Path : Z:\voasrv\HPCHEM1\MSVOA W\Data\VW121318\
Data File : VW007409.D
Acq On : 11 Dec 2018 22:19
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA W/SOIL
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W121118S.M
Title : SW846 8260
Last Update : Tue Dec 11 02:58:16 2018

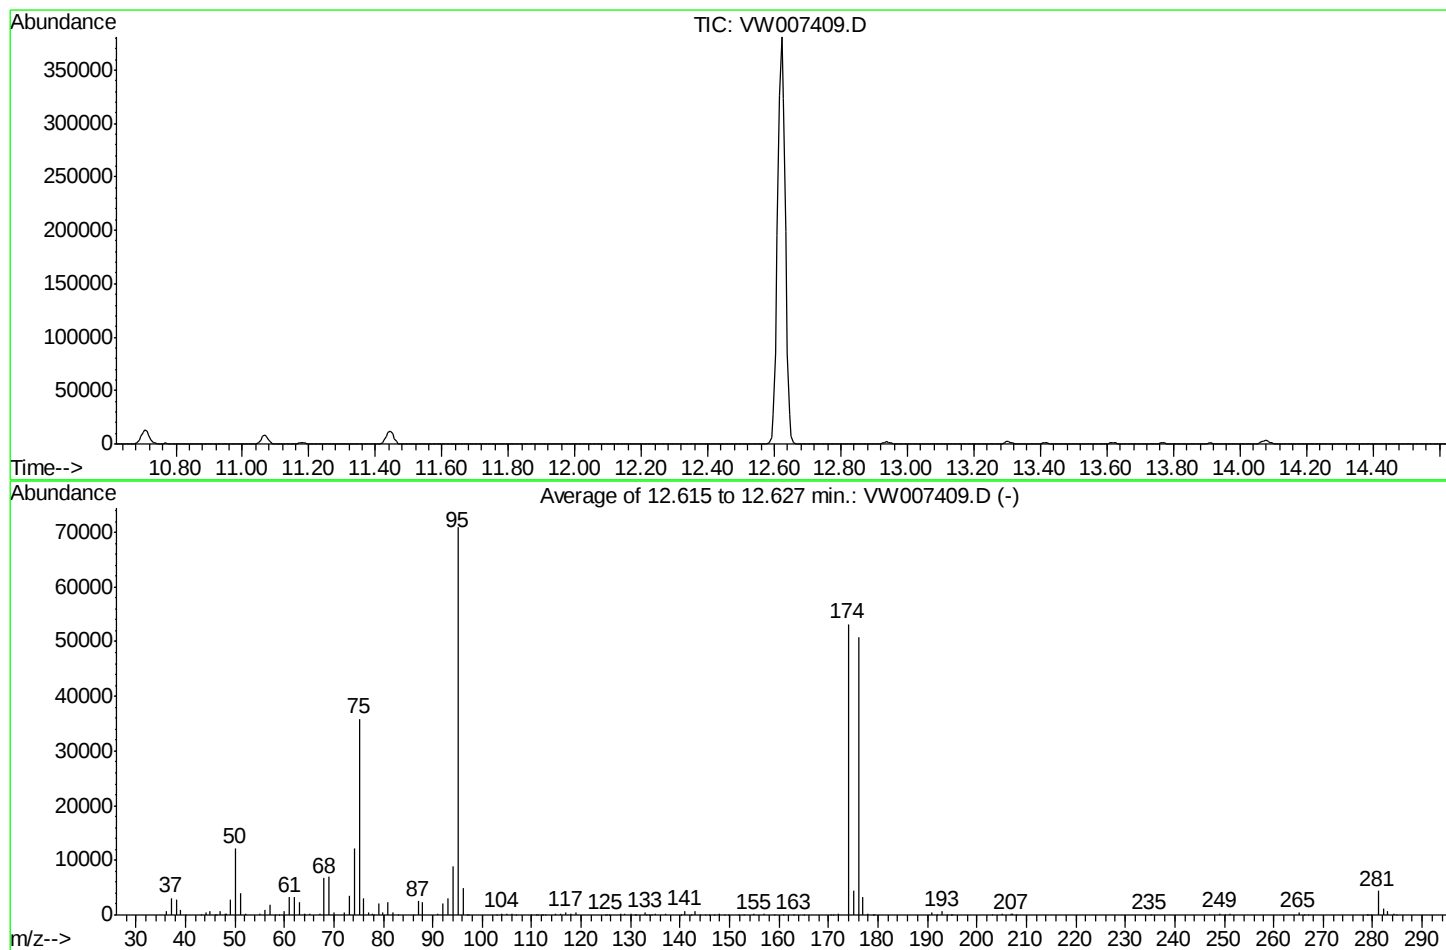

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	12150	PASS
75	95	30	60	50.5	35824	PASS
95	95	100	100	100.0	70912	PASS
96	95	5	9	6.9	4887	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.0	53154	PASS
175	174	5	9	8.2	4382	PASS
176	174	95	101	95.4	50725	PASS
177	176	5	9	6.7	3392	PASS