




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121323\
 Data File : VW027607.D
 Acq On : 13 Dec 2023 20:12
 Operator : SY/MD
 Sample : 05799-02
 Misc : 4.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQZ1

Manual IntegrationsAPPROVED

Quant Time: Dec 14 00:21:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 13 04:25:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/14/2023
 Supervised By :Mahesh Dadoda 12/15/2023

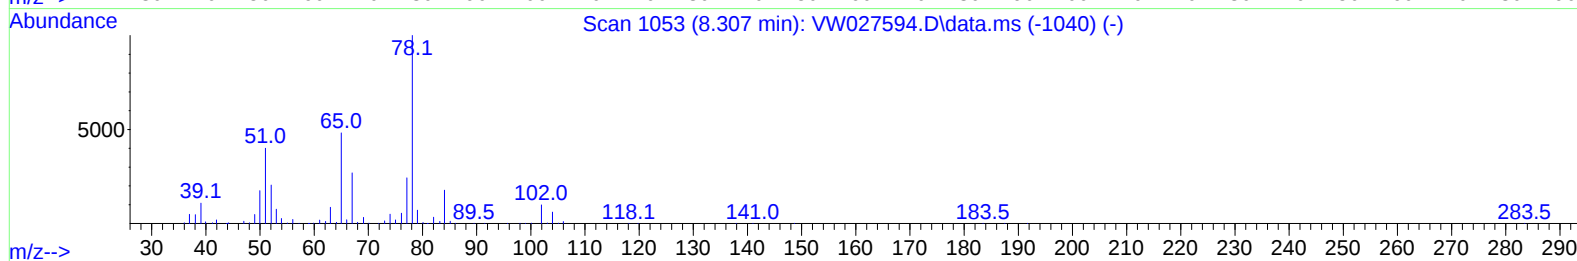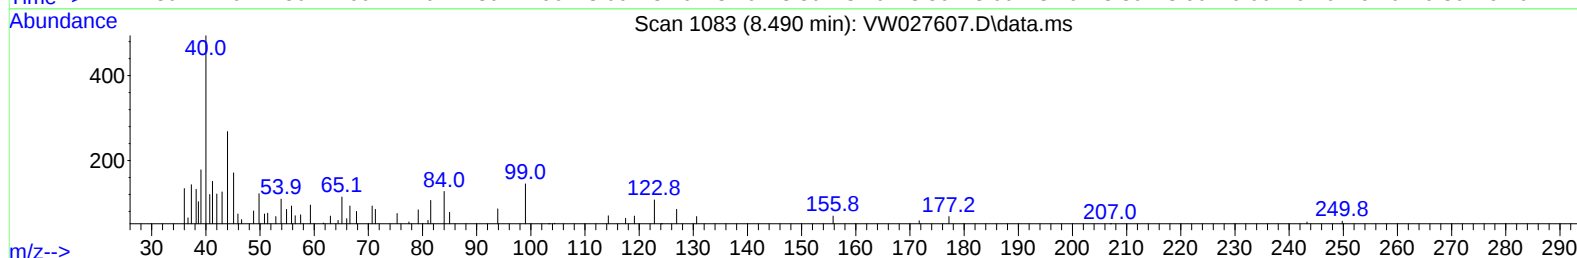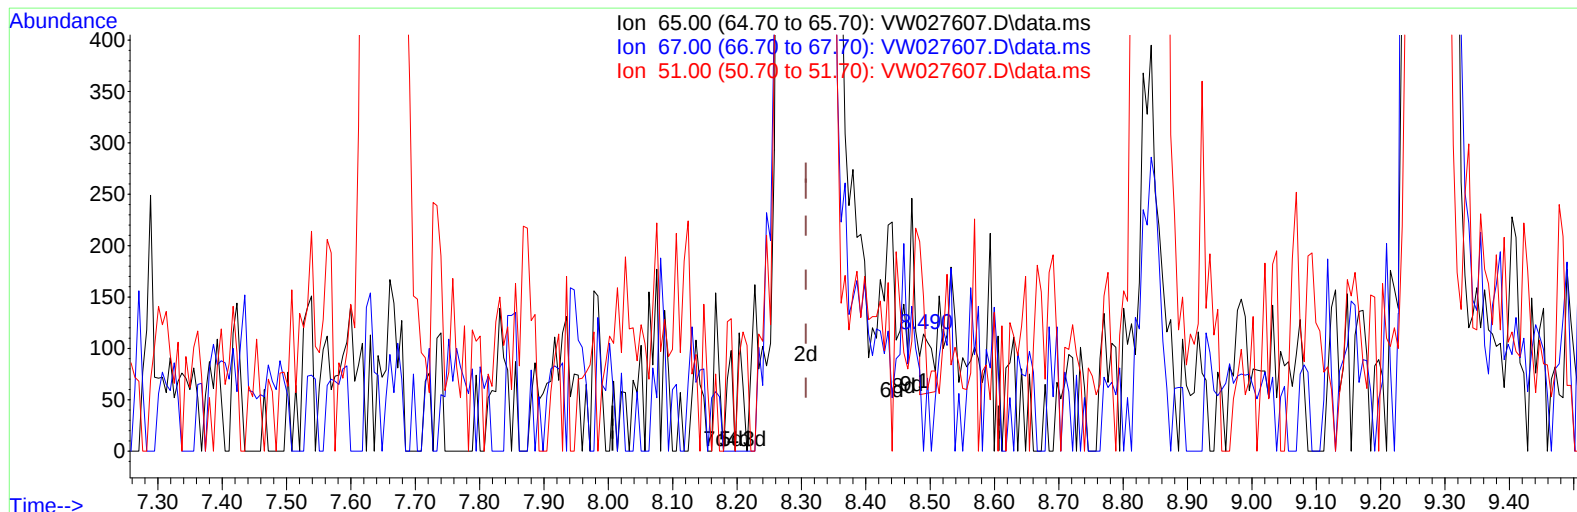

TIC: VW027607.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.490min (+ 0.183) 0.01 ug/L

response 63

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.20	41.27
51.00	135.30	123.81
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121323\
 Data File : VW027607.D
 Acq On : 13 Dec 2023 20:12
 Operator : SY/MD
 Sample : 05799-02
 Misc : 4.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQZ1

Manual IntegrationsAPPROVED

Quant Time: Dec 14 00:21:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 13 04:25:58 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/14/2023
 Supervised By :Mahesh Dadoda 12/15/2023

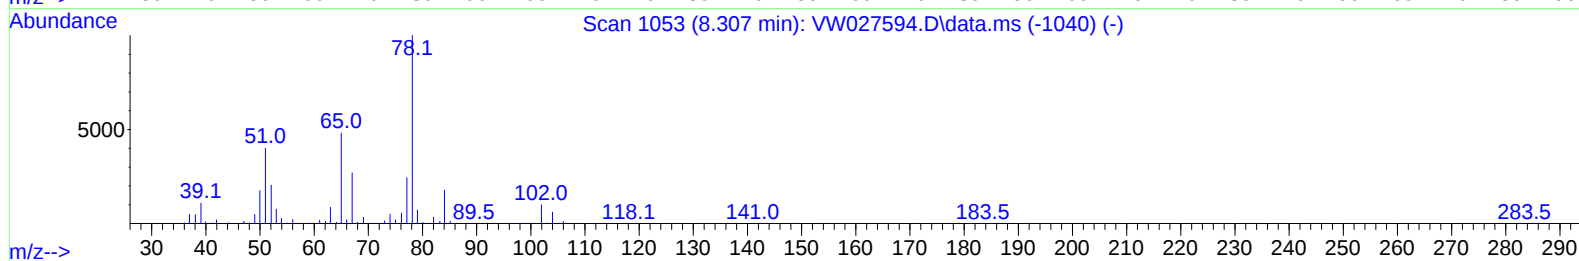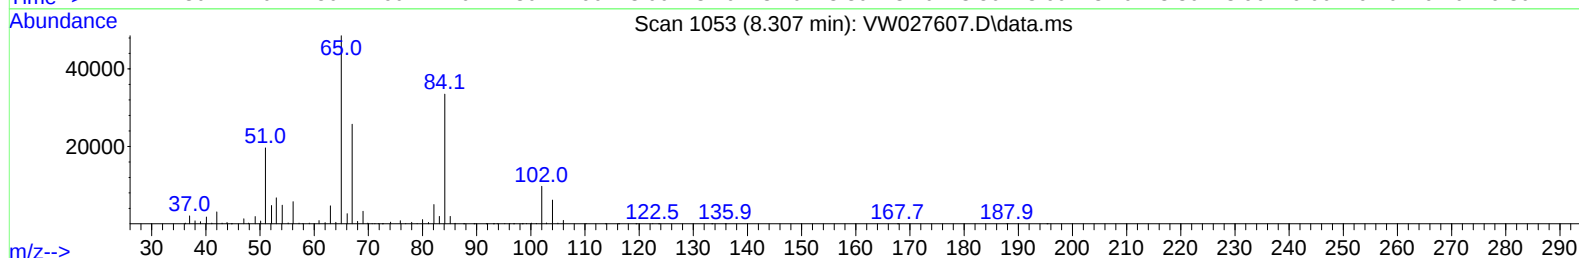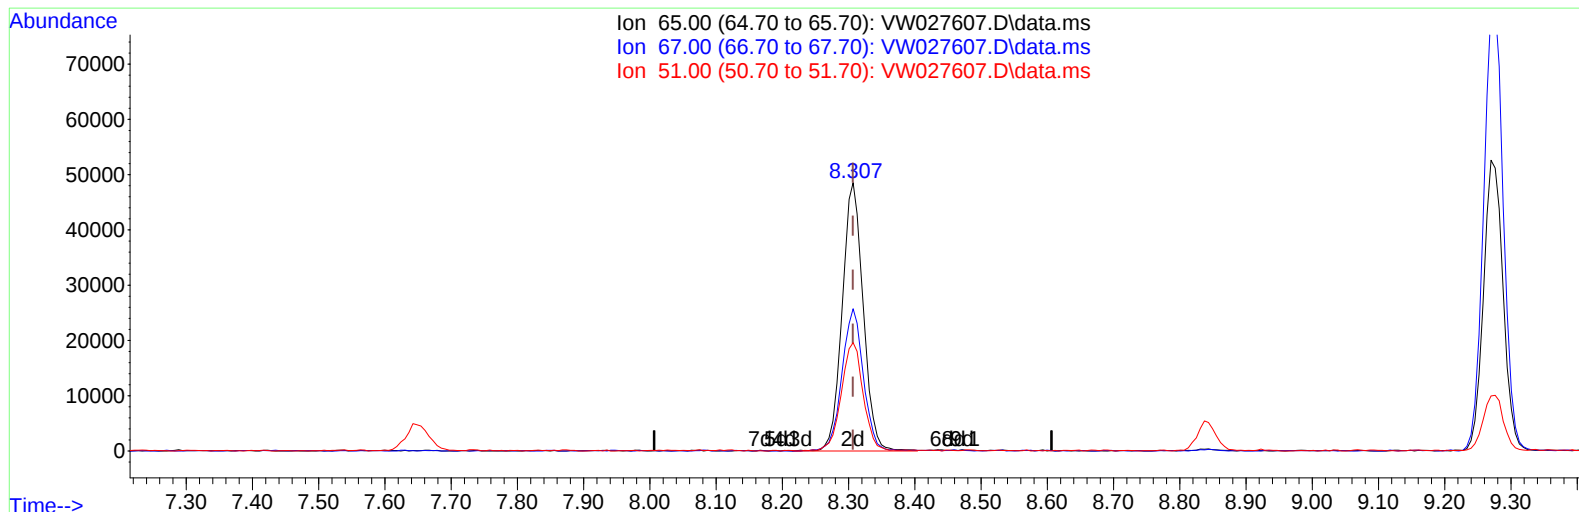

TIC: VW027607.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 14.96 ug/L m

response 106804

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.20	0.02#
51.00	135.30	0.07#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121323\
 Data File : VW027607.D
 Acq On : 13 Dec 2023 20:12
 Operator : SY/MD
 Sample : 05799-02
 Misc : 4.27g/10mL/MSVOA_W/SOIL
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BGQZ1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/14/2023
 Supervised By :Mahesh Dadoda 12/15/2023

Quant Time: Dec 14 00:21:02 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 13 04:25:58 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	467823	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	358431	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	143522	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	228376	24.258	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	97.040%		
7) Chloroethane-d5	2.899	69	155829	22.833	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	91.320%		
11) 1,1-Dichloroethene-d2	4.027	65	94560	23.738	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	94.960%		
21) 2-Butanone-d5	7.075	46	36998	14.998	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	30.000%		
24) Chloroform-d	7.648	84	286194	20.495	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	81.960%		
26) 1,2-Dichloroethane-d4	8.307	65	106804m	14.957	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	59.840%#		
32) Benzene-d6	8.276	84	651804	25.819	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	103.280%		
36) 1,2-Dichloropropane-d6	9.276	67	167625	22.523	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	90.080%		
41) Toluene-d8	10.325	98	582090	26.353	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	105.400%		
43) trans-1,3-Dichloroprop...	10.575	79	47281	16.429	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	65.720%		
47) 2-Hexanone-d5	10.922	63	25256	18.214	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	36.420%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	69381	11.334	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	45.320%		
66) 1,2-Dichlorobenzene-d4	13.849	152	106750	21.219	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	84.880%		
Target Compounds						Qvalue
46) Tetrachloroethene	10.861	164	121303	25.181	ug/L	93

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121323\
Data File : VW027607.D
Acq On : 13 Dec 2023 20:12
Operator : SY/MD
Sample : 05799-02
Misc : 4.27g/10mL/MSVOA_W/SOIL
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BGQZ1

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/14/2023
Supervised By :Mahesh Dadoda 12/15/2023

Quant Time: Dec 14 00:21:02 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 13 04:25:58 2023
Response via : Initial Calibration

