

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
 Data File : VW031234.D
 Acq On : 13 Dec 2024 13:49
 Operator : SY/MD
 Sample : VW1213SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 14 00:45:40 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 14 00:44:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	781523	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	674188	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	330235	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.357	65	261986	22.280	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.120%
7) Chloroethane-d5	2.893	69	182374	20.966	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.880%
11) 1,1-Dichloroethene-d2	4.021	65	124363	22.296	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	89.200%
21) 2-Butanone-d5	7.100	46	102705	46.378	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	92.760%
24) Chloroform-d	7.648	84	462146	21.582	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	86.320%
26) 1,2-Dichloroethane-d4	8.301	65	251952	23.429	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	93.720%
32) Benzene-d6	8.270	84	979616	22.670	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.680%
36) 1,2-Dichloropropane-d6	9.270	67	280167	22.246	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	89.000%
41) Toluene-d8	10.319	98	903377	22.472	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	89.880%
43) trans-1,3-Dichloroprop...	10.575	79	131507	22.646	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.600%
47) 2-Hexanone-d5	10.922	63	82776	48.875	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	97.740%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	186467	23.582	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	94.320%
66) 1,2-Dichlorobenzene-d4	13.848	152	267261	21.800	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	87.200%
Target Compounds				Qvalue		
39) cis-1,3-Dichloropropene	10.032	75	10321	0.588	ug/L #	59


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
Data File : VW031234.D
Acq On : 13 Dec 2024 13:49
Operator : SY/MD
Sample : VW1213SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 14 00:45:40 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 14 00:44:31 2024
Response via : Initial Calibration

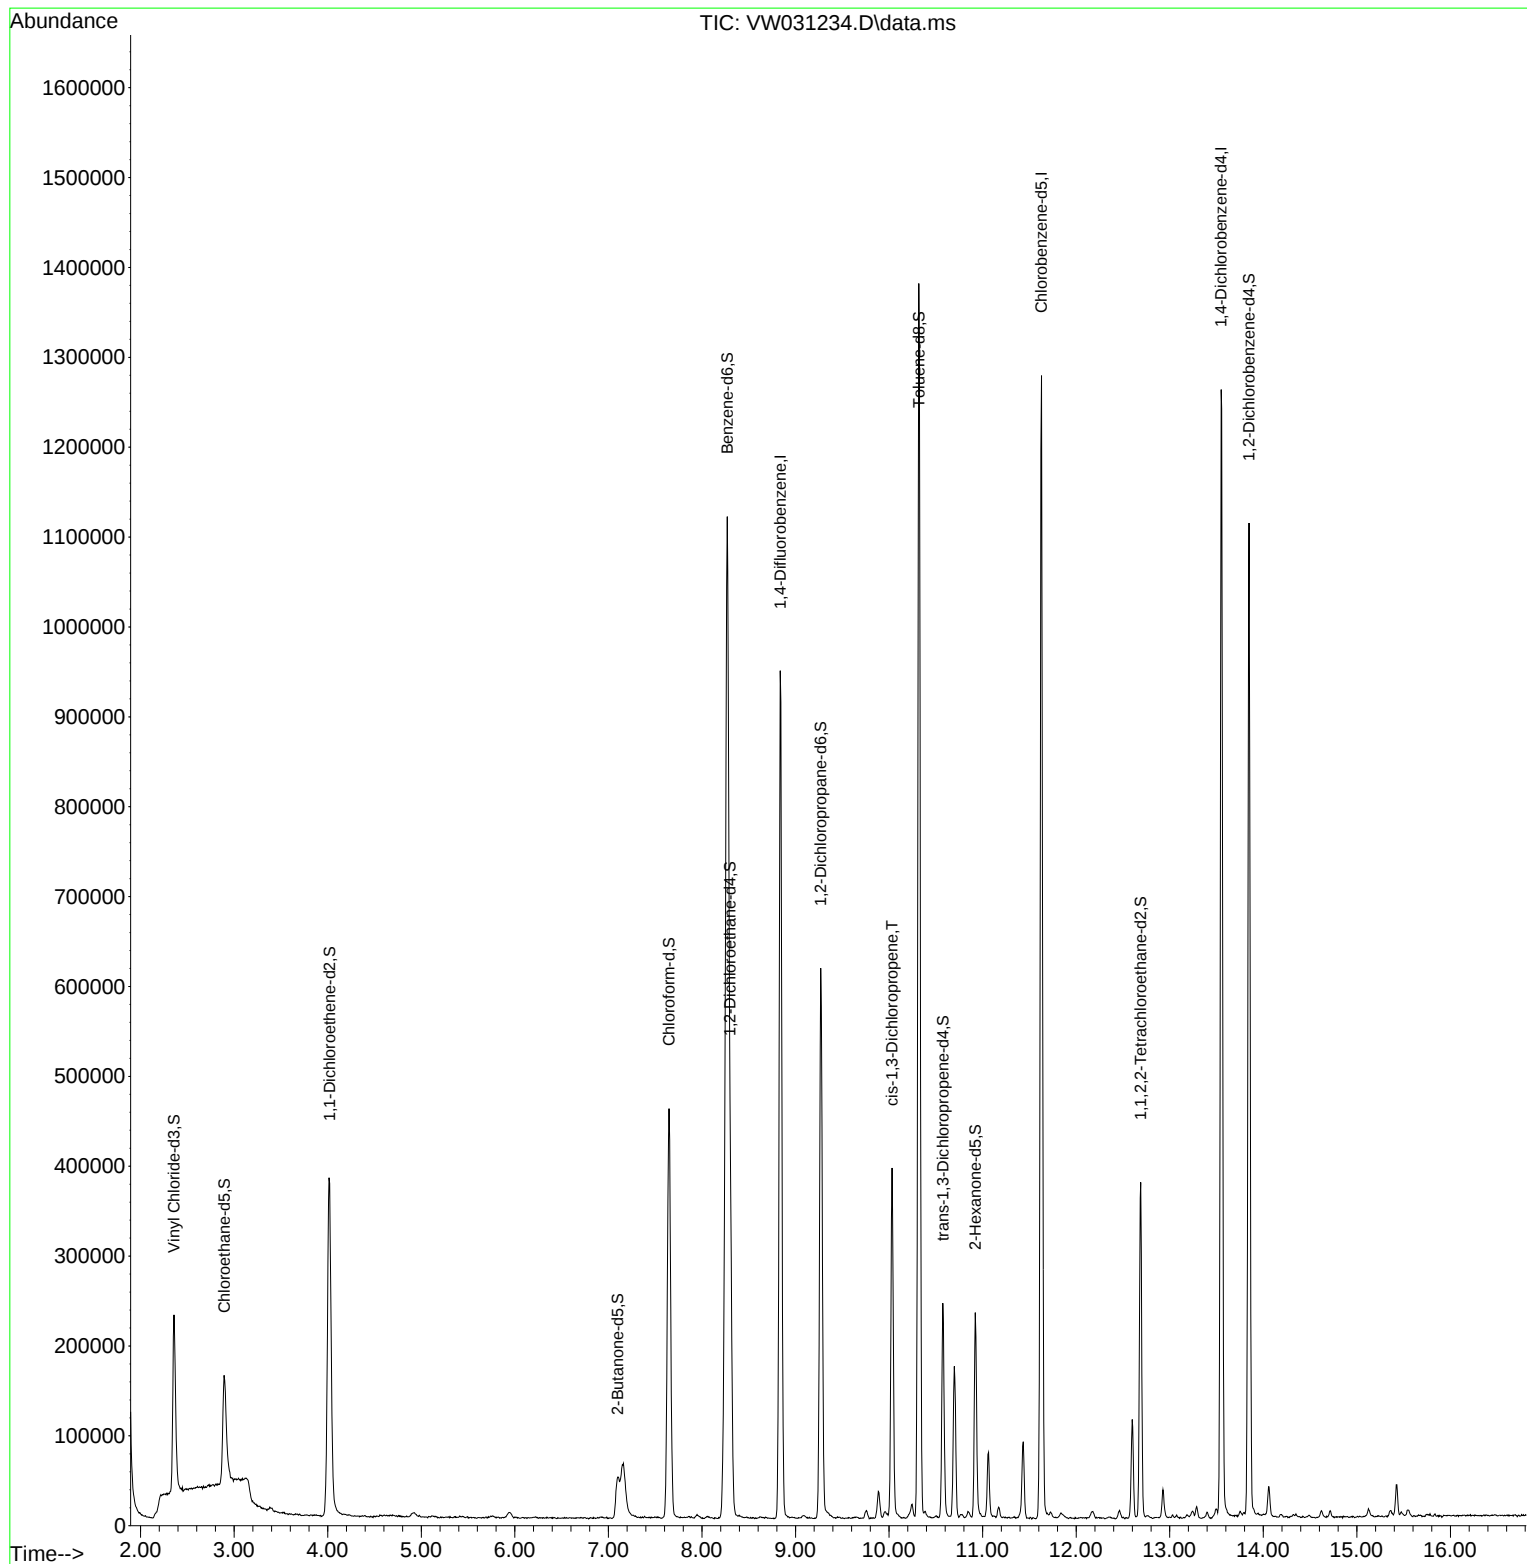

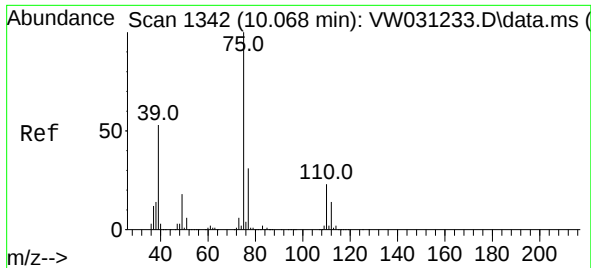

#39
 cis-1,3-Dichloropropene
 Concen: 0.588 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.036 min
 Lab File: VW031234.D
 Acq: 13 Dec 2024 13:49

Instrument :
 MSVOA_W
 ClientSampleId :

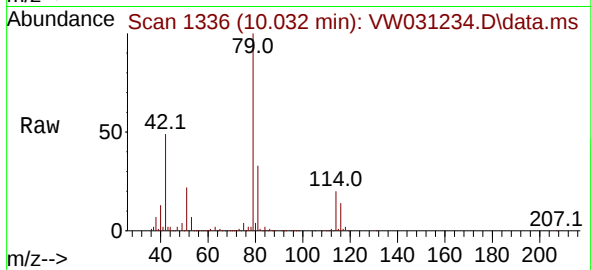

Tgt Ion: 75 Resp: 10321
 Ion Ratio Lower Upper
 75 100
 77 53.6 21.8 40.4#

