

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
 Data File : VW031235.D
 Acq On : 13 Dec 2024 14:34
 Operator : SY/MD
 Sample : P5066-10
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 14 00:45:53 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 14 00:44:31 2024
 Response via : Initial Calibration

Compound		R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards							
1) 1,4-Difluorobenzene		8.837	114	765082	25.000	ug/L	0.00
28) Chlorobenzene-d5		11.623	117	658838	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4		13.550	152	311223	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3		2.357	65	288997	25.105	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	100.400%	
7) Chloroethane-d5		2.893	69	205266	24.105	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	96.440%	
11) 1,1-Dichloroethene-d2		4.015	65	137595	25.198	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	100.800%	
21) 2-Butanone-d5		7.094	46	111115	51.254	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	102.500%	
24) Chloroform-d		7.642	84	502456	23.969	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	95.880%	
26) 1,2-Dichloroethane-d4		8.301	65	274164	26.042	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.160%	
32) Benzene-d6		8.270	84	1057962	25.054	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	100.200%	
36) 1,2-Dichloropropane-d6		9.270	67	304375	24.732	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	98.920%	
41) Toluene-d8		10.319	98	967892	24.638	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	98.560%	
43) trans-1,3-Dichloroprop...		10.575	79	143456	25.280	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	101.120%	
47) 2-Hexanone-d5		10.922	63	88820	53.665	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	107.320%	
56) 1,1,2,2-Tetrachloroeth...		12.690	84	201479	26.074	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	104.280%	
66) 1,2-Dichlorobenzene-d4		13.842	152	298699	25.853	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	103.400%	
Target Compounds							
39) cis-1,3-Dichloropropene		10.032	75	11331	0.660	ug/L	Qvalue # 69


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
Data File : VW031235.D
Acq On : 13 Dec 2024 14:34
Operator : SY/MD
Sample : P5066-10
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :

Quant Time: Dec 14 00:45:53 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 14 00:44:31 2024
Response via : Initial Calibration

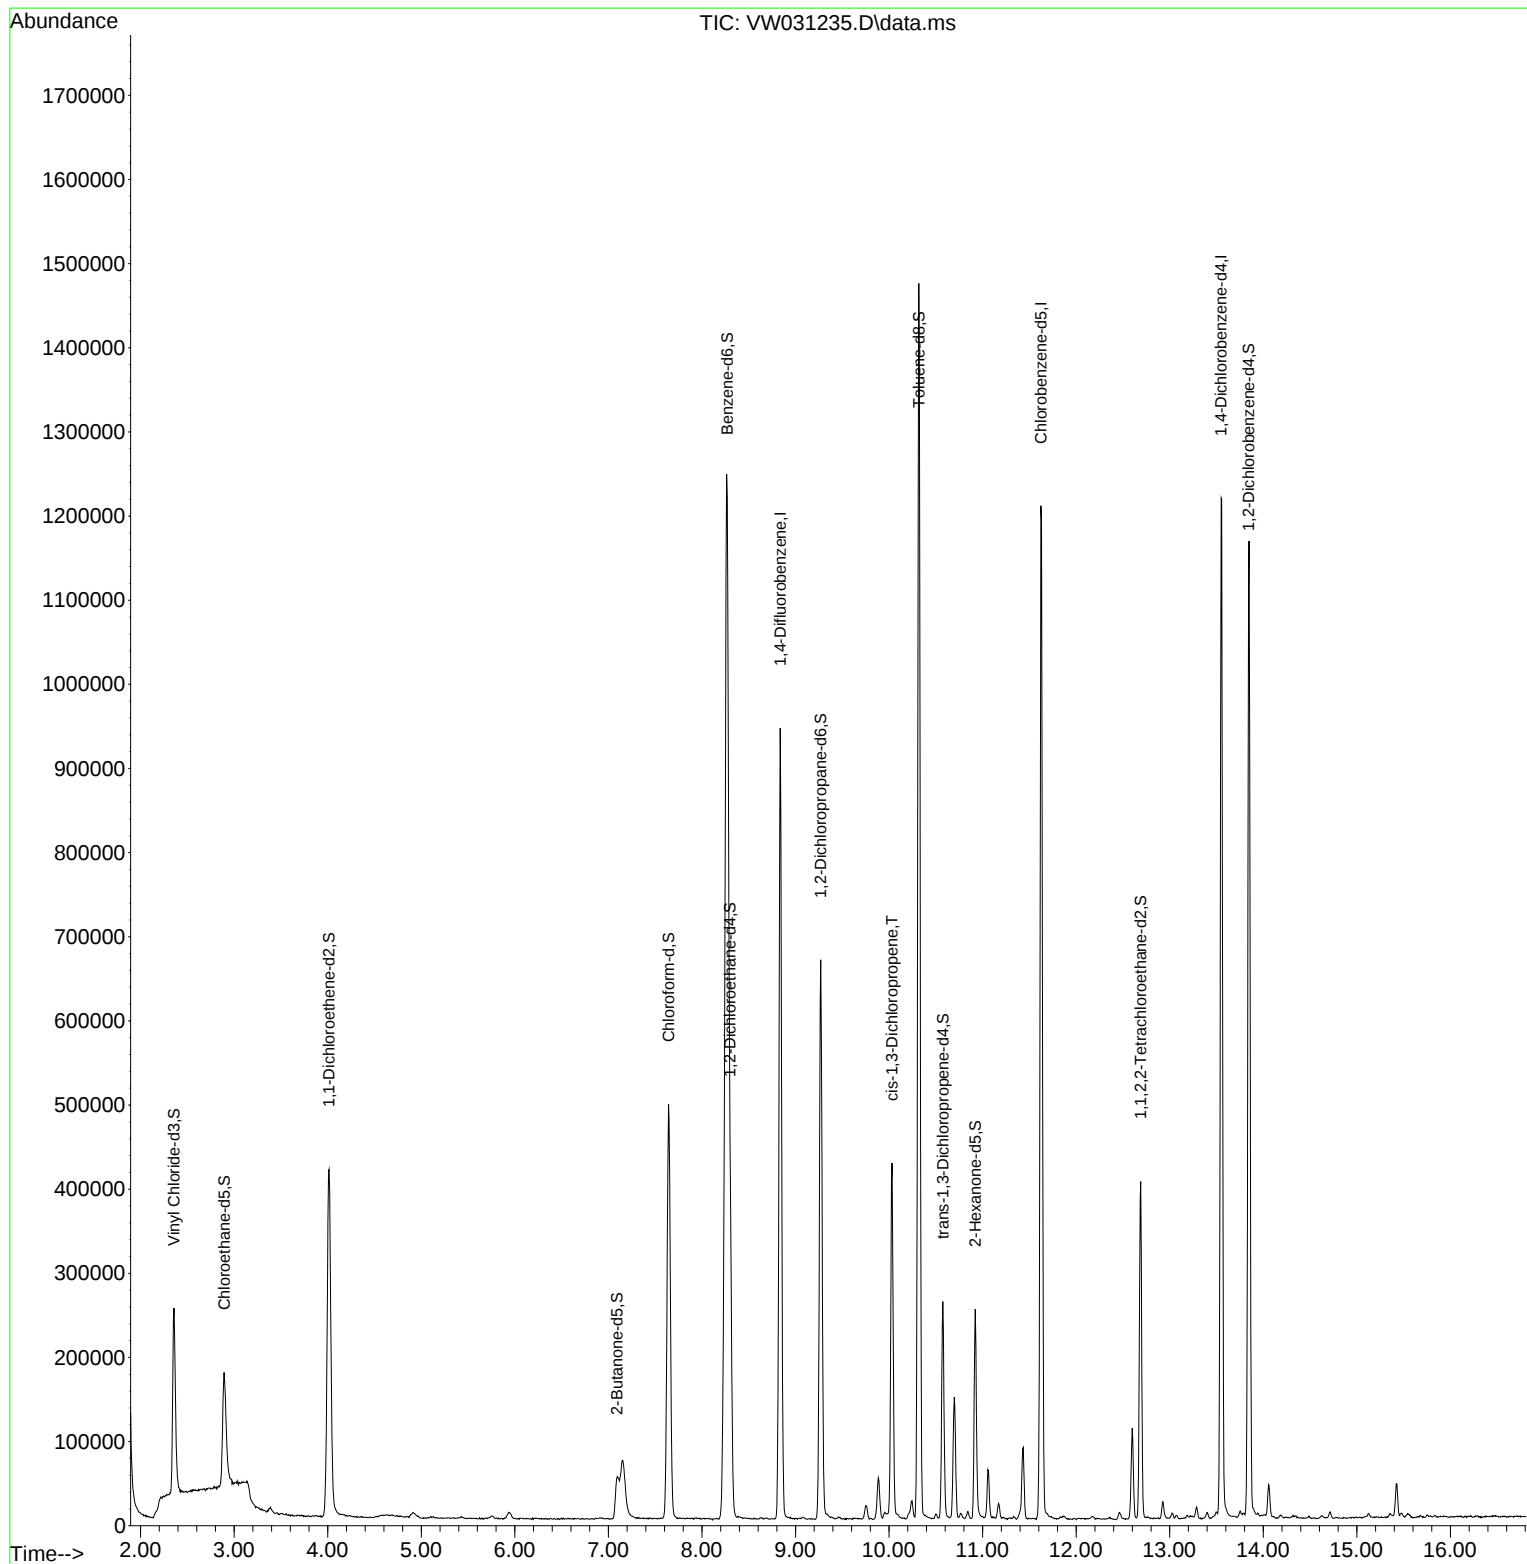

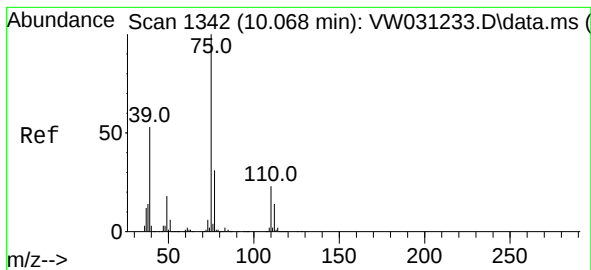

#39
 cis-1,3-Dichloropropene
 Concen: 0.660 ug/L
 RT: 10.032 min Scan# 14
 Delta R.T. -0.036 min
 Lab File: VW031235.D
 Acq: 13 Dec 2024 14:34

Instrument :
 MSVOA_W
 ClientSampleId :

Tgt Ion: 75 Resp: 11331
 Ion Ratio Lower Upper
 75 100
 77 48.0 21.8 40.4#

