

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
 Data File : VW031247.D
 Acq On : 13 Dec 2024 19:20
 Operator : SY/MD
 Sample : P5155-13
 Misc : 4.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 14 00:48:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 14 00:44:31 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	1057204	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	711867	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	212907	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	363382	22.844	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	91.360%
7) Chloroethane-d5	2.899	69	262539	22.312	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.240%
11) 1,1-Dichloroethene-d2	4.015	65	163589	21.681	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	86.720%
21) 2-Butanone-d5	7.100	46	93834	31.323	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	62.640%
24) Chloroform-d	7.648	84	604520	20.870	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	83.480%
26) 1,2-Dichloroethane-d4	8.307	65	319974	21.995	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	88.000%
32) Benzene-d6	8.276	84	1182934	25.926	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	103.720%
36) 1,2-Dichloropropane-d6	9.270	67	354038	26.624	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	106.480%
41) Toluene-d8	10.319	98	976469	23.005	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	92.000%
43) trans-1,3-Dichloroprop...	10.575	79	119999	19.571	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	78.280%
47) 2-Hexanone-d5	10.922	63	74717	41.781	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	83.560%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	204792	24.528	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	98.120%
66) 1,2-Dichlorobenzene-d4	13.848	152	164276	20.784	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	83.120%
Target Compounds						
					Qvalue	
48) 2-Hexanone	10.922	43	9509	1.920	ug/L	# 70


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSV0A_W\Data\VW121324\
Data File : VW031247.D
Acq On : 13 Dec 2024 19:20
Operator : SY/MD
Sample : P5155-13
Misc : 4.07g/10mL/MSV0A_W/SOIL/A
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSV0A_W
ClientSampleId :


Quant Time: Dec 14 00:48:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSV0A_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 14 00:44:31 2024
Response via : Initial Calibration

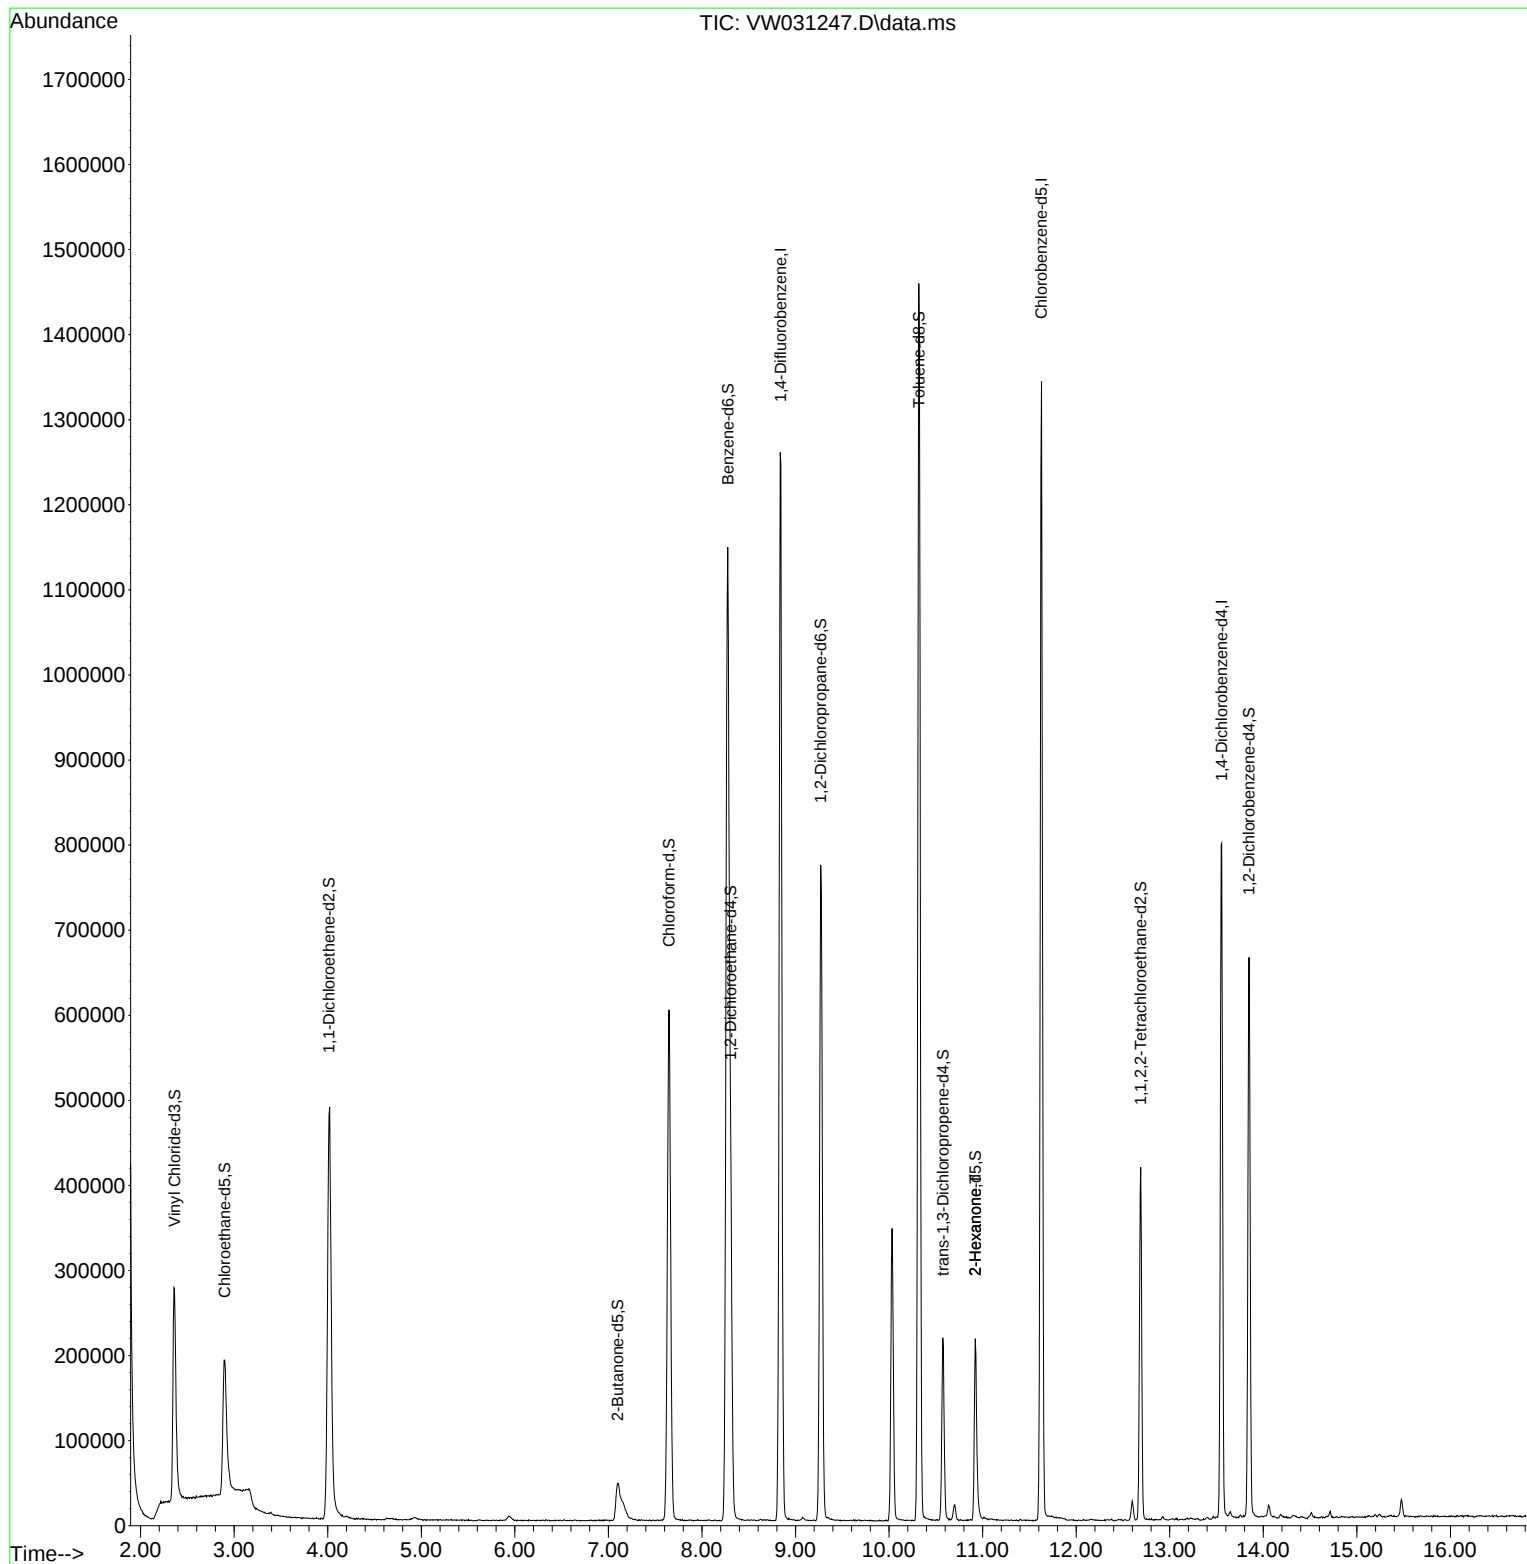

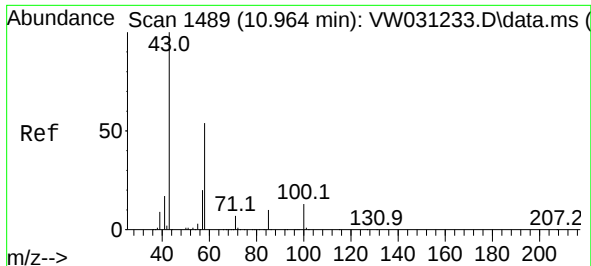

#48
 2-Hexanone
 Concen: 1.920 ug/L
 RT: 10.922 min Scan# 14
 Delta R.T. -0.042 min
 Lab File: VW031247.D
 Acq: 13 Dec 2024 19:20

Instrument :
 MSVOA_W
 ClientSampleId :

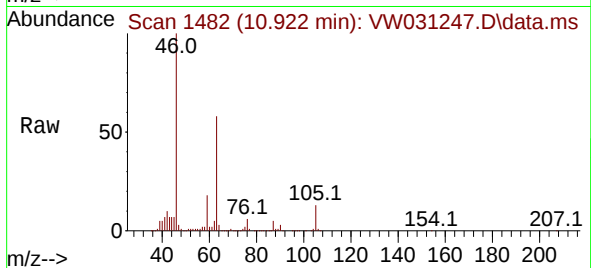

Tgt Ion: 43 Resp: 9509

Ion	Ratio	Lower	Upper
43	100		
58	26.0	43.0	64.6#
57	21.2	15.7	23.5
100	0.0	10.3	15.5#

