




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
 Data File : VW031238.D
 Acq On : 13 Dec 2024 15:45
 Operator : SY/MD
 Sample : P5155-22
 Misc : 4.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28W5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 12/16/2024
 Supervised By :Mahesh Dadoda 12/17/2024

Quant Time: Dec 14 00:46:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 14 00:44:31 2024
 Response via : Initial Calibration

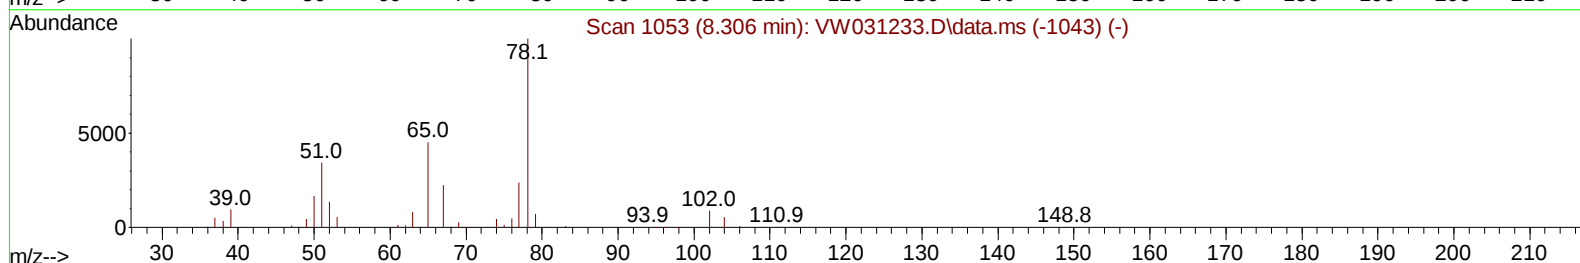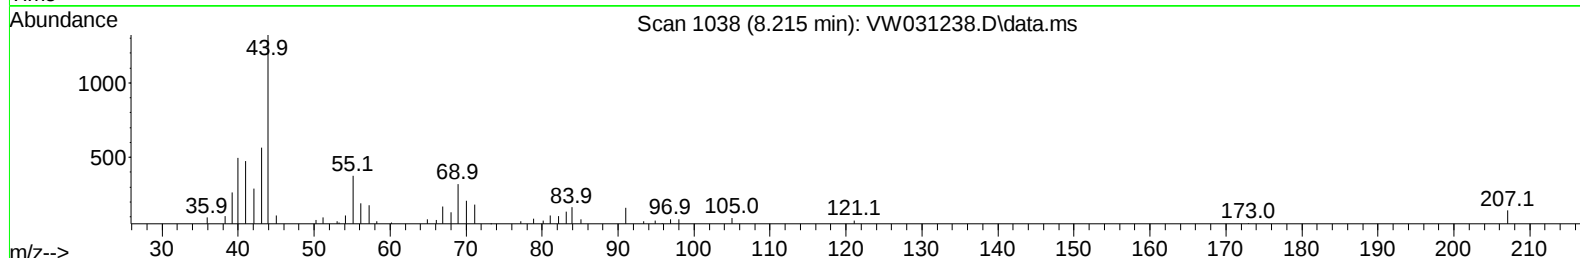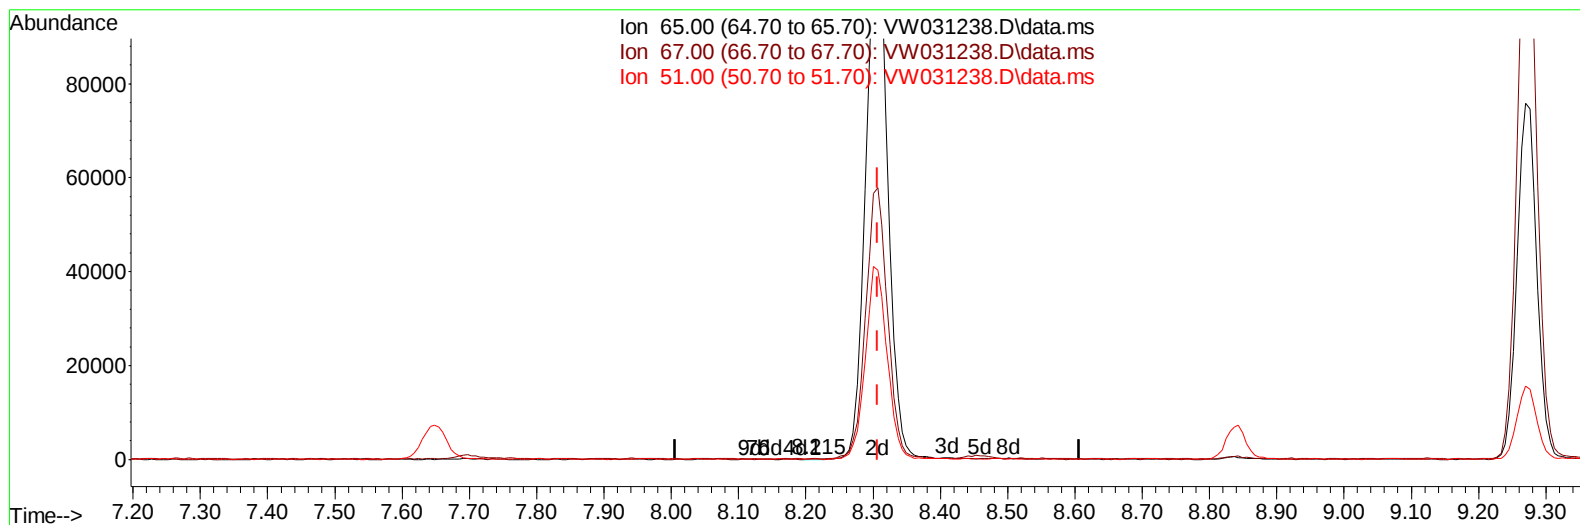

TIC: VW031238.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.215min (-0.091) 0.01 ug/L

response 134

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	50.75
51.00	108.10	100.75
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
 Data File : VW031238.D
 Acq On : 13 Dec 2024 15:45
 Operator : SY/MD
 Sample : P5155-22
 Misc : 4.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28W5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 12/16/2024
 Supervised By :Mahesh Dadoda 12/17/2024

Quant Time: Dec 14 00:46:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 14 00:44:31 2024
 Response via : Initial Calibration

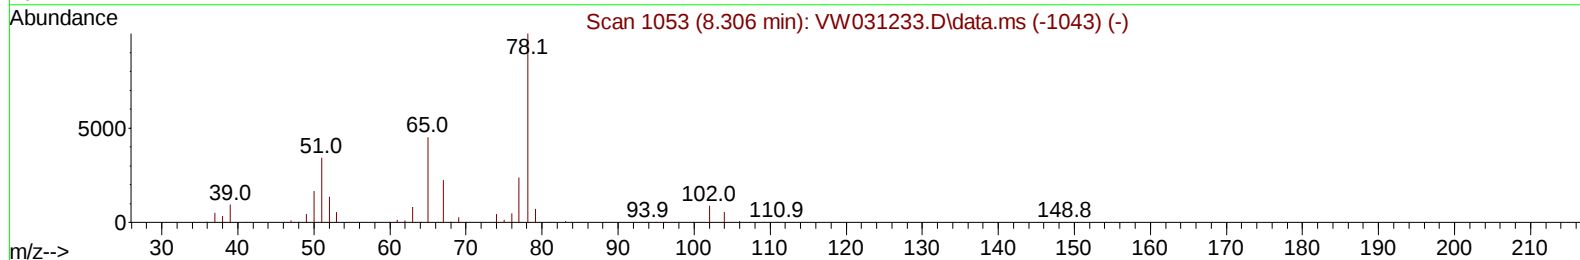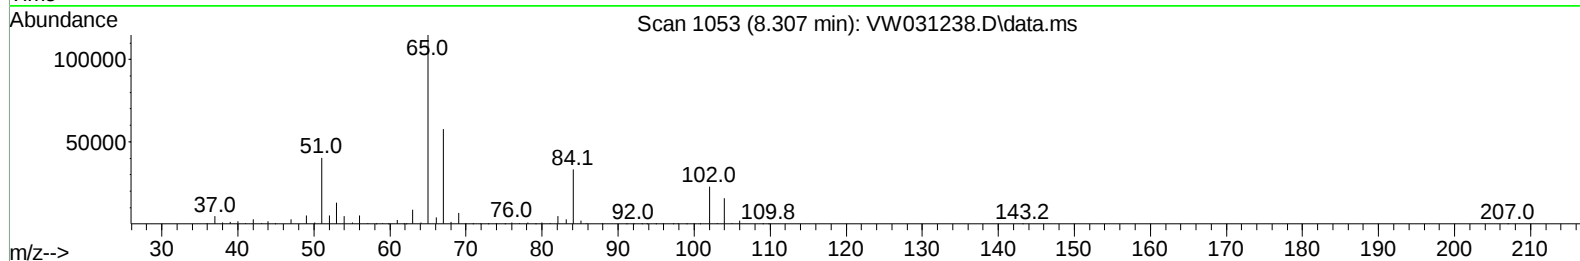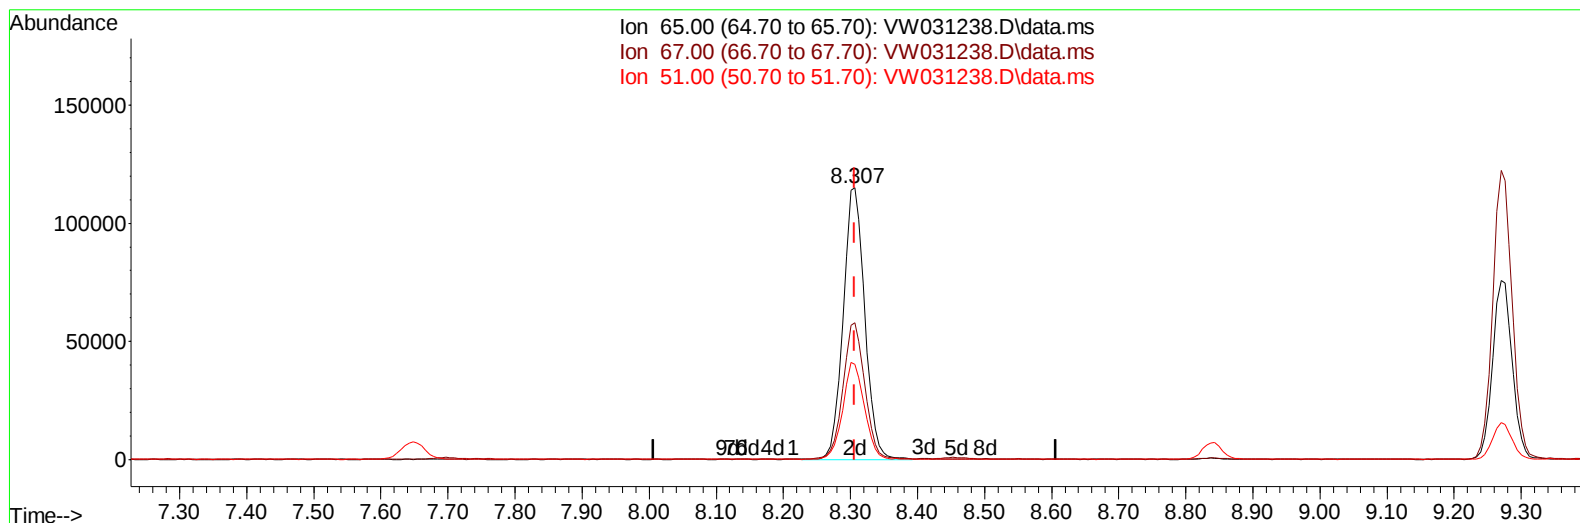

TIC: VW031238.D\data.ms

(26) 1,2-Dichloroethane-d4 (S)

8.307min (+ 0.000) 25.93 ug/L m

response 257723

Ion	Exp%	Act%
65.00	100.00	100.00
67.00	54.50	0.03#
51.00	108.10	0.05#
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121324\
 Data File : VW031238.D
 Acq On : 13 Dec 2024 15:45
 Operator : SY/MD
 Sample : P5155-22
 Misc : 4.07g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28W5

Manual IntegrationsAPPROVED

Quant Time: Dec 14 00:46:31 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Sat Dec 14 00:44:31 2024
 Response via : Initial Calibration

Reviewed By :Romaben Patel 12/16/2024
 Supervised By :Mahesh Dadoda 12/17/2024

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	722319	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	323849	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152	72890	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.356	65	331307	30.484	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	121.920%	
7) Chloroethane-d5	2.893	69	239663	29.811	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	119.240%	
11) 1,1-Dichloroethene-d2	4.015	65	125284	24.302	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	97.200%	
21) 2-Butanone-d5	7.100	46	127102	62.100	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	124.200%	
24) Chloroform-d	7.648	84	450777	22.777	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	91.120%	
26) 1,2-Dichloroethane-d4	8.307	65	257723m	25.930	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	103.720%	
32) Benzene-d6	8.276	84	829683	39.971	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	159.880%#	
36) 1,2-Dichloropropane-d6	9.270	67	247449	40.904	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	163.600%#	
41) Toluene-d8	10.318	98	493867	25.576	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	102.320%	
43) trans-1,3-Dichloroprop...	10.575	79	94937	34.035	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	136.160%#	
47) 2-Hexanone-d5	10.922	63	87671	107.764	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	215.520%#	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	99946	26.313	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	105.240%	
66) 1,2-Dichlorobenzene-d4	13.848	152	50256	18.572	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	74.280%#	
Target Compounds						
13) Acetone	4.173	43	109634	38.463	ug/L #	100
14) Carbon disulfide	4.381	76	10126	0.351	ug/L #	92
22) 2-Butanone	7.197	43	39291	11.376	ug/L	90
35) Methylcyclohexane	9.337	83	4272	0.434	ug/L #	66
40) 4-Methyl-2-pentanone	10.209	43	11596	4.378	ug/L	94
42) Toluene	10.386	91	8353	0.383	ug/L	92
46) Tetrachloroethene	10.867	164	1213	0.293	ug/L	92

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121324\
Data File : VW031238.D
Acq On : 13 Dec 2024 15:45
Operator : SY/MD
Sample : P5155-22
Misc : 4.07g/10mL/MSVOA_W/SOIL/A
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28W5

Manual IntegrationsAPPROVED

Reviewed By :Romaben Patel 12/16/2024
Supervised By :Mahesh Dadoda 12/17/2024

Quant Time: Dec 14 00:46:31 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Sat Dec 14 00:44:31 2024
Response via : Initial Calibration

