

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121423\
 Data File : VW027616.D
 Acq On : 14 Dec 2023 09:34
 Operator : SY/MD
 Sample : VW1214SBL01
 Misc : 5.00g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 15 03:29:08 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 15 03:28:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	252105	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	219070	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	105207	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	84588	16.673	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	66.680%		
7) Chloroethane-d5	2.899	69	69480	18.892	ug/L	0.00
Spiked Amount 25.000	Range 30 - 150		Recovery =	75.560%		
11) 1,1-Dichloroethene-d2	4.021	65	39093	18.211	ug/L	0.00
Spiked Amount 25.000	Range 45 - 110		Recovery =	72.840%		
21) 2-Butanone-d5	7.081	46	43810	32.955	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	65.920%		
24) Chloroform-d	7.648	84	151438	20.124	ug/L	0.00
Spiked Amount 25.000	Range 40 - 150		Recovery =	80.480%		
26) 1,2-Dichloroethane-d4	8.307	65	74053	19.244	ug/L	0.00
Spiked Amount 25.000	Range 70 - 130		Recovery =	76.960%		
32) Benzene-d6	8.270	84	320764	20.789	ug/L	0.00
Spiked Amount 25.000	Range 20 - 135		Recovery =	83.160%		
36) 1,2-Dichloropropane-d6	9.270	67	96454	21.205	ug/L	0.00
Spiked Amount 25.000	Range 70 - 120		Recovery =	84.800%		
41) Toluene-d8	10.319	98	269501	19.963	ug/L	0.00
Spiked Amount 25.000	Range 30 - 130		Recovery =	79.840%		
43) trans-1,3-Dichloroprop...	10.575	79	30231	17.187	ug/L	0.00
Spiked Amount 25.000	Range 30 - 135		Recovery =	68.760%		
47) 2-Hexanone-d5	10.922	63	29552	34.869	ug/L	0.00
Spiked Amount 50.000	Range 20 - 135		Recovery =	69.740%		
56) 1,1,2,2-Tetrachloroeth...	12.690	84	66599	17.800	ug/L	0.00
Spiked Amount 25.000	Range 45 - 120		Recovery =	71.200%		
66) 1,2-Dichlorobenzene-d4	13.848	152	73196	19.848	ug/L	0.00
Spiked Amount 25.000	Range 75 - 120		Recovery =	79.400%		
Target Compounds					Qvalue	
71) Naphthalene	15.360	128	2952	0.404	ug/L #	92


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121423\
Data File : VW027616.D
Acq On : 14 Dec 2023 09:34
Operator : SY/MD
Sample : VW1214SBL01
Misc : 5.00g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 15 03:29:08 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 15 03:28:28 2023
Response via : Initial Calibration

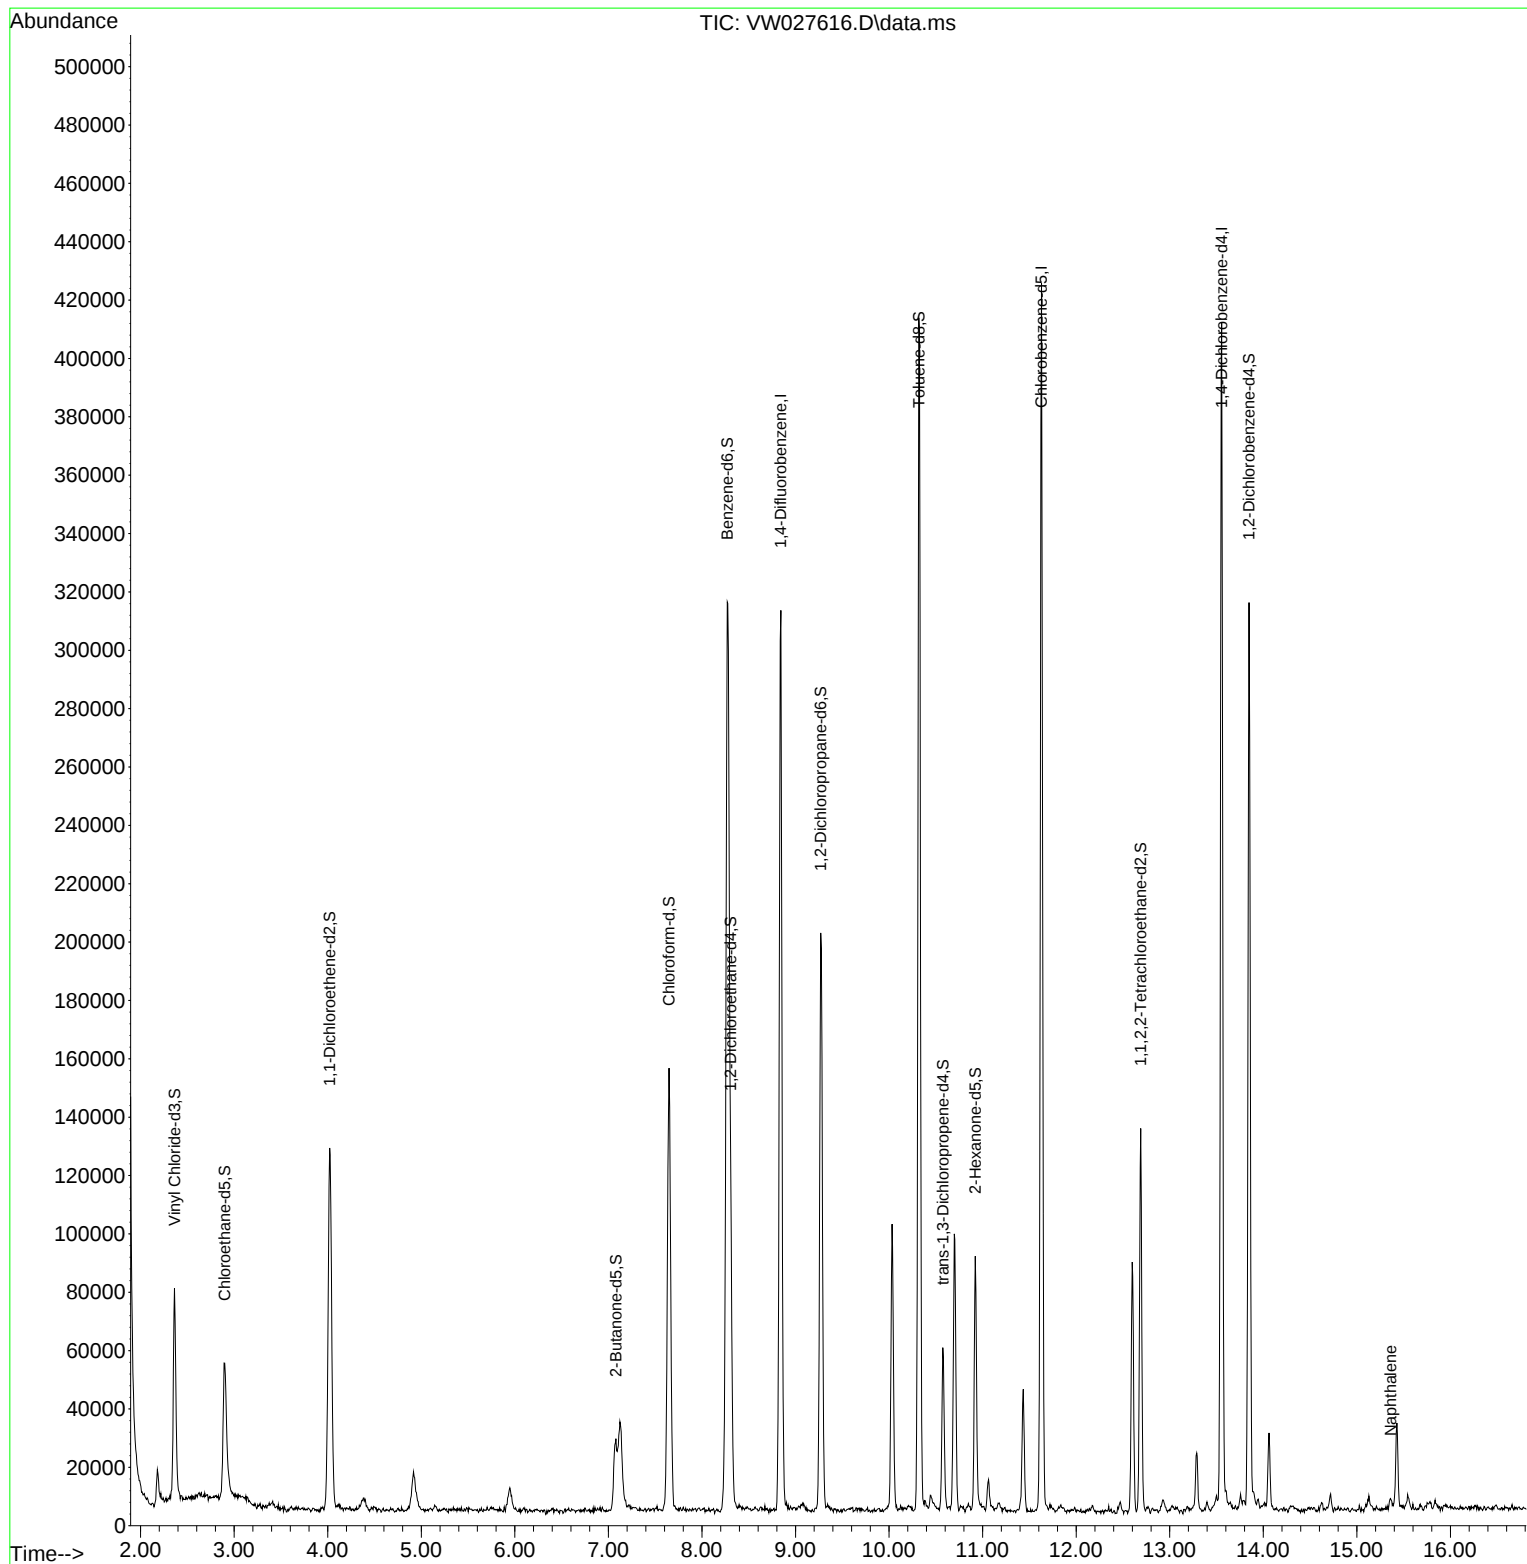

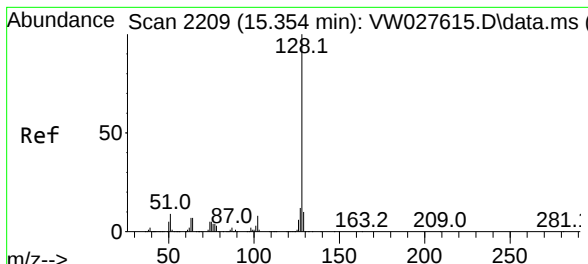

#71
Naphthalene
Concen: 0.404 ug/L
RT: 15.360 min Scan# 21
Delta R.T. 0.006 min
Lab File: VW027616.D
Acq: 14 Dec 2023 09:34

Instrument :
MSVOA_W
ClientSampleId :

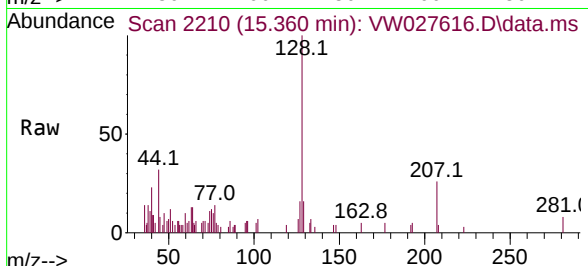

Tgt Ion:	128	Resp:	2952
Ion	Ratio	Lower	Upper
128	100		
127	18.1	10.3	15.5#
129	11.3	8.6	12.8

