




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121423\
 Data File : VW027618.D
 Acq On : 14 Dec 2023 10:32
 Operator : SY/MD
 Sample : 05806-06
 Misc : 5.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0LQ8RE

Manual IntegrationsAPPROVED

Quant Time: Dec 15 03:29:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 15 03:28:28 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/15/2023
 Supervised By :Mahesh Dadoda 12/15/2023

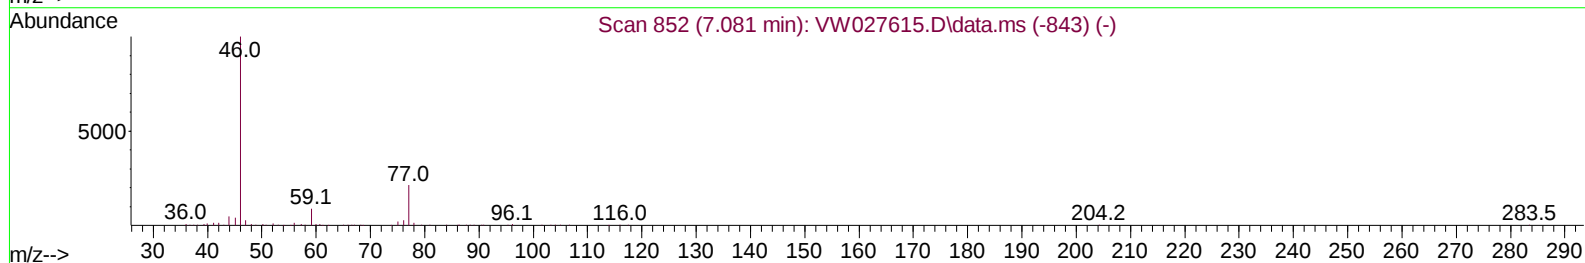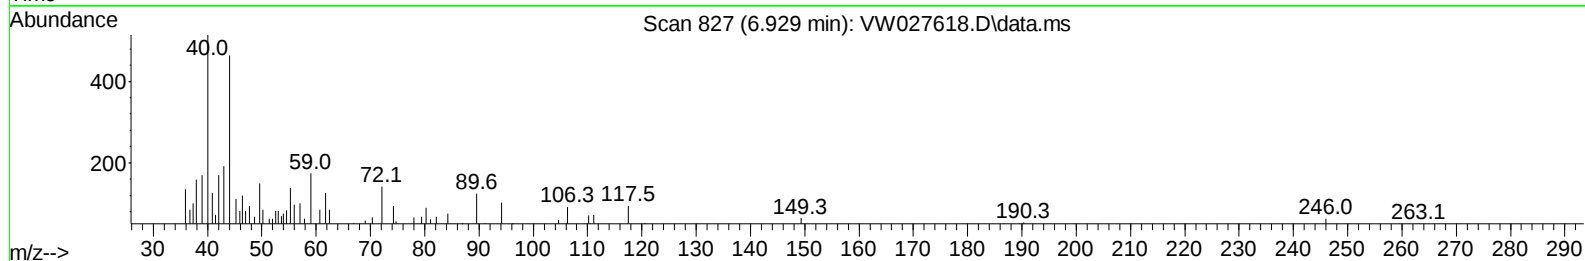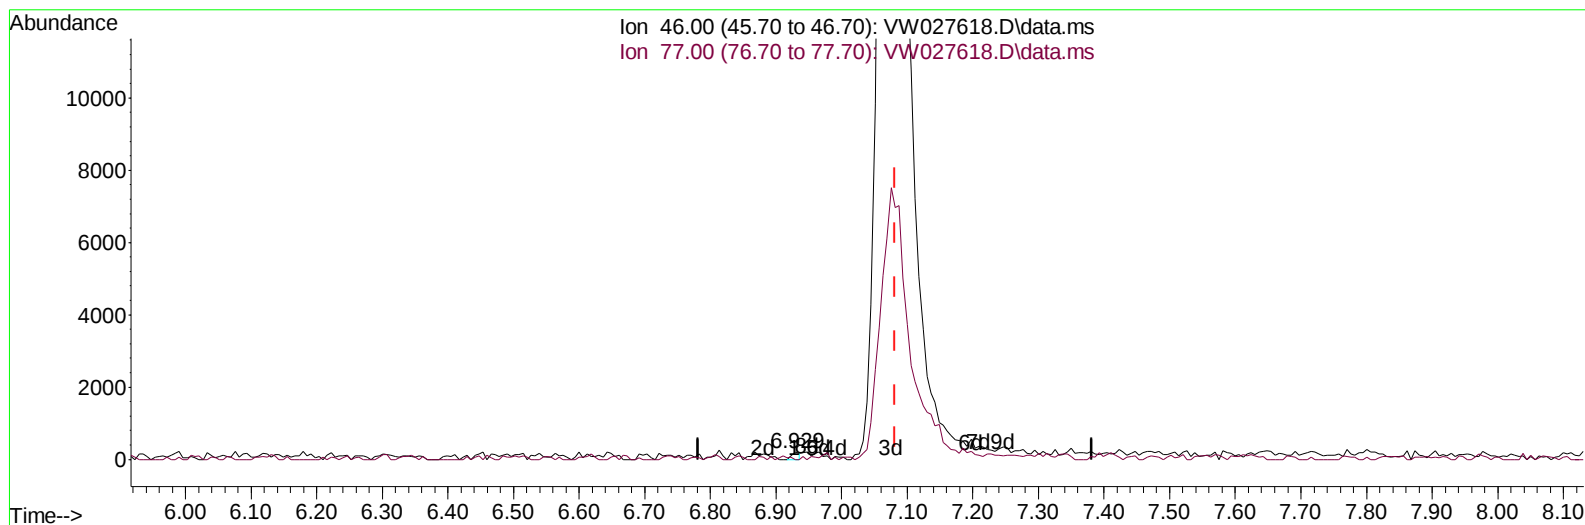

TIC: VW027618.D\data.ms

(21) 2-Butanone-d5 (S)

6.929min (-0.152) 0.05 ug/L

response 178

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	18.30	15.17
0.00	0.00	0.00
0.00	0.00	0.00




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121423\
 Data File : VW027618.D
 Acq On : 14 Dec 2023 10:32
 Operator : SY/MD
 Sample : 05806-06
 Misc : 5.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0LQ8RE

Manual IntegrationsAPPROVED

Quant Time: Dec 15 03:29:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 15 03:28:28 2023
 Response via : Initial Calibration

Reviewed By :Semsettin Yesilyurt 12/15/2023
 Supervised By :Mahesh Dadoda 12/15/2023

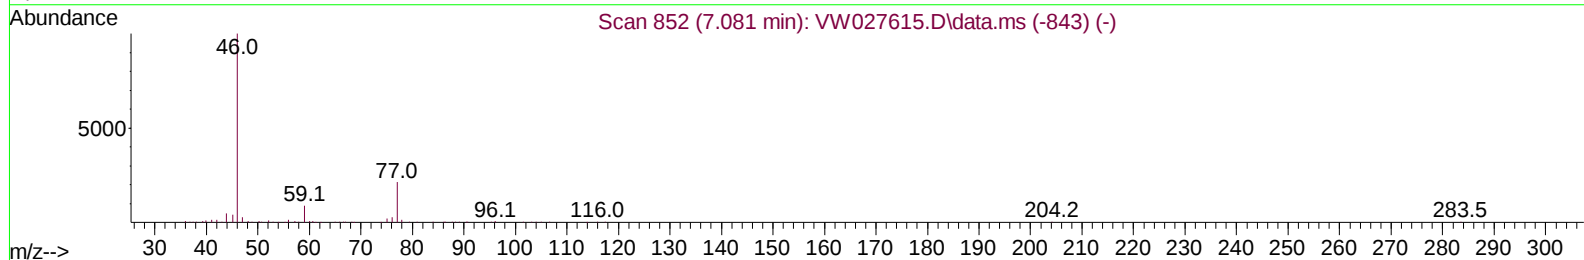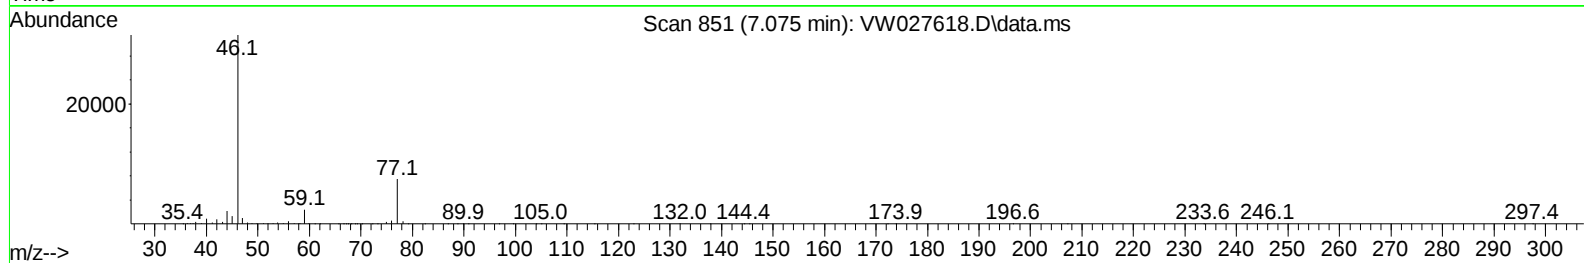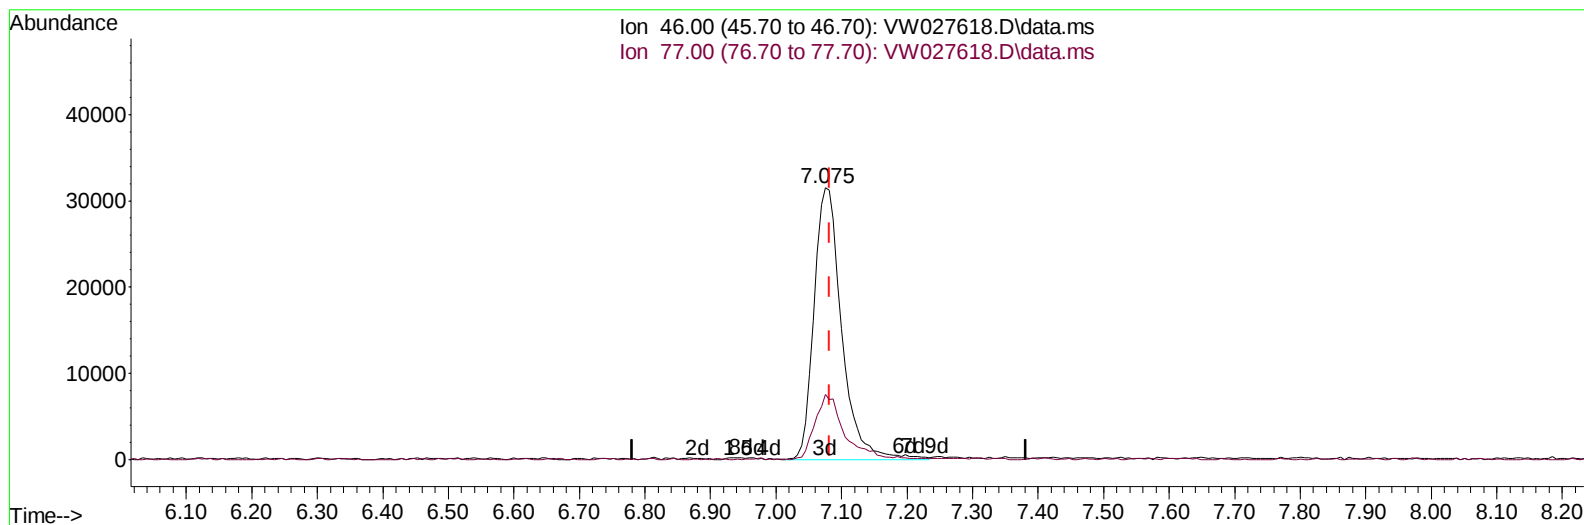

TIC: VW027618.D\data.ms

(21) 2-Butanone-d5 (S)

7.075min (-0.006) 28.44 ug/L m

response 92322

Ion	Exp%	Act%
46.00	100.00	100.00
77.00	18.30	0.03#
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121423\
 Data File : VW027618.D
 Acq On : 14 Dec 2023 10:32
 Operator : SY/MD
 Sample : 05806-06
 Misc : 5.07g/10mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E0LQ8RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/15/2023
 Supervised By :Mahesh Dadoda 12/15/2023

Quant Time: Dec 15 03:29:36 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
 Quant Title : SFAM01.0
 QLast Update : Fri Dec 15 03:28:28 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Difluorobenzene	8.843	114	615699	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	454395	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	135037	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	283672	22.895	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	91.600%	
7) Chloroethane-d5	2.899	69	206749	23.018	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150	Recovery	=	92.080%	
11) 1,1-Dichloroethene-d2	4.027	65	117868	22.482	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110	Recovery	=	89.920%	
21) 2-Butanone-d5	7.075	46	92322m	28.436	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	56.880%	
24) Chloroform-d	7.648	84	439863	23.934	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150	Recovery	=	95.720%	
26) 1,2-Dichloroethane-d4	8.307	65	203310	21.633	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130	Recovery	=	86.520%	
32) Benzene-d6	8.276	84	946431	29.572	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135	Recovery	=	118.280%	
36) 1,2-Dichloropropane-d6	9.276	67	277012	29.361	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120	Recovery	=	117.440%	
41) Toluene-d8	10.325	98	769319	27.474	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130	Recovery	=	109.880%	
43) trans-1,3-Dichloroprop...	10.581	79	82876	22.715	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135	Recovery	=	90.880%	
47) 2-Hexanone-d5	10.922	63	60317	34.312	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135	Recovery	=	68.620%	
56) 1,1,2,2-Tetrachloroeth...	12.690	84	141371	18.217	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120	Recovery	=	72.880%	
66) 1,2-Dichlorobenzene-d4	13.848	152	132143	27.917	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120	Recovery	=	111.680%	

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121423\
Data File : VW027618.D
Acq On : 14 Dec 2023 10:32
Operator : SY/MD
Sample : 05806-06
Misc : 5.07g/10mL/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E0LQ8RE

Manual IntegrationsAPPROVED

Reviewed By :Semsettin Yesilyurt 12/15/2023
Supervised By :Mahesh Dadoda 12/15/2023

Quant Time: Dec 15 03:29:36 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120623SMA.M
Quant Title : SFAM01.0
QLast Update : Fri Dec 15 03:28:28 2023
Response via : Initial Calibration

