

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121619\
Quantitation Report (Qedit)




Data File : VW014368.D
Acq On : 16 Dec 2019 14:56
Operator : SY/VA
Sample : K6322-08RE
Misc : 4.23G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
C0C46RE

Manual Integrations
APPROVED

MMDadoda
12/18/2019 12:58:40 PM

Quant Time: Dec 17 07:30:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 17 07:27:11 2019
Response via : Initial Calibration

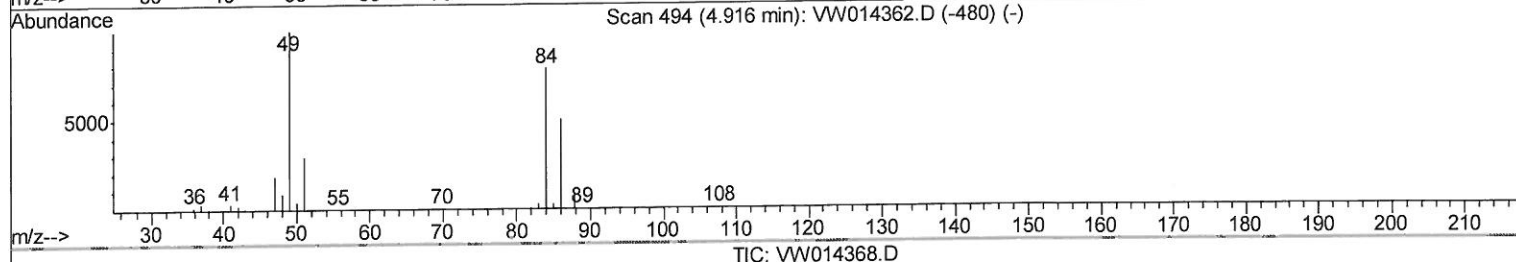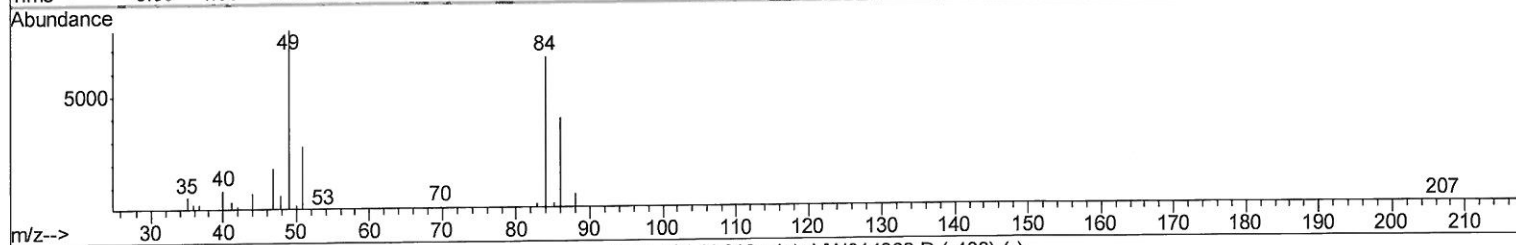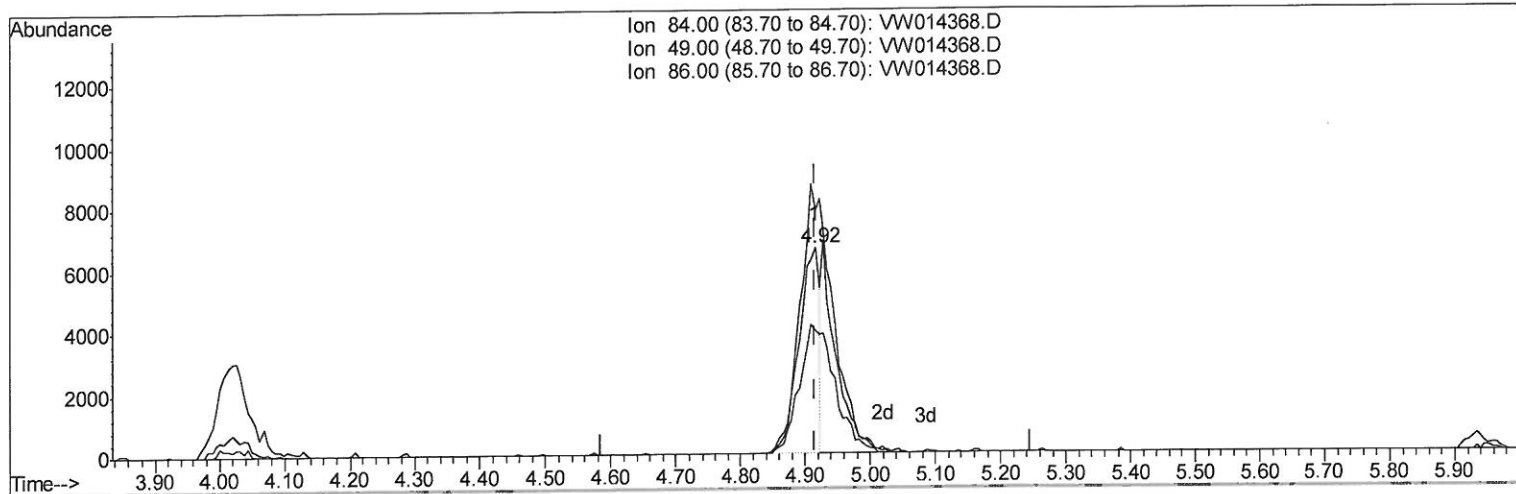

(16) Methylene chloride (T)

4.916min (-0.000) 0.98ug/L

response 14324

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	118.14
86.00	62.40	59.37
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121619\
Quantitation Report (Qedit)




Data File : VW014368.D
Acq On : 16 Dec 2019 14:56
Operator : SY/VA
Sample : K6322-08RE
Misc : 4.23G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sampled :
C0C46RE

Manual Integrations
APPROVED

MM Dadoda
12/18/2019 12:58:40 PM

Quant Time: Dec 17 07:30:21 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 17 07:27:11 2019
Response via : Initial Calibration

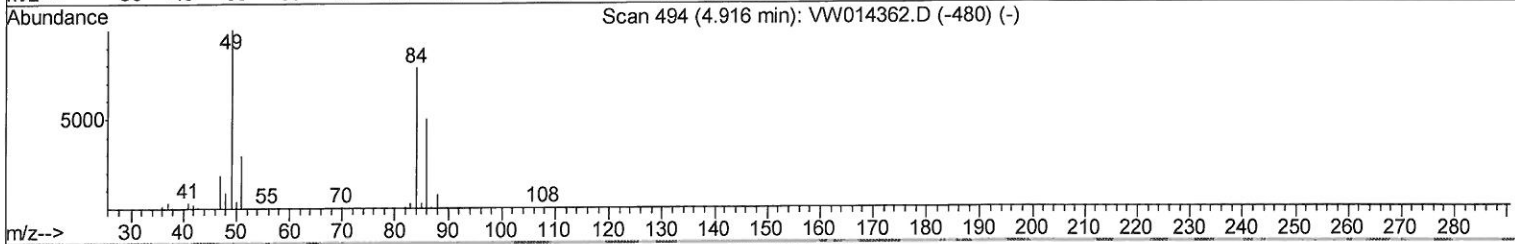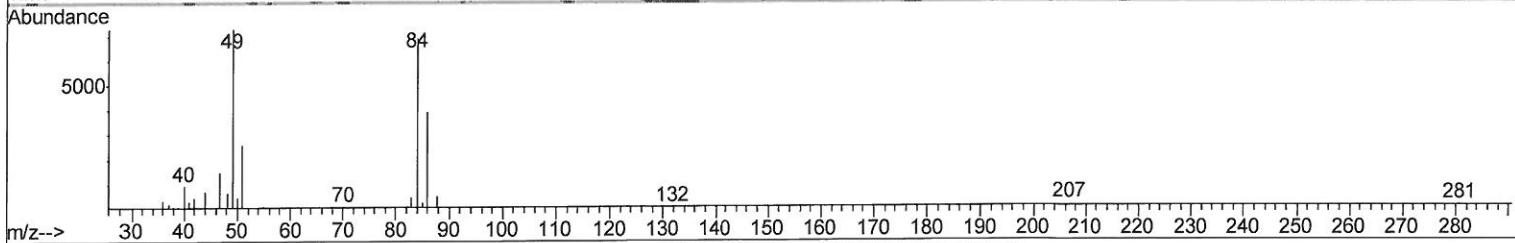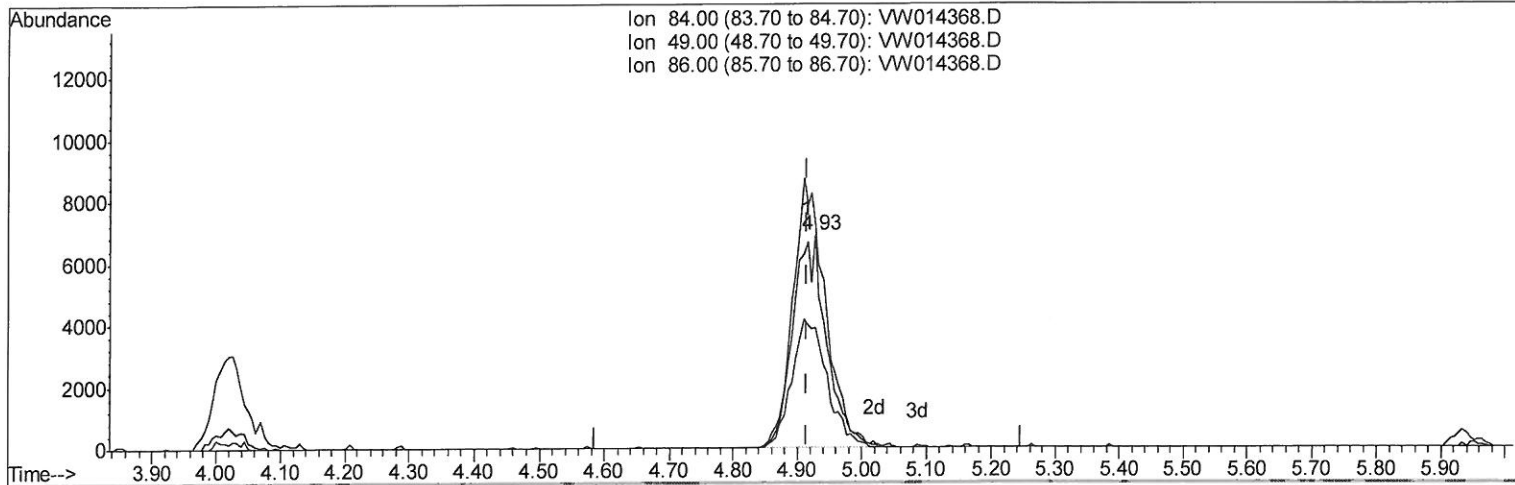

TIC: VW014368.D

(16) Methylene chloride (T)

4.928min (+0.012) 1.71ug/L m

response 24968

Ion	Exp%	Act%
84.00	100	100
49.00	120.30	105.65
86.00	62.40	56.63
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121619\
 Quantitation Report (QT Reviewed)

Data File : VW014368.D
 Acq On : 16 Dec 2019 14:56
 Operator : SY/VA
 Sample : K6322-08RE
 Misc : 4.23G/10ML/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 Client Sampled :
 C0C46RE

Manual Integrations
 APPROVED

MMDadoda
 12/18/2019 12:58:40 PM

Quant Time: Dec 17 07:56:01 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Tue Dec 17 07:27:11 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	953160	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	754332	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	237812	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	303103	21.00	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	84.00%
7) Chloroethane-d5	2.89	69	265290	24.72	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	98.88%
10) 1,1-Dichloroethene-d2	4.02	63	433706	17.01	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	68.04%
20) 2-Butanone-d5	7.07	46	158249	42.07	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	84.14%
24) Chloroform-d	7.65	84	629778	25.95	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	103.80%
26) 1,2-Dichloroethane-d4	8.31	65	330908	26.01	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	104.04%
29) Benzene-d6	8.27	84	1262586	28.56	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	114.24%
33) 1,2-Dichloropropane-d6	9.27	67	412996	30.36	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	121.44%#
37) Toluene-d8	10.32	98	1015055	25.39	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	101.56%
38) trans-1,3-Dichloropropene-	10.57	79	126753	22.21	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	88.84%
39) 2-Hexanone-d5	10.92	63	122348	45.24	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.48%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	283350	25.56	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	102.24%
61) 1,2-Dichlorobenzene-d4	13.85	152	242092	26.64	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	106.56%

Target Compounds

16) Methylene chloride	4.93	84	24968m	1.709	ug/L	Qvalue
------------------------	------	----	--------	-------	------	--------

12/17/19 Sy

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121619\
Quantitation Report (QT Reviewed)

Data File : VW014368.D
Acq On : 16 Dec 2019 14:56
Operator : SY/VA
Sample : K6322-08RE
Misc : 4.23G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
Client Sample Id :
C0C46RE

Manual Integrations
APPROVED

MMDadoda
12/18/2019 12:58:40 PM

Quant Time: Dec 17 07:56:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Tue Dec 17 07:27:11 2019
Response via : Initial Calibration

