


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121718\
 Data File : VW007521.D
 Acq On : 14 Dec 2018 08:28
 Operator : SY/AP
 Sample : BFB
 Misc : 5.00G/5ML/MSVOA_W/SOIL
 ALS Vial : 46 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\82W121118S.M
 Title : SW846 8260
 Last Update : Tue Dec 11 02:58:16 2018

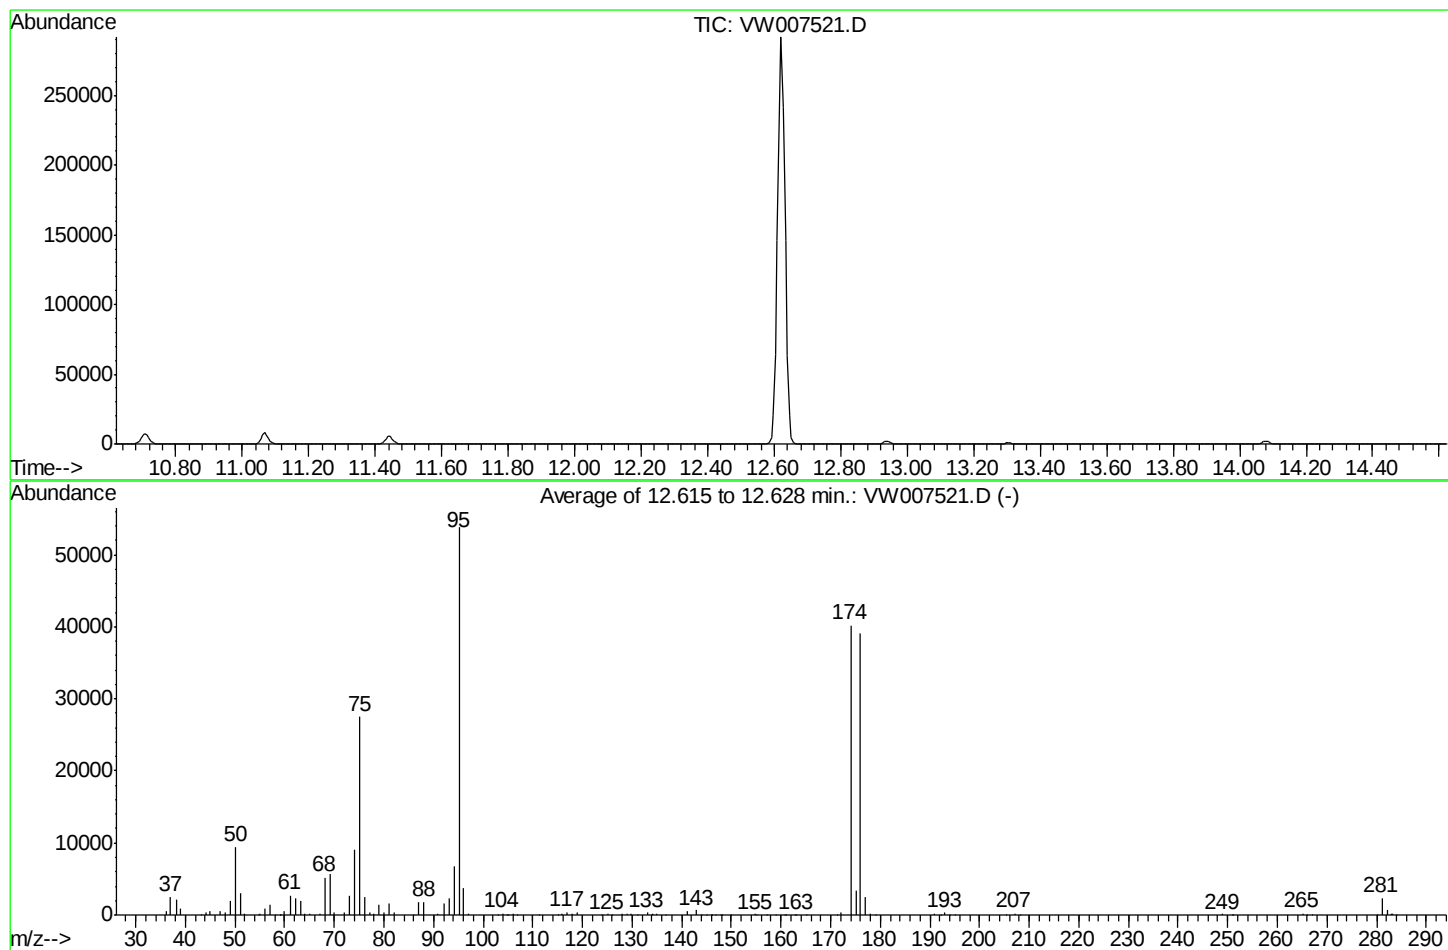

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.6	9453	PASS
75	95	30	60	51.1	27496	PASS
95	95	100	100	100.0	53816	PASS
96	95	5	9	7.0	3753	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	74.7	40186	PASS
175	174	5	9	8.3	3318	PASS
176	174	95	101	97.4	39157	PASS
177	176	5	9	6.5	2555	PASS