


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_W\DATA\VW121718\
Data File : VW007572.D
Acq On : 15 Dec 2018 10:07
Operator : SY/AP
Sample : BFB
Misc : 5.00G/5ML/MSVOA_W/SOIL
ALS Vial : 56 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\82W121118S.M
Title : SW846 8260
Last Update : Tue Dec 11 02:58:16 2018

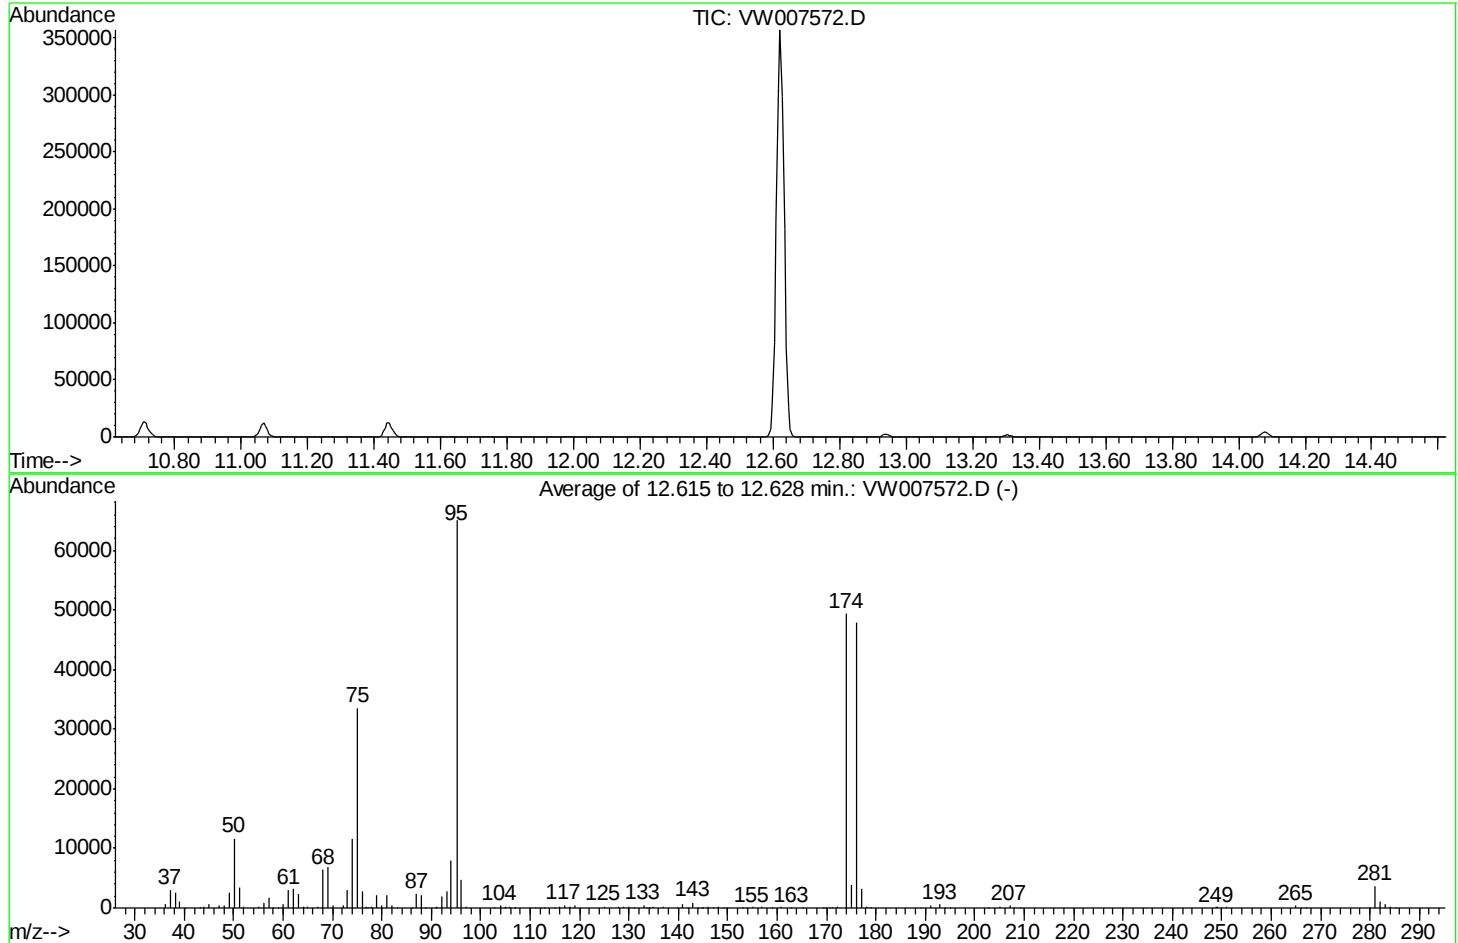

AutoFind: Scans 1757, 1758, 1759; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	11643	PASS
75	95	30	60	51.6	33573	PASS
95	95	100	100	100.0	65042	PASS
96	95	5	9	7.2	4673	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	75.9	49344	PASS
175	174	5	9	8.0	3961	PASS
176	174	95	101	96.9	47800	PASS
177	176	5	9	6.6	3161	PASS