

Data File : VW014389.D
Acq On : 17 Dec 2019 13:44
Operator : SY/VA
Sample : K6270-09
Misc : 4.98G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETK85

Quant Time: Dec 18 01:40:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 01:35:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1184564	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1070468	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	468000	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	352551	19.65	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	78.60%
7) Chloroethane-d5	2.89	69	295303	22.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	88.56%
10) 1,1-Dichloroethene-d2	4.24	63	119	0.00	ug/L	0.22
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.00%#
20) 2-Butanone-d5	7.07	46	223940	47.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	95.82%
24) Chloroform-d	7.77	84	209	0.01	ug/L	0.12
Spiked Amount	25.000	Range	40 - 150	Recovery	=	0.04%#
26) 1,2-Dichloroethane-d4	8.47	65	176	0.01	ug/L	0.17
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.04%#
29) Benzene-d6	8.27	84	1542684	24.59	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	98.36%
33) 1,2-Dichloropropane-d6	9.27	67	487854	25.28	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.12%
37) Toluene-d8	10.32	98	1358599	23.95	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	95.80%
38) trans-1,3-Dichloropropene-	10.58	79	185408	22.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	91.60%
39) 2-Hexanone-d5	10.92	63	188726	49.17	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.34%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	373684	23.76	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	95.04%
61) 1,2-Dichlorobenzene-d4	13.85	152	449305	25.12	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	100.48%

Target Compounds


					Qvalue
13) Acetone	4.12	43	27577	6.119 ug/L	96
30) Cyclohexane	7.96	56	22318	0.835 ug/L	86
34) Benzene	8.32	78	125639	1.854 ug/L	100
36) Methylcyclohexane	9.33	83	37539	1.288 ug/L	95
44) Toluene	10.38	91	288547	4.061 ug/L	98
49) 2-Hexanone	10.92	43	26197	3.205 ug/L #	60
53) Ethylbenzene	11.73	91	81246	1.054 ug/L	94
54) m,p-Xylene	11.83	106	50412	1.700 ug/L	91
55) o-xylene	12.16	106	19804	0.704 ug/L	89


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014389.D
Acq On : 17 Dec 2019 13:44
Operator : SY/VA
Sample : K6270-09
Misc : 4.98G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETK85

Quant Time: Dec 18 01:40:50 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 01:35:45 2019
Response via : Initial Calibration

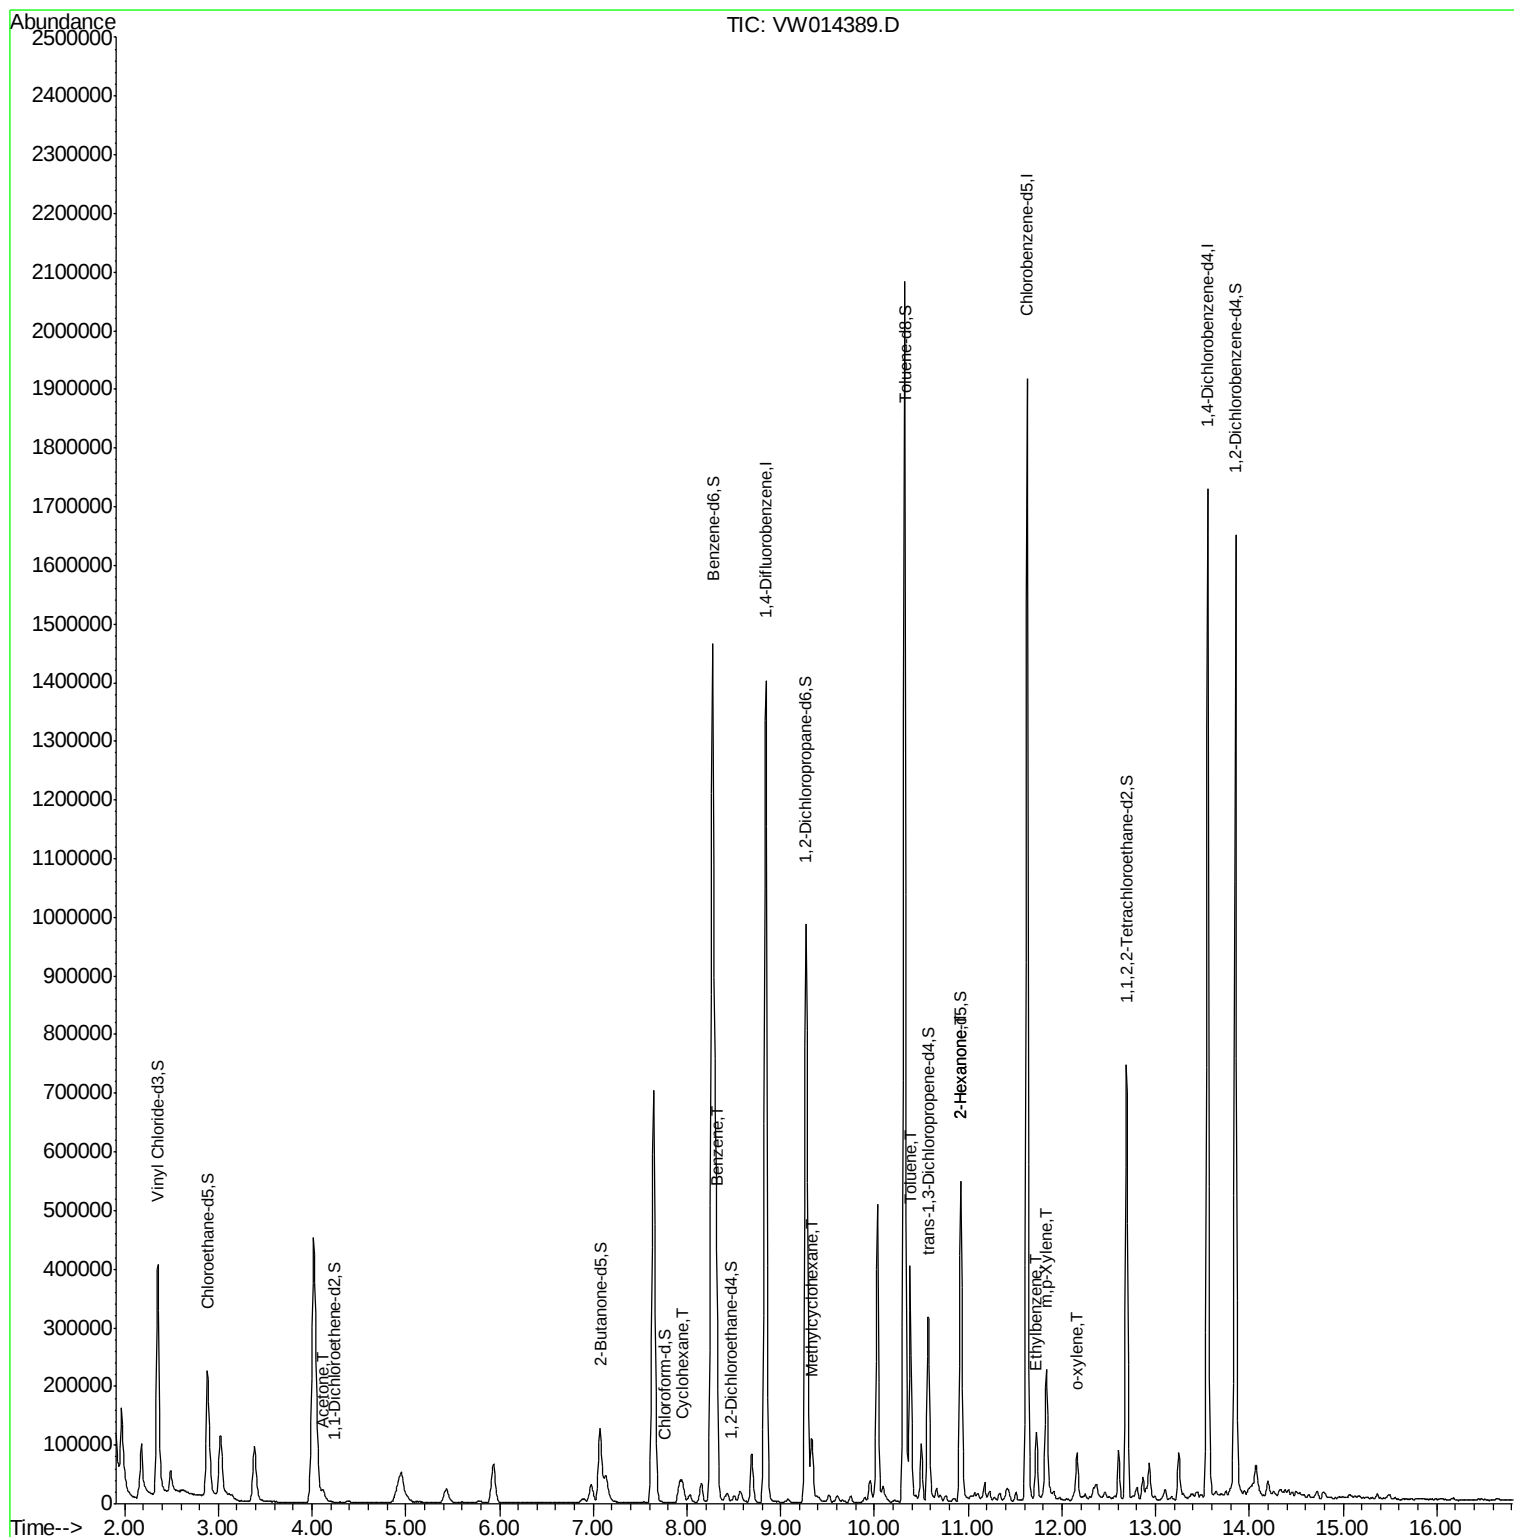

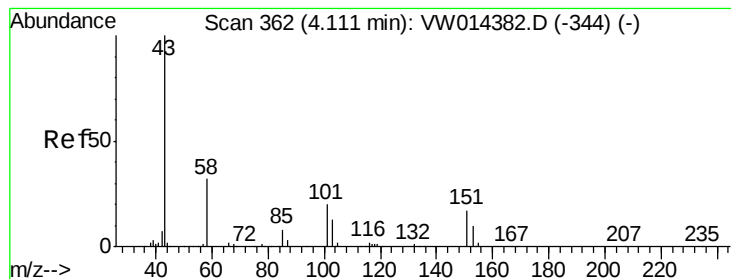

#13

Acetone

Concen: 6.119 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW014389.D

Acq: 17 Dec 2019 13:44

Instrument :

MSVOA_W

ClientSampled :





ETK85

Tgt Ion: 43 Resp: 27577

Ion Ratio Lower Upper

43 100

58 30.6 0.0 65.4

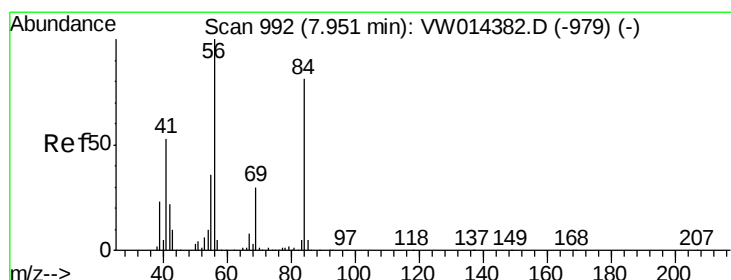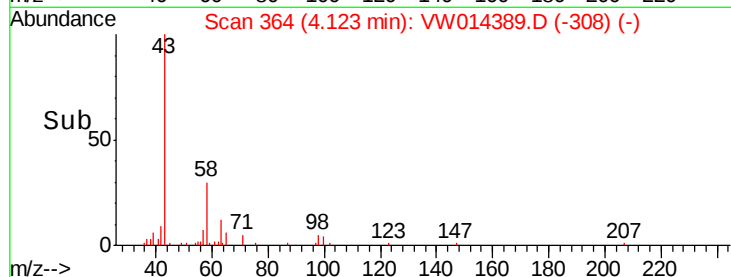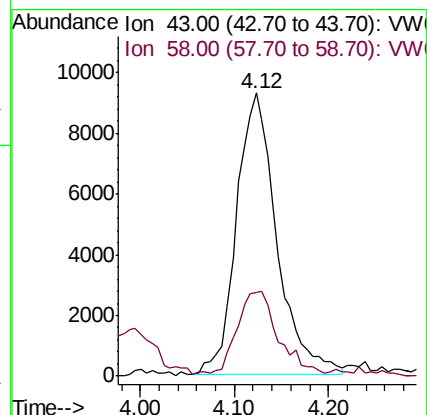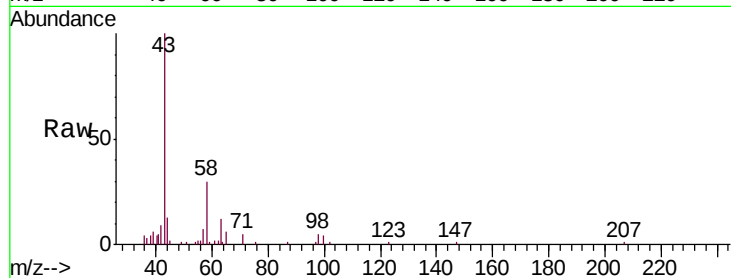

#30

Cyclohexane

Concen: 0.835 ug/L

RT: 7.96 min Scan# 993

Delta R.T. 0.01 min

Lab File: VW014389.D

Acq: 17 Dec 2019 13:44




Tgt Ion: 56 Resp: 22318


Ion Ratio Lower Upper

56 100

69 29.2 24.6 37.0

84 71.7 70.2 105.2

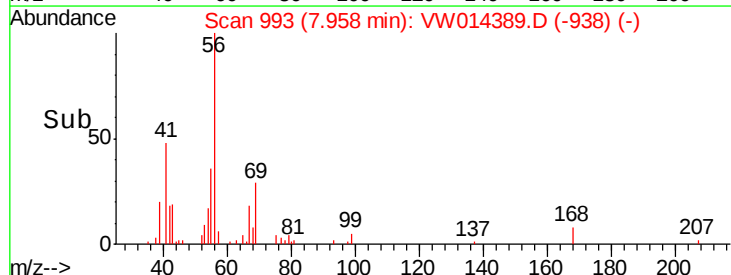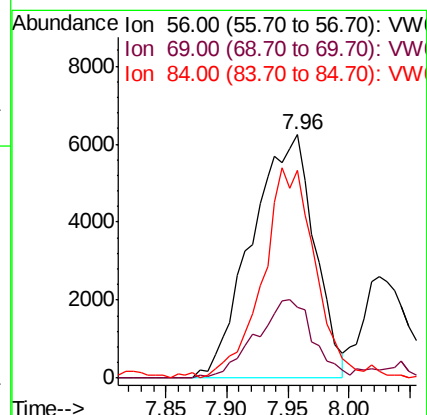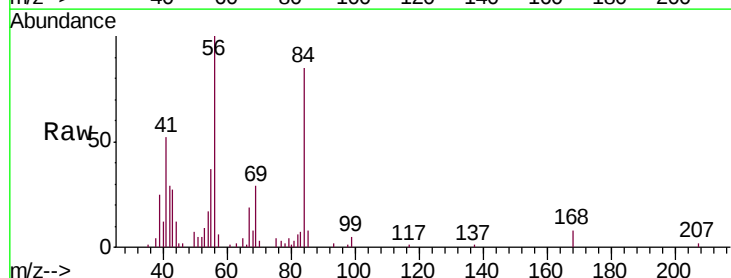

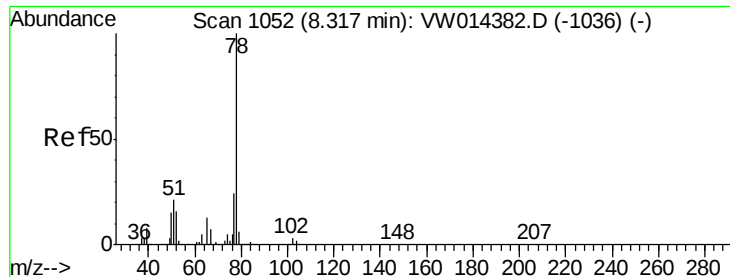

#34

Benzene

Concen: 1.854 ug/L

RT: 8.32 min Scan# 1053

Delta R.T. 0.01 min

Lab File: VW014389.D

Acq: 17 Dec 2019 13:44





Instrument :

MSVOA_W

ClientSampleId :

ETK85

Tgt Ion: 78 Resp: 125639

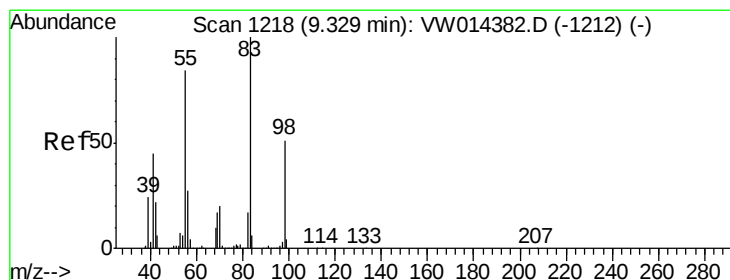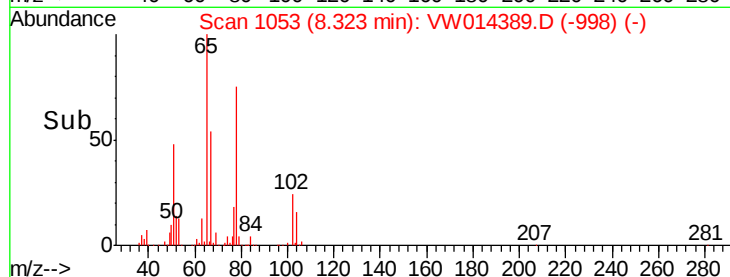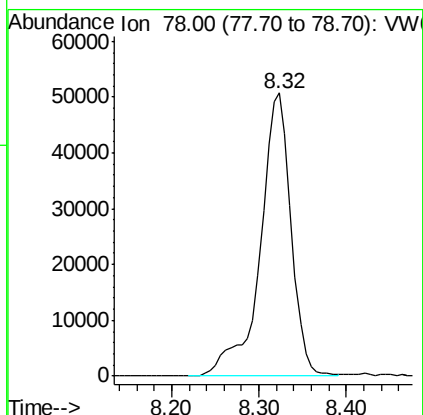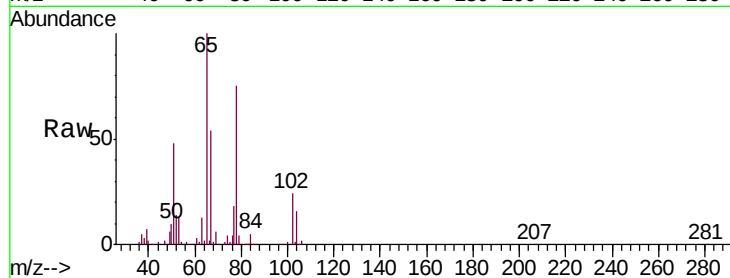

#36

Methylcyclohexane

Concen: 1.288 ug/L

RT: 9.33 min Scan# 1218




Delta R.T. -0.00 min


Lab File: VW014389.D

Acq: 17 Dec 2019 13:44

Tgt Ion: 83 Resp: 37539

Ion	Ratio	Lower	Upper
83	100		
55	82.2	59.8	89.8
98	49.1	39.5	59.3

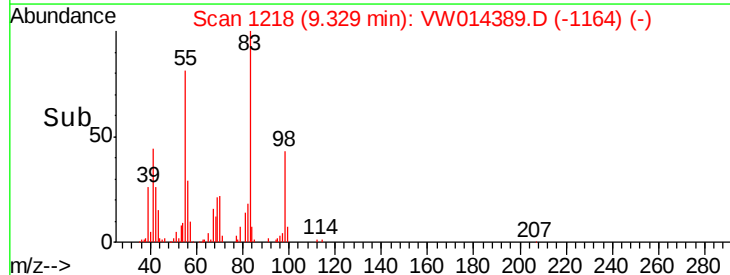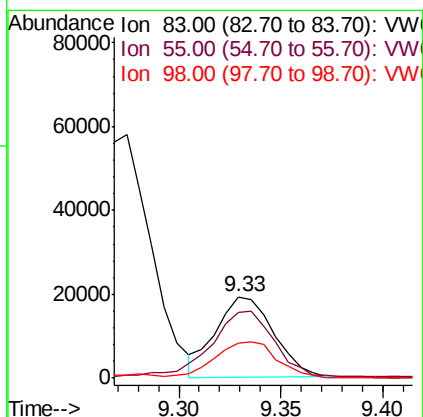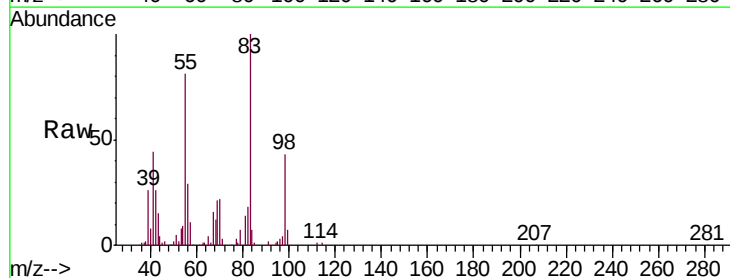

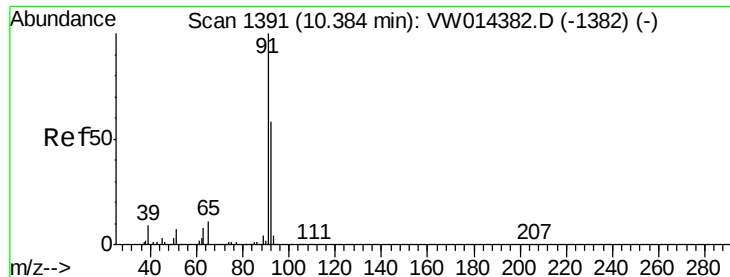

#44

Toluene

Concen: 4.061 ug/L

RT: 10.38 min Scan# 1391

Delta R.T. -0.00 min

Lab File: VW014389.D

Acq: 17 Dec 2019 13:44

Instrument :

MSVOA_W

ClientSampleId :





ETK85

Tgt Ion: 91 Resp: 288547

Ion Ratio Lower Upper

91 100

92 57.1 40.7 75.7

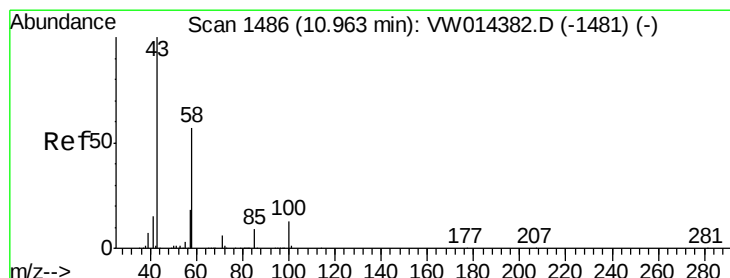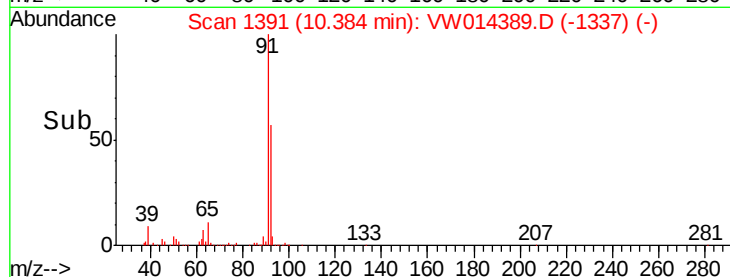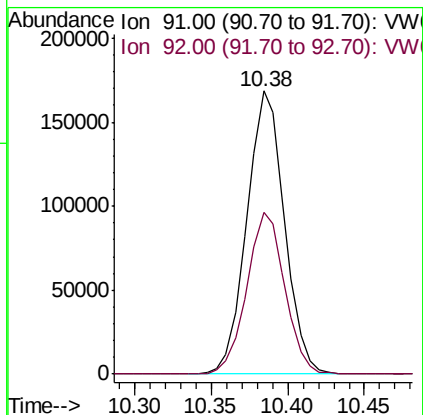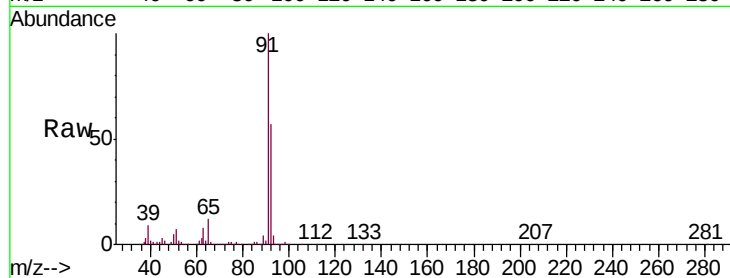

#49

2-Hexanone

Concen: 3.205 ug/L

RT: 10.92 min Scan# 1479

Delta R.T. -0.04 min

Lab File: VW014389.D

Acq: 17 Dec 2019 13:44

Tgt Ion: 43 Resp: 26197




Ion Ratio Lower Upper


43 100

58 23.1 44.4 66.6#

57 37.1 16.5 24.7#

100 1.7 11.1 16.7#

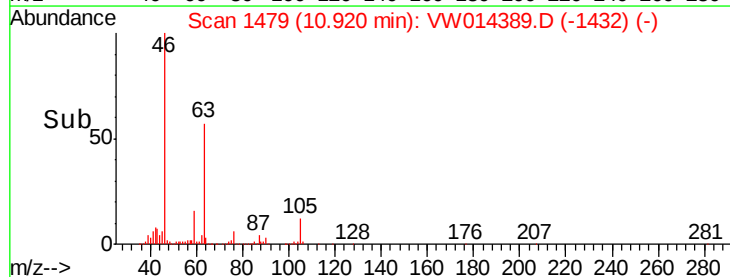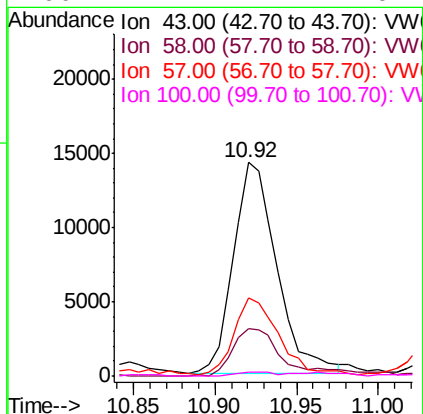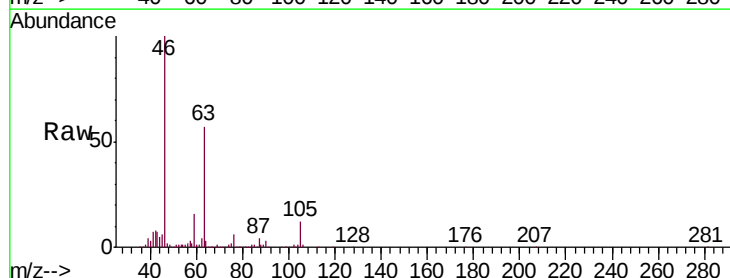

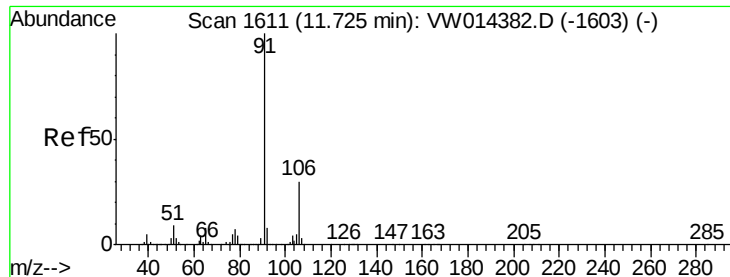

#53

Ethylbenzene

Concen: 1.054 ug/L

RT: 11.73 min Scan# 1611

Delta R.T. -0.00 min

Lab File: VW014389.D

Acq: 17 Dec 2019 13:44

Instrument :

MSVOA_W

ClientSampled :


ETK85

Tgt Ion: 91 Resp: 81246

Ion Ratio Lower Upper




91 100

106 28.4 22.3 41.5

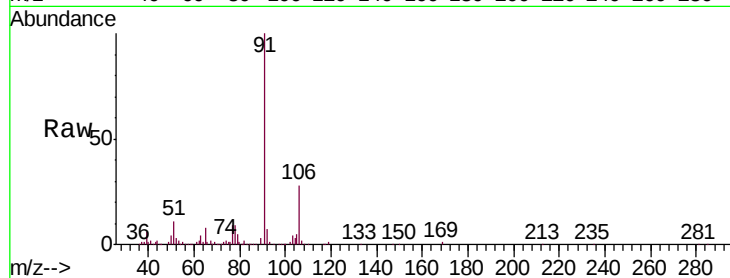

Abundance Ion 91.00 (90.70 to 91.70): VW

Ion 106.00 (105.70 to 106.70): V

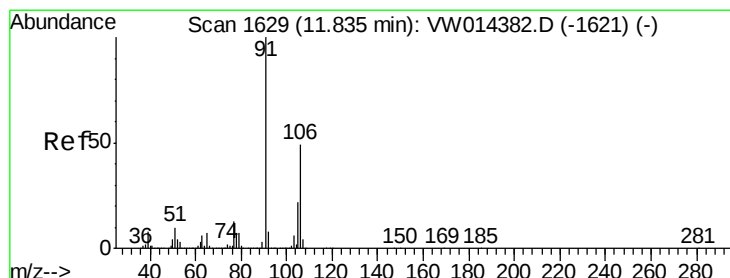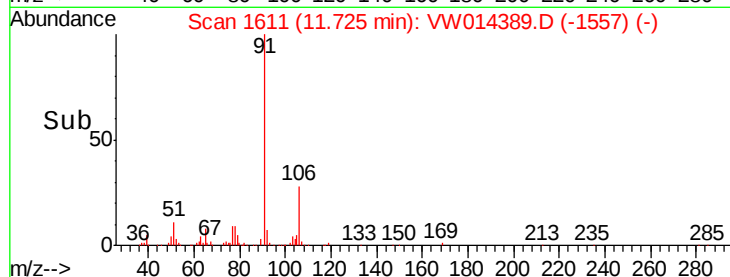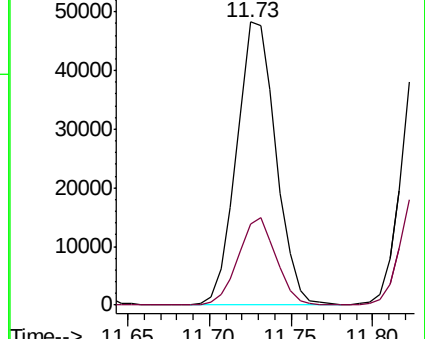

#54

m,p-Xylene

Concen: 1.700 ug/L

RT: 11.83 min Scan# 1629

Delta R.T. -0.00 min

Lab File: VW014389.D


Acq: 17 Dec 2019 13:44

Tgt Ion: 106 Resp: 50412

Ion Ratio Lower Upper



106 100


91 211.3 138.7 257.5

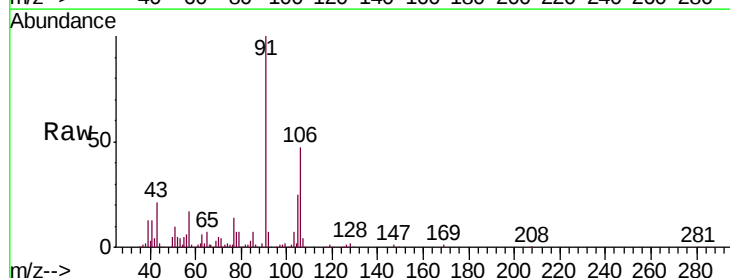

Abundance Ion 106.00 (105.70 to 106.70): V

Ion 91.00 (90.70 to 91.70): VW

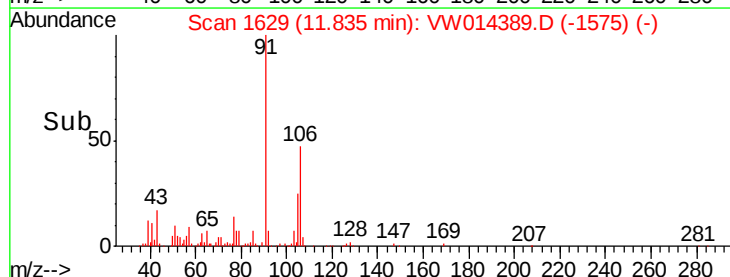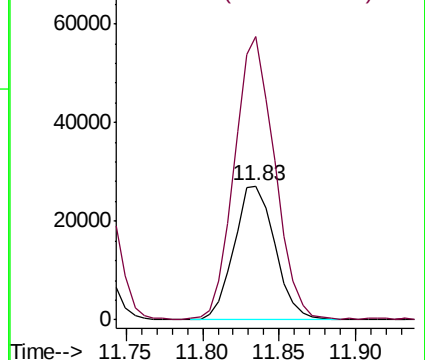

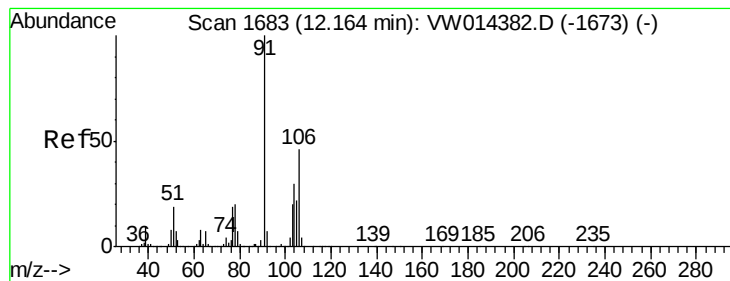

#55

o-xylene

Concen: 0.704 ug/L

RT: 12.16 min Scan# 1683

Delta R.T. -0.00 min

Lab File: VW014389.D

Acq: 17 Dec 2019 13:44

Instrument :

MSVOA_W

ClientSampleId :

ETK85

Tgt Ion:106 Resp: 19804

Ion Ratio Lower Upper

106 100

91 229.6 148.3 275.5

