

Data File : VW014390.D
Acq On : 17 Dec 2019 14:10
Operator : SY/VA
Sample : K6270-10
Misc : 5.43G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETK86

Quant Time: Dec 18 01:41:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 01:35:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1218869	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	1077423	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.56	152	479359	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	334345	18.11	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	72.44%
7) Chloroethane-d5	2.89	69	279037	20.33	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	81.32%
10) 1,1-Dichloroethene-d2	4.19	63	246	0.01	ug/L	0.17
Spiked Amount	25.000	Range	45 - 110	Recovery	=	0.04%#
20) 2-Butanone-d5	7.07	46	237409	49.36	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	98.72%
24) Chloroform-d	7.65	84	702484	22.64	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	90.56%
26) 1,2-Dichloroethane-d4	8.05	65	51	0.00	ug/L	-0.25
Spiked Amount	25.000	Range	70 - 130	Recovery	=	0.00%#
29) Benzene-d6	8.27	84	1438834	22.79	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	91.16%
33) 1,2-Dichloropropane-d6	9.27	67	462645	23.81	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	95.24%
37) Toluene-d8	10.32	98	1263728	22.13	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	88.52%
38) trans-1,3-Dichloropropene-	10.57	79	183550	22.52	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	90.08%
39) 2-Hexanone-d5	10.92	63	203114	52.58	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	105.16%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	391886	24.75	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	99.00%
61) 1,2-Dichlorobenzene-d4	13.85	152	438748	23.95	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	95.80%

Target Compounds


					Qvalue
13) Acetone	4.12	43	21280	4.589 ug/L	87
30) Cyclohexane	7.95	56	24789	0.922 ug/L #	79
34) Benzene	8.32	78	118745	1.741 ug/L	100
36) Methylcyclohexane	9.33	83	40931	1.395 ug/L #	85
44) Toluene	10.38	91	272595	3.811 ug/L	98
49) 2-Hexanone	10.93	43	28320	3.442 ug/L #	58
53) Ethylbenzene	11.73	91	93782	1.208 ug/L	96
54) m,p-Xylene	11.83	106	50495	1.691 ug/L	98
55) o-xylene	12.16	106	22466	0.793 ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data File : VW014390.D
Acq On : 17 Dec 2019 14:10
Operator : SY/VA
Sample : K6270-10
Misc : 5.43G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
ETK86

Quant Time: Dec 18 01:41:01 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 01:35:45 2019
Response via : Initial Calibration

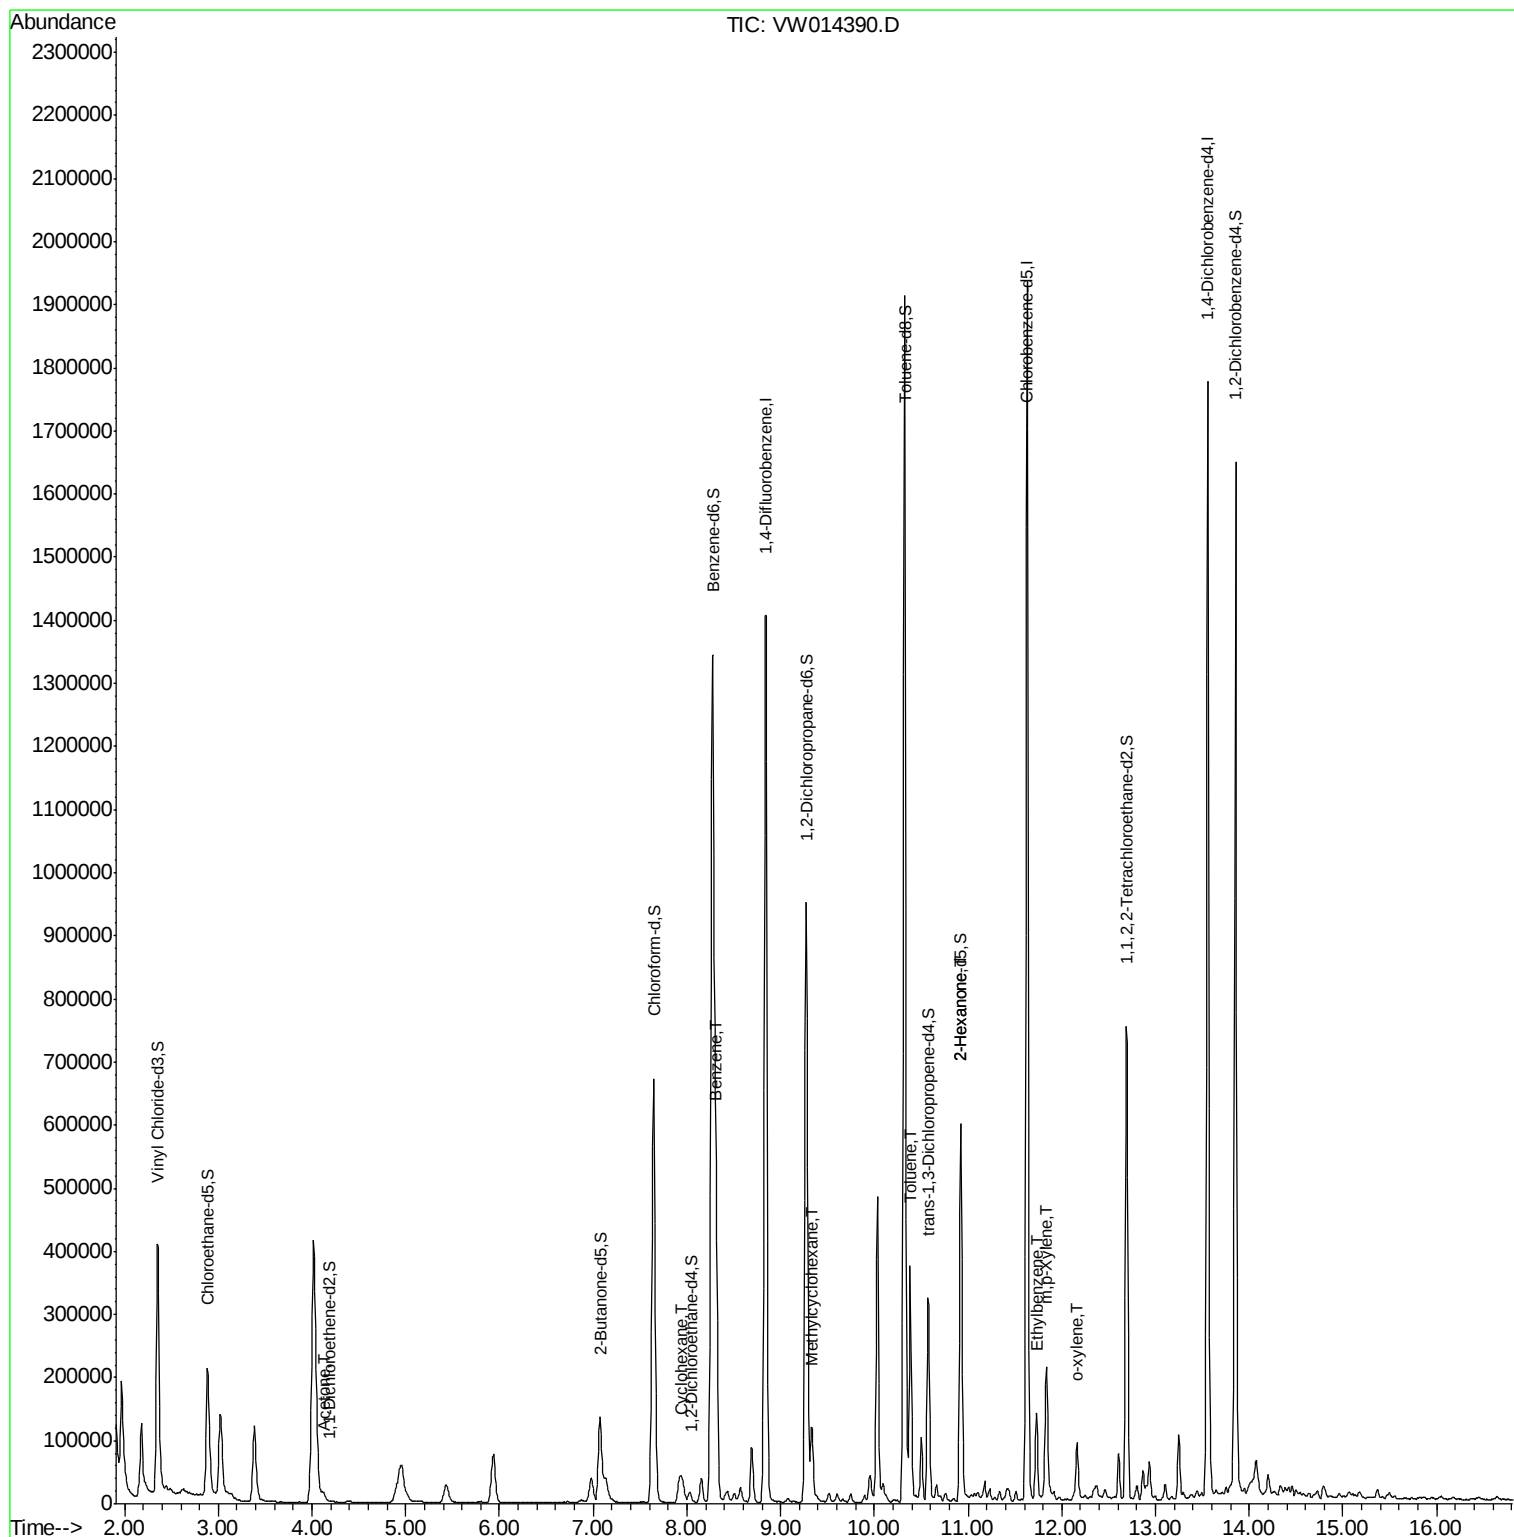

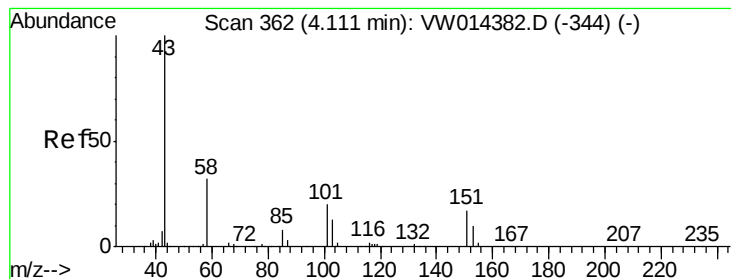

#13

Acetone

Concen: 4.589 ug/L

RT: 4.12 min Scan# 364

Delta R.T. 0.01 min

Lab File: VW014390.D

Acq: 17 Dec 2019 14:10

Instrument :

MSVOA_W

ClientSampleId :





ETK86

Tgt Ion: 43 Resp: 21280

Ion Ratio Lower Upper

43 100

58 25.3 0.0 65.4

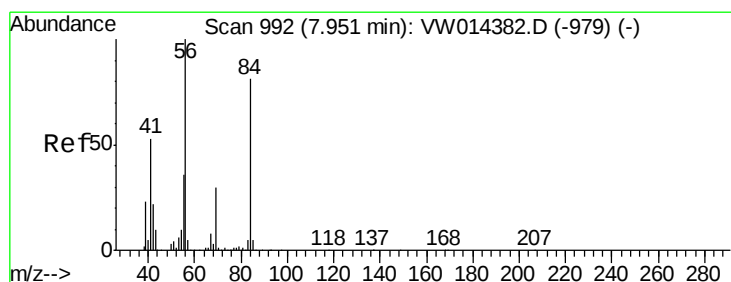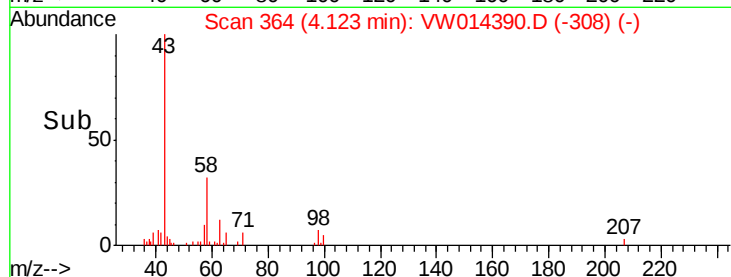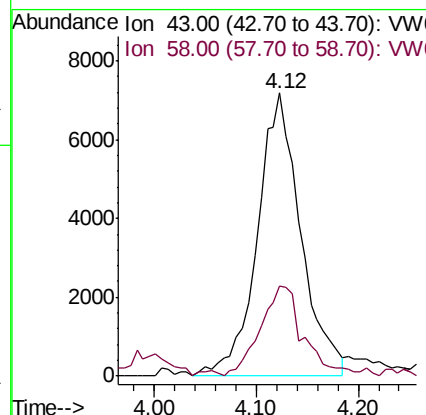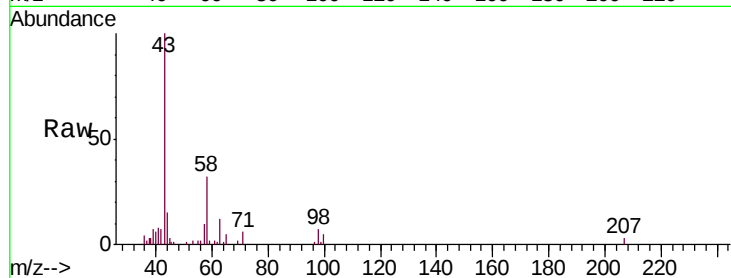

#30

Cyclohexane

Concen: 0.922 ug/L

RT: 7.95 min Scan# 992

Delta R.T. 0.00 min

Lab File: VW014390.D

Acq: 17 Dec 2019 14:10




Tgt Ion: 56 Resp: 24789


Ion Ratio Lower Upper

56 100

69 25.6 24.6 37.0

84 64.6 70.2 105.2#

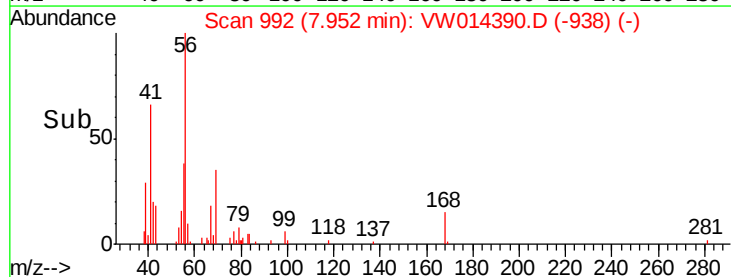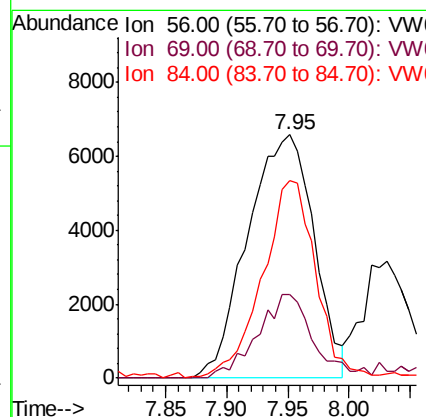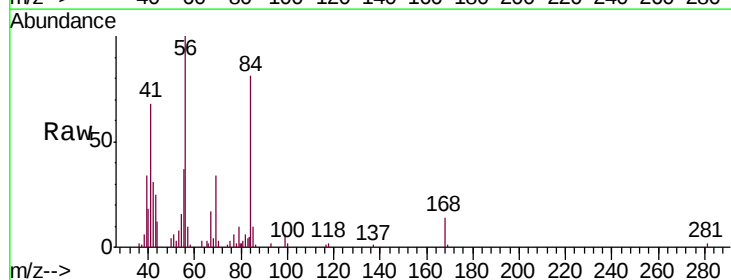

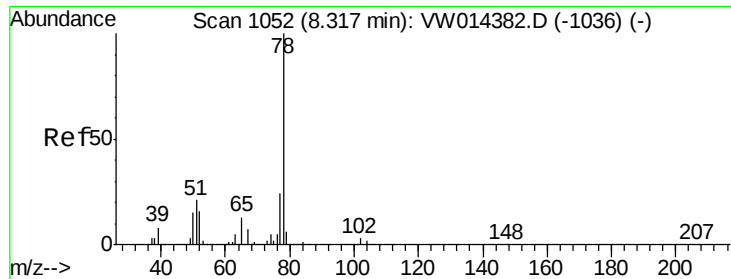

#34

Benzene

Concen: 1.741 ug/L

RT: 8.32 min Scan# 1052

Delta R.T. 0.00 min

Lab File: VW014390.D

Acq: 17 Dec 2019 14:10


Instrument :

MSVOA_W




ClientSampleId :

ETK86

Tgt Ion: 78 Resp: 118745

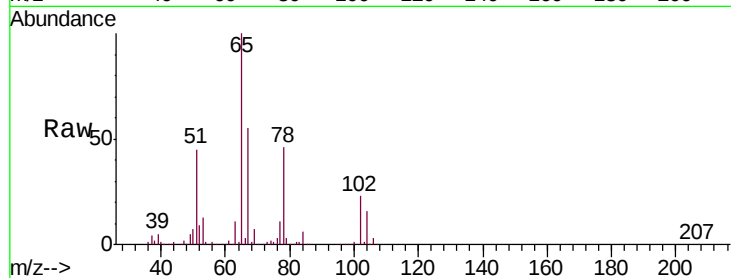

Abundance Ion 78.00 (77.70 to 78.70): VW

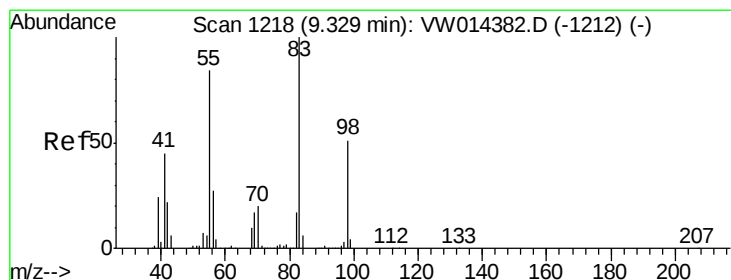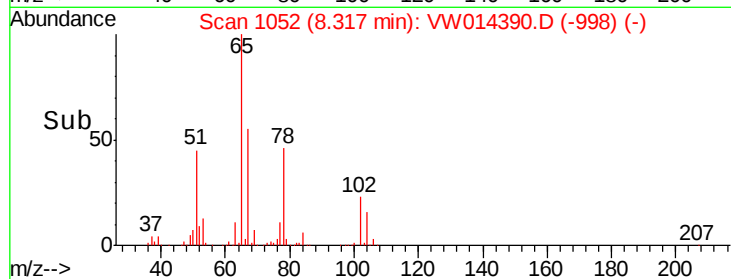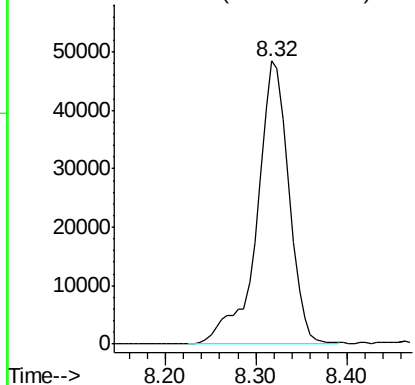

#36

Methylcyclohexane

Concen: 1.395 ug/L

RT: 9.33 min Scan# 1218


Delta R.T. 0.00 min

Lab File: VW014390.D

Acq: 17 Dec 2019 14:10

Tgt Ion: 83 Resp: 40931



Ion	Ratio	Lower	Upper
83	100		
55	95.3	59.8	89.8#
98	49.4	39.5	59.3

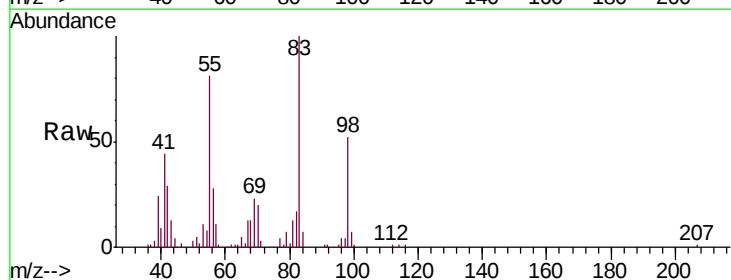


Abundance Ion 83.00 (82.70 to 83.70): VW

Ion 55.00 (54.70 to 55.70): VW

Ion 98.00 (97.70 to 98.70): VW

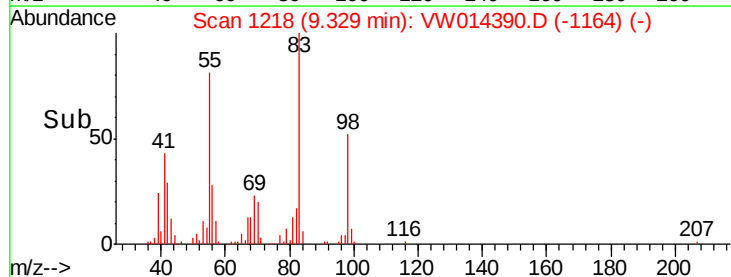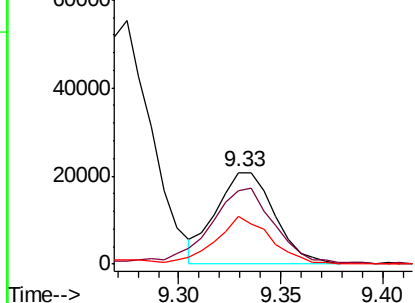

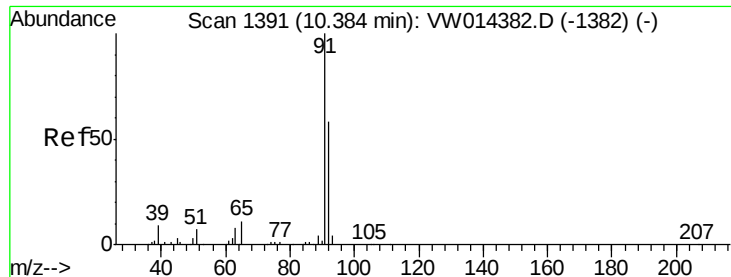

#44

Toluene

Concen: 3.811 ug/L

RT: 10.38 min Scan# 1391

Delta R.T. 0.00 min

Lab File: VW014390.D

Acq: 17 Dec 2019 14:10

Instrument :

MSVOA_W

ClientSampleId :





ETK86

Tgt Ion: 91 Resp: 272595

Ion Ratio Lower Upper

91 100

92 56.5 40.7 75.7

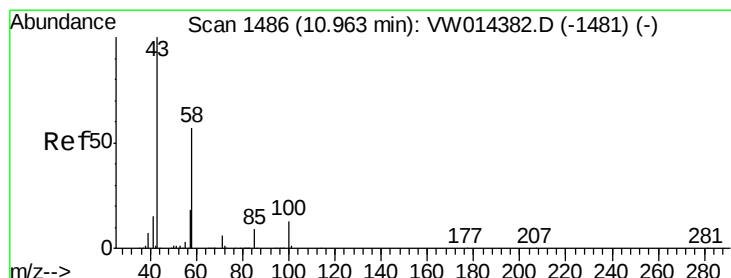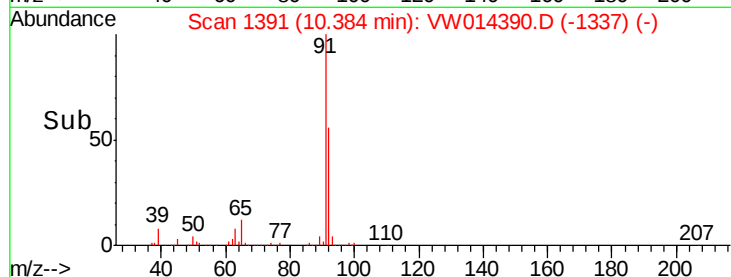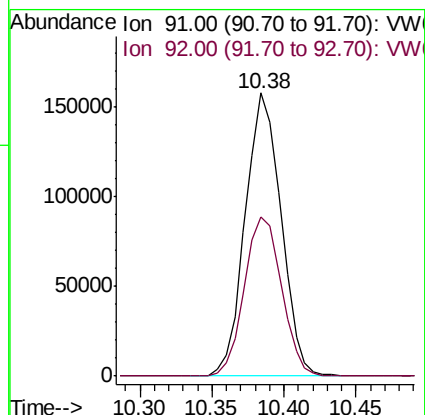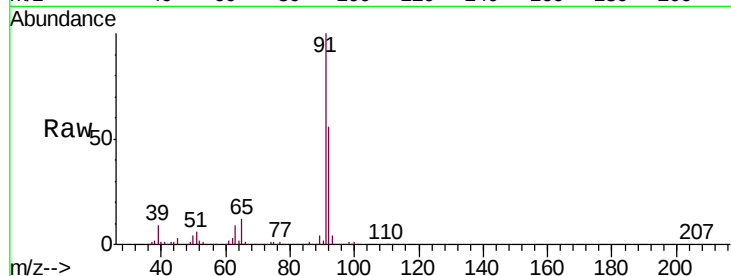

#49

2-Hexanone

Concen: 3.442 ug/L

RT: 10.93 min Scan# 1480

Delta R.T. -0.04 min

Lab File: VW014390.D

Acq: 17 Dec 2019 14:10

Tgt Ion: 43 Resp: 28320




Ion Ratio Lower Upper


43 100

58 23.7 44.4 66.6#

57 40.0 16.5 24.7#

100 0.7 11.1 16.7#


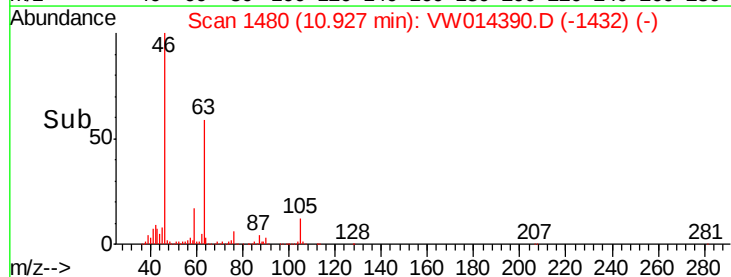
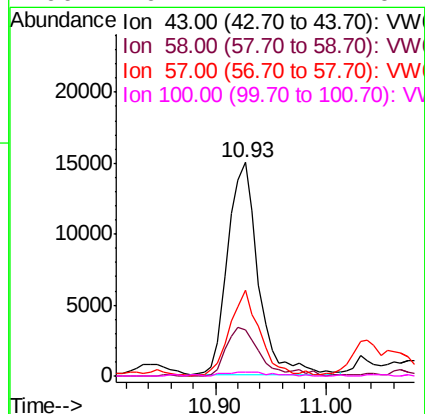
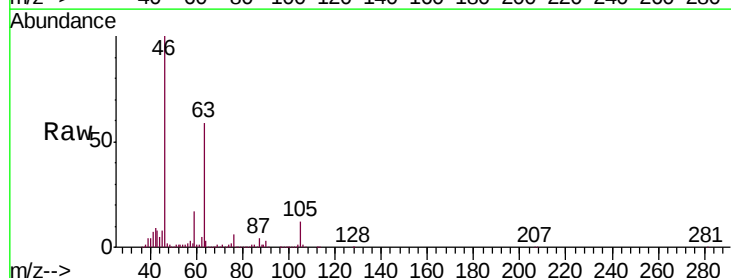


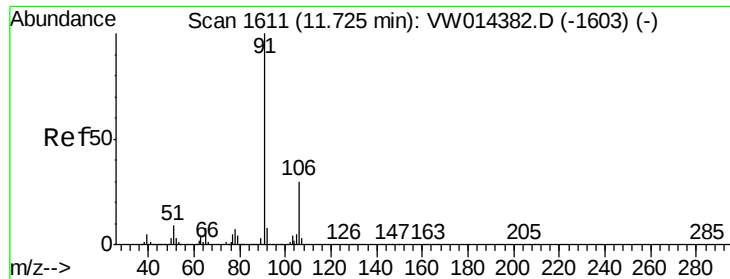

#53
Ethylbenzene
Concen: 1.208 ug/L
RT: 11.73 min Scan# 1612
Delta R.T. 0.01 min
Lab File: VW014390.D
Acq: 17 Dec 2019 14:10




Instrument :
MSVOA_W
ClientSampleId :
ETK86


Tgt Ion: 91 Resp: 93782
Ion Ratio Lower Upper
91 100
106 29.8 22.3 41.5

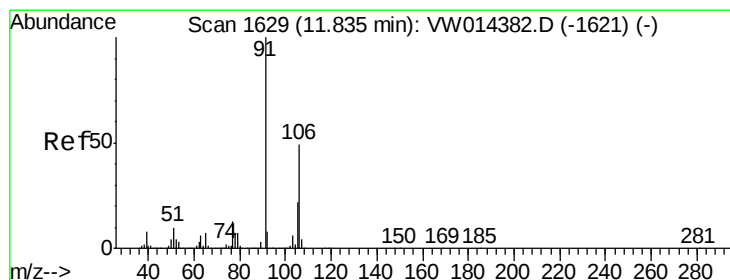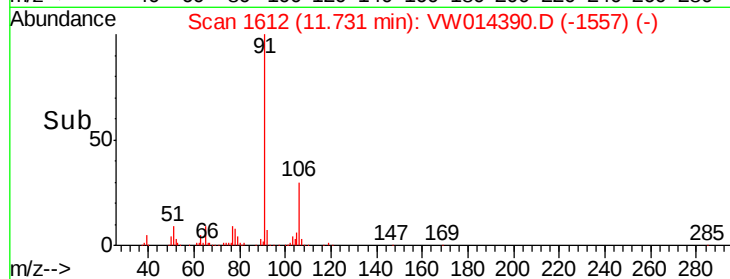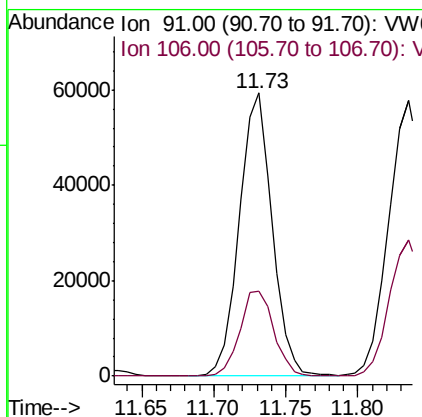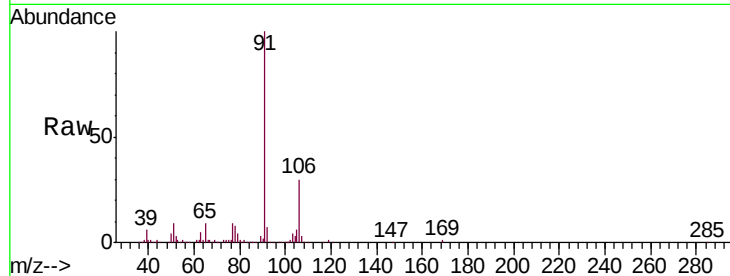

#54
m,p-Xylene
Concen: 1.691 ug/L
RT: 11.83 min Scan# 1629
Delta R.T. 0.00 min
Lab File: VW014390.D
Acq: 17 Dec 2019 14:10

Tgt Ion: 106 Resp: 50495
Ion Ratio Lower Upper
106 100
91 201.2 138.7 257.5

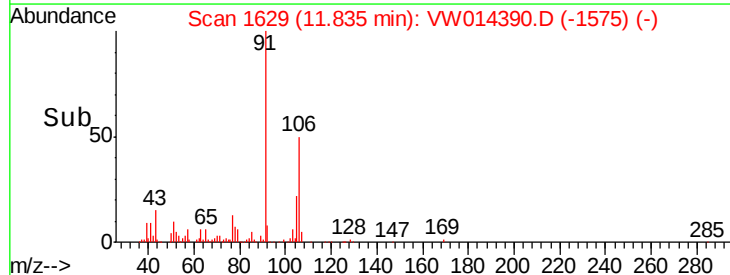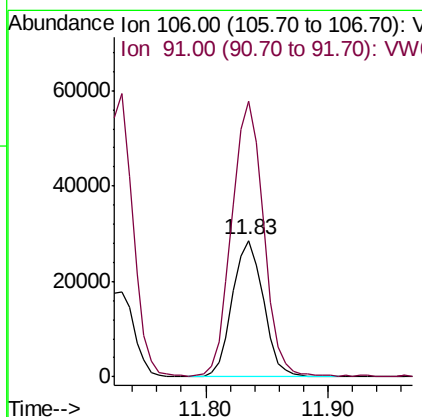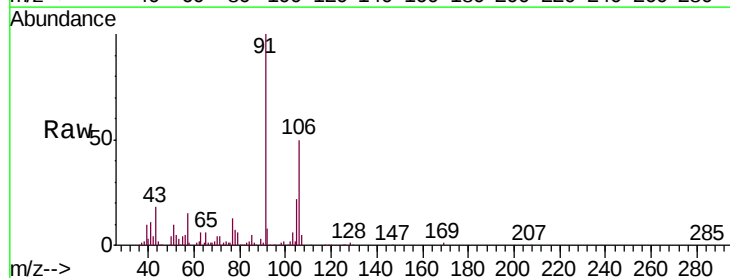

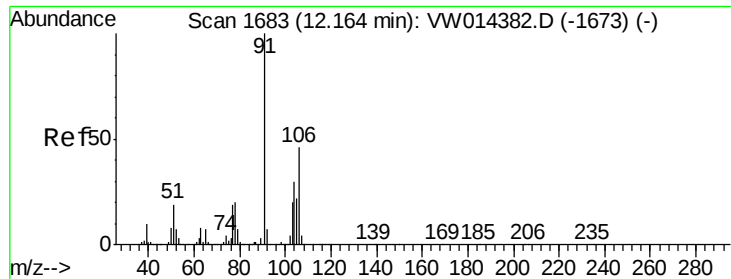

#55
o-xylene
Concen: 0.793 ug/L
RT: 12.16 min Scan# 1683
Delta R.T. 0.00 min
Lab File: VW014390.D
Acq: 17 Dec 2019 14:10

Instrument :
MSVOA_W
ClientSampleId :
ETK86

Tgt Ion:106 Resp: 22466
Ion Ratio Lower Upper
106 100
91 214.5 148.3 275.5

