

Data Path : Z:\VOASRV\HPCHEM1\MSVOA W\DATA\VW121719\
 Data File : VW014383.D
 Acq On : 17 Dec 2019 10:40
 Operator : SY/VA
 Sample : VW1217SBL01
 Misc : 5.00G/10ML/MSVOA W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK12

Quant Time: Dec 18 01:45:11 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
 Quant Title : VOC Analysis
 QLast Update : Wed Dec 18 01:35:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	1032531	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	921004	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	387476	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	292432	18.70	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	74.80%
7) Chloroethane-d5	2.89	69	243865	20.98	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	83.92%
10) 1,1-Dichloroethene-d2	4.01	63	432815	15.67	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	62.68%
20) 2-Butanone-d5	7.07	46	207415	50.91	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	101.82%
24) Chloroform-d	7.64	84	588783	22.40	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	89.60%
26) 1,2-Dichloroethane-d4	8.30	65	324365	23.53	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	94.12%
29) Benzene-d6	8.27	84	1215569	22.52	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	90.08%
33) 1,2-Dichloropropane-d6	9.27	67	382263	23.02	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	92.08%
37) Toluene-d8	10.32	98	1054594	21.61	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	86.44%
38) trans-1,3-Dichloropropene-	10.57	79	144521	20.74	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	82.96%
39) 2-Hexanone-d5	10.92	63	149248	45.20	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.40%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	303439	22.42	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	89.68%
61) 1,2-Dichlorobenzene-d4	13.85	152	338920	22.89	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	91.56%


Target Compounds					Ovalue
13) Acetone	4.12	43	14637	3.726 ug/L	82


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA W\DATA\VW121719\
Data File : VW014383.D
Acq On : 17 Dec 2019 10:40
Operator : SY/VA
Sample : VW1217SBL01
Misc : 5.00G/10ML/MSVOA W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
VBLK12

Quant Time: Dec 18 01:45:11 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Wed Dec 18 01:35:45 2019
Response via : Initial Calibration

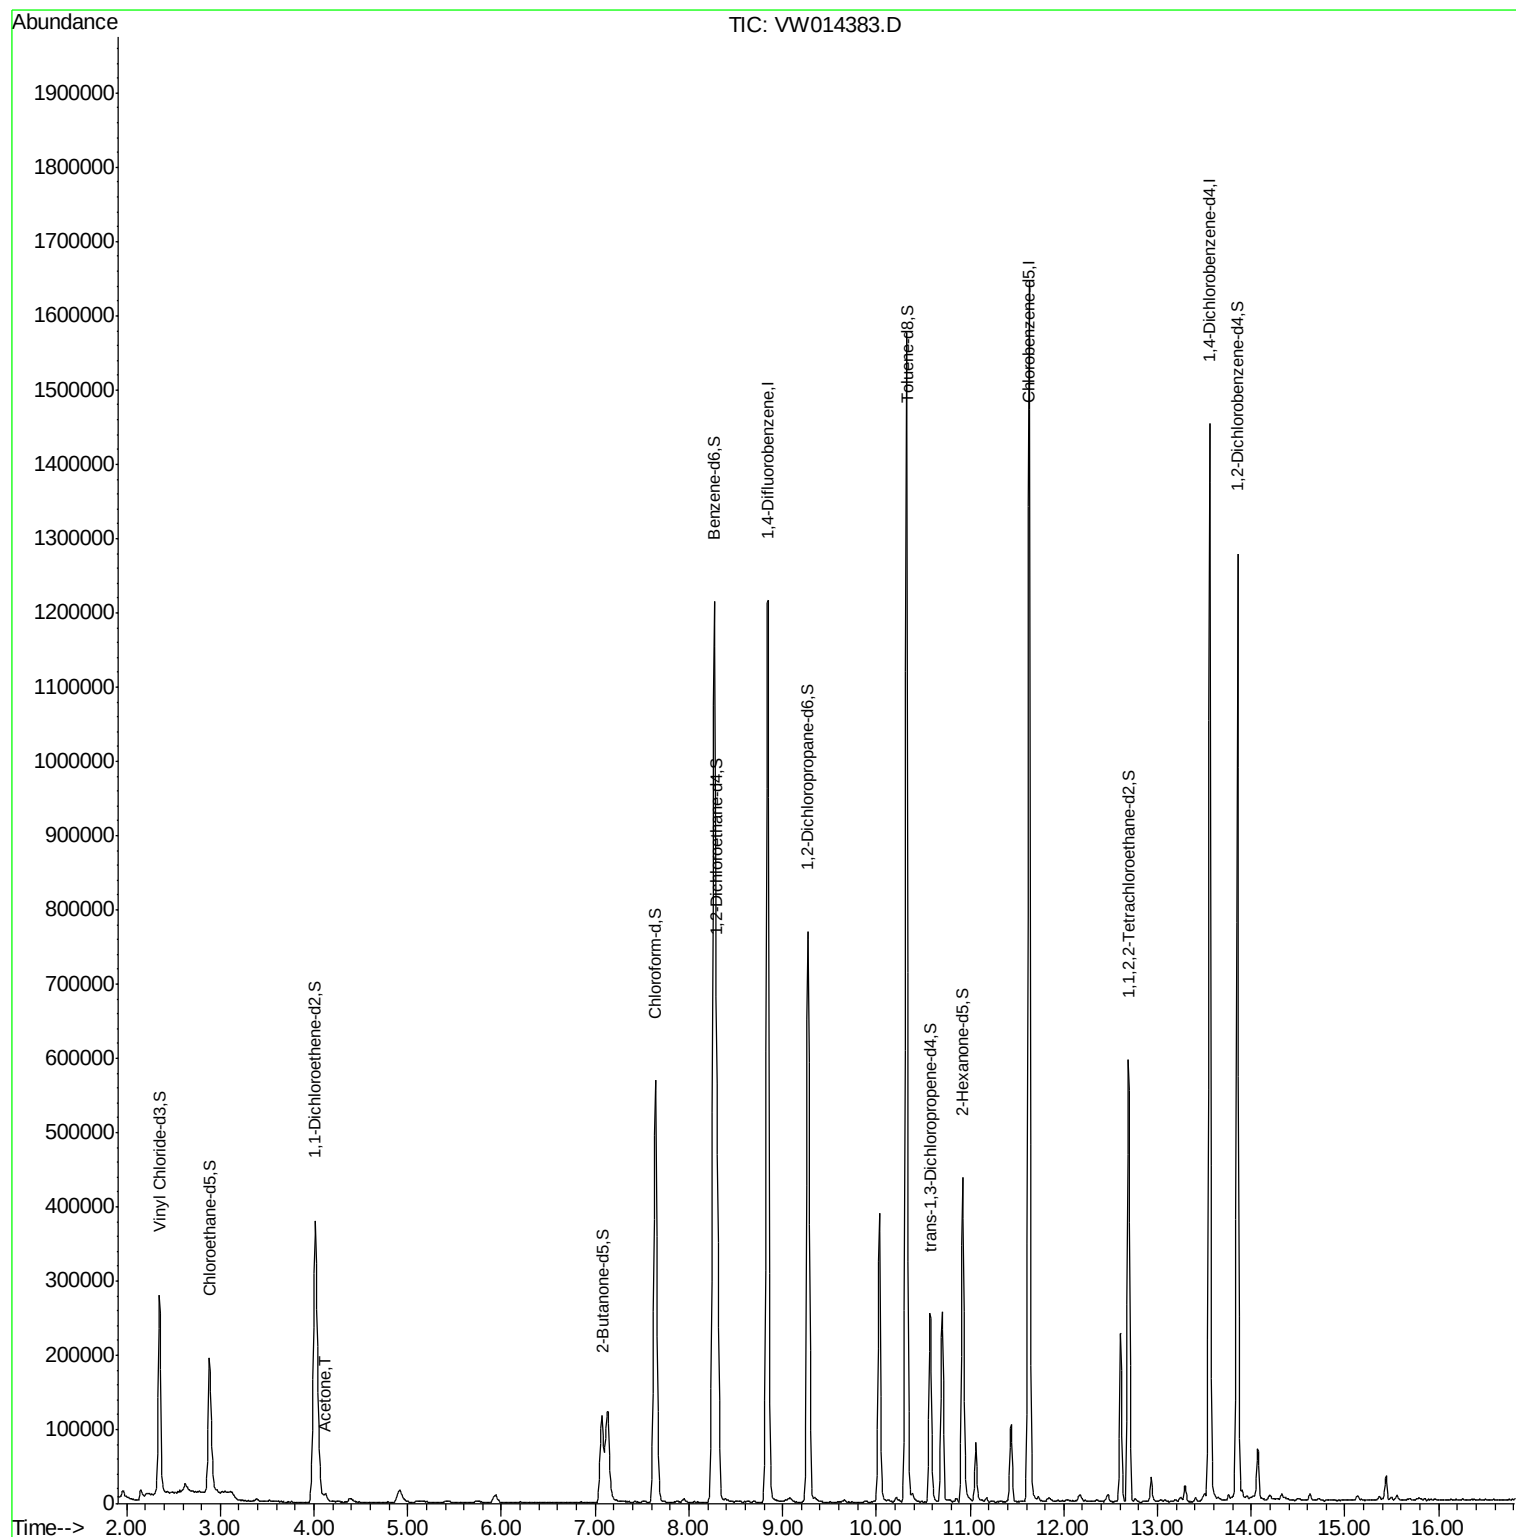

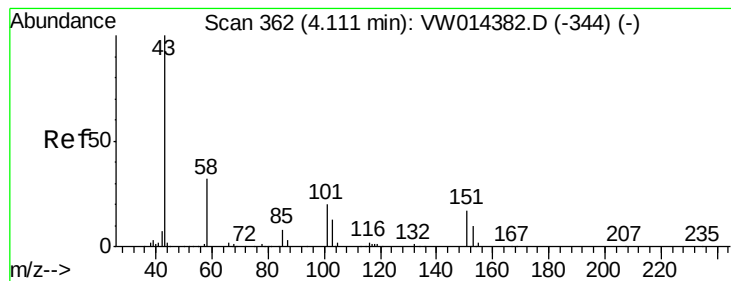

#13
 Acetone
 Concen: 3.726 ug/L
 RT: 4.12 min Scan# 363
 Delta R.T. 0.01 min
 Lab File: VW014383.D
 Acq: 17 Dec 2019 10:40

Instrument :
 MSVOA_W
 ClientSampleId :
 VBLK12

Tot Ion: 43 Resp: 14637
 Ion Ratio Lower Upper
 43 100
 58 22.5 0.0 65.4

