


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121721\
 Data File : VW021419.D
 Acq On : 17 Dec 2021 08:35
 Operator : SY/VA
 Sample : BFB483
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Title : SFAM01.0
 Last Update : Fri Dec 17 00:58:26 2021

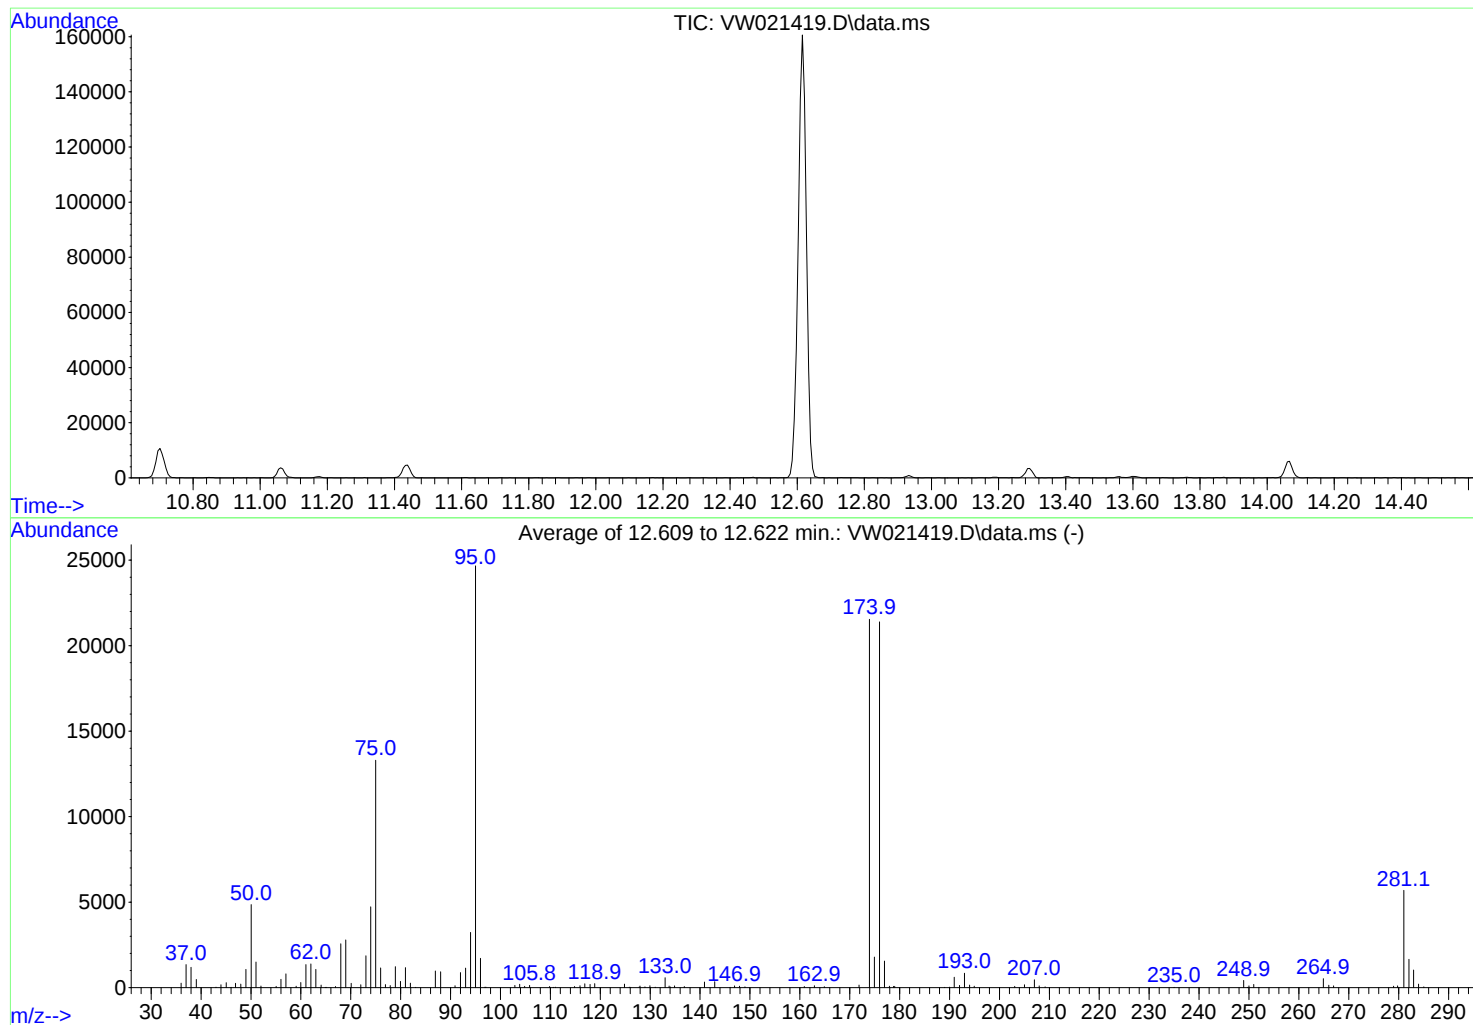

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	4856	PASS
75	95	30	80	53.9	13300	PASS
95	95	100	100	100.0	24667	PASS
96	95	5	9	7.0	1715	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.3	21541	PASS
175	174	5	9	8.3	1788	PASS
176	174	95	105	99.3	21387	PASS
177	176	5	10	7.3	1558	PASS