
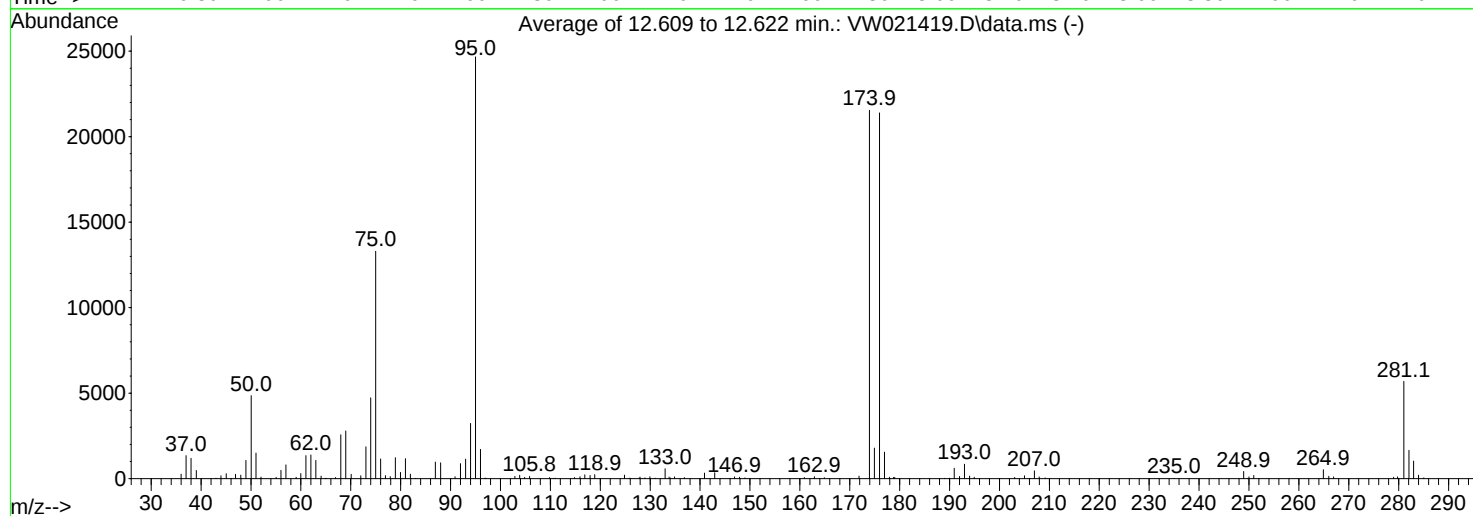


Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121721\
 Data File : VW021419.D
 Acq On : 17 Dec 2021 08:35
 Operator : SY/VA
 Sample : BFB483
 Misc : 5.00g/10.0mL/MSVOA_W/SOIL
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 BFB483

Integration File: LSCINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM120921SMA.M
 Title : SFAM01.0
 Last Update : Fri Dec 24 01:43:02 2021

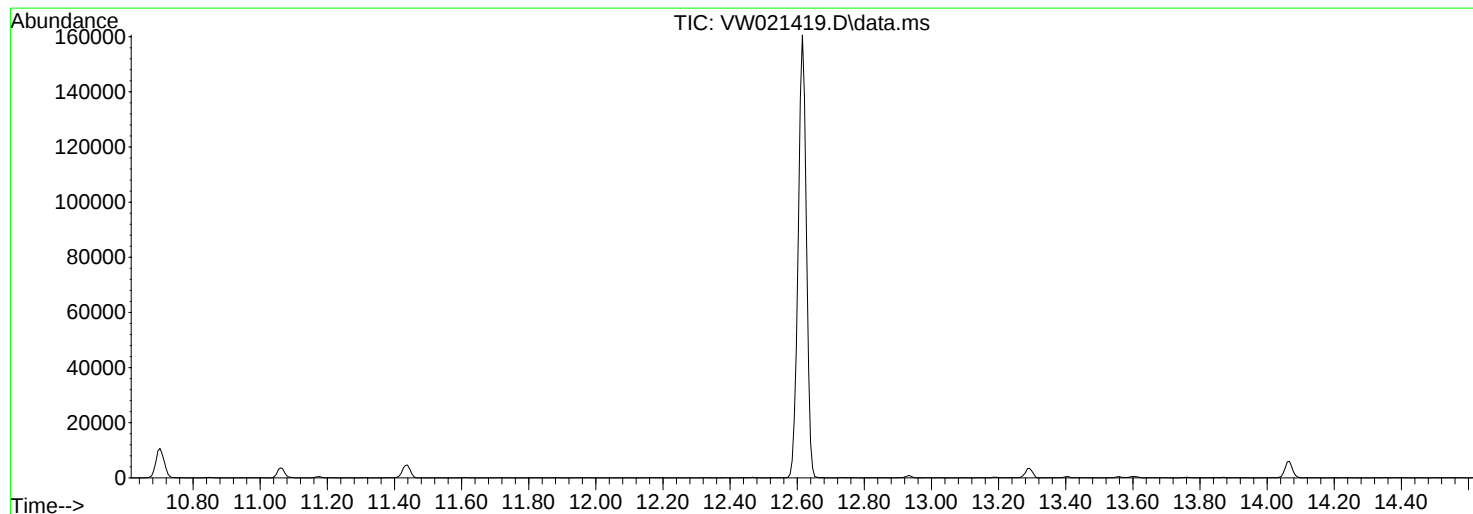

AutoFind: Scans 1756, 1757, 1758; Background Corrected with Scan 1749

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.7	4856	PASS
75	95	30	80	53.9	13300	PASS
95	95	100	100	100.0	24667	PASS
96	95	5	9	7.0	1715	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	120	87.3	21541	PASS
175	174	5	9	8.3	1788	PASS
176	174	95	105	99.3	21387	PASS
177	176	5	10	7.3	1558	PASS

m/z	Abundance
44.00	59.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

m/z	Abundance
36.00	282.0
37.00	1353.0
38.00	1209.0
39.00	449.0
43.00	73.0
44.00	200.0
45.00	359.0
46.90	265.0
48.00	225.0
49.00	1021.0
50.00	4772.0
51.00	1408.0
52.00	101.0
55.10	72.0
56.00	449.0
57.00	661.0
59.10	141.0
60.00	271.0
61.00	1263.0
62.00	1390.0
63.00	1029.0
64.10	136.0
66.90	94.0
68.00	2329.0
69.00	2648.0
70.10	261.0
72.00	167.0
73.00	2139.0
74.00	4302.0
75.00	12364.0
76.00	1137.0
77.00	206.0
77.90	84.0
79.00	1111.0
79.90	331.0
81.00	1036.0
82.00	237.0
83.00	60.0
86.90	957.0
88.00	827.0
90.90	98.0
92.00	791.0
93.00	1059.0
94.00	2977.0
95.00	22056.0
96.00	1690.0
96.90	73.0
103.00	187.0
103.90	204.0
104.80	75.0
105.90	122.0
109.80	105.0
110.60	59.0
111.00	82.0
114.90	69.0
115.90	124.0
117.00	217.0
117.90	184.0
118.90	281.0
124.80	251.0
126.10	68.0
127.80	117.0
130.00	101.0
131.00	72.0
133.00	870.0
133.80	283.0
134.90	131.0
136.80	62.0
140.90	254.0
142.90	315.0
146.90	161.0
147.90	72.0
149.00	77.0
160.90	110.0
163.00	95.0
164.90	117.0
171.90	155.0
174.00	18000.0
174.90	1358.0
175.90	15848.0
177.00	1444.0
178.10	92.0
178.80	214.0
189.00	65.0
190.00	87.0
191.00	1008.0
192.10	190.0
193.00	1258.0
194.00	220.0
194.90	82.0
203.10	153.0
205.10	233.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

206.10	59.0
207.00	661.0
208.00	119.0
209.10	85.0
235.00	68.0
249.00	659.0
250.00	163.0
251.00	311.0
252.00	57.0
264.90	800.0
266.10	234.0
267.00	199.0
279.00	98.0
279.80	236.0
281.10	8179.0
282.10	2363.0
283.00	1311.0
284.00	273.0
285.00	87.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

m/z	Abundance
36.00	269.0
37.00	1446.0
38.00	1278.0
39.10	516.0
44.00	203.0
45.00	243.0
46.90	334.0
48.00	215.0
49.00	1158.0
50.00	5381.0
51.00	1781.0
52.00	62.0
55.00	90.0
56.00	601.0
57.00	961.0
59.00	115.0
60.00	347.0
61.00	1483.0
62.00	1482.0
63.00	1178.0
64.00	155.0
64.90	58.0
67.00	96.0
68.00	2924.0
69.00	3074.0
70.10	241.0
72.00	167.0
73.10	2065.0
74.00	5281.0
75.00	14868.0
76.00	1274.0
76.90	175.0
77.90	132.0
78.90	1305.0
79.90	425.0
80.90	1318.0
81.90	294.0
87.00	1005.0
88.00	1041.0
90.80	125.0
92.00	917.0
93.00	1219.0
94.00	3412.0
95.00	27608.0
96.00	1970.0
97.10	76.0
102.90	133.0
103.90	210.0
104.90	88.0
105.90	132.0
109.90	80.0
114.80	90.0
116.00	113.0
116.80	251.0
118.00	213.0
118.90	197.0
124.90	236.0
125.80	72.0
128.00	109.0
128.90	83.0
130.00	141.0
133.00	549.0
134.10	111.0
135.00	105.0
136.90	77.0
140.90	341.0
142.90	385.0
146.00	52.0
146.90	81.0
147.90	110.0
149.00	54.0
160.90	94.0
162.90	179.0
164.90	61.0
171.80	142.0
174.00	21112.0
175.00	2023.0
176.00	26960.0
176.90	1751.0
177.90	105.0
179.00	145.0
191.00	590.0
191.90	132.0
193.00	824.0
194.00	176.0
195.00	121.0
203.00	72.0
204.90	188.0
207.00	456.0
207.90	136.0
209.20	61.0
248.90	404.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

250.00	148.0
250.90	154.0
264.90	576.0
265.90	175.0
266.90	114.0
279.10	92.0
281.00	6421.0
282.00	1454.0
283.00	1086.0
284.00	224.0
285.10	55.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483

m/z	Abundance
36.00	232.0
37.00	1244.0
38.00	1090.0
39.00	463.0
44.00	271.0
45.10	272.0
46.00	52.0
47.00	158.0
47.90	183.0
49.00	1032.0
50.10	4416.0
51.00	1318.0
52.00	107.0
55.00	66.0
56.00	407.0
57.00	781.0
60.00	284.0
61.00	1287.0
62.00	1286.0
63.00	988.0
64.10	158.0
65.10	65.0
68.00	2430.0
69.00	2648.0
70.10	249.0
72.00	162.0
73.00	1390.0
74.00	4607.0
75.00	12669.0
76.00	1054.0
77.00	165.0
77.90	142.0
78.90	1250.0
80.00	335.0
80.90	1156.0
81.90	250.0
86.90	953.0
88.00	913.0
91.00	112.0
92.00	921.0
93.00	1153.0
94.00	3292.0
95.00	24336.0
96.00	1484.0
102.80	71.0
103.80	183.0
104.80	69.0
105.80	143.0
114.90	52.0
115.90	97.0
116.90	220.0
117.90	163.0
118.90	233.0
124.80	74.0
125.00	70.0
127.90	174.0
129.00	60.0
129.80	110.0
133.00	311.0
134.80	65.0
136.90	53.0
140.90	393.0
143.00	347.0
146.80	68.0
147.80	60.0
162.80	69.0
171.90	151.0
173.90	25512.0
174.90	1982.0
175.90	21352.0
177.00	1479.0
177.80	53.0
179.00	85.0
190.80	230.0
192.10	65.0
193.00	441.0
194.00	54.0
195.00	56.0
204.90	83.0
207.00	263.0
207.90	58.0
249.00	188.0
249.70	53.0
250.90	83.0
265.00	200.0
278.90	66.0
279.80	85.0
281.00	2454.0
282.00	1142.0
283.00	705.0
284.00	118.0

Instrument :
MSVOA_W
ClientSampleId :
BFB483