

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121724\
 Data File : VW031319.D
 Acq On : 17 Dec 2024 15:49
 Operator : SY/MD
 Sample : P5258-16
 Misc : 4.20g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :

Quant Time: Dec 18 00:19:33 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 18 00:14:15 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	8.837	114	991710	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117	649795	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.556	152	176821	25.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	2.363	65	262512	17.593	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	70.360%
7) Chloroethane-d5	2.899	69	207510	18.800	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.200%
11) 1,1-Dichloroethene-d2	4.015	65	116677	16.485	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	65.920%
21) 2-Butanone-d5	7.094	46	93055	33.115	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	66.220%
24) Chloroform-d	7.648	84	474632	17.468	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	69.880%
26) 1,2-Dichloroethane-d4	8.301	65	263102	19.280	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	77.120%
32) Benzene-d6	8.270	84	932340	22.386	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	89.560%
36) 1,2-Dichloropropane-d6	9.270	67	284662	23.452	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	93.800%
41) Toluene-d8	10.319	98	737284	19.029	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	76.120%
43) trans-1,3-Dichloroprop...	10.575	79	97050	17.340	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	69.360%
47) 2-Hexanone-d5	10.922	63	73772	45.193	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	90.380%
56) 1,1,2,2-Tetrachloroeth...	12.690	84	173264	22.735	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.920%
66) 1,2-Dichlorobenzene-d4	13.848	152	113846	17.343	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	69.360%#
Target Compounds						
39) cis-1,3-Dichloropropene	10.032	75	7794	0.460	ug/L	Qvalue # 66


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121724\
Data File : VW031319.D
Acq On : 17 Dec 2024 15:49
Operator : SY/MD
Sample : P5258-16
Misc : 4.20g/10mL/MSVOA_W/SOIL/A
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :


Quant Time: Dec 18 00:19:33 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 18 00:14:15 2024
Response via : Initial Calibration

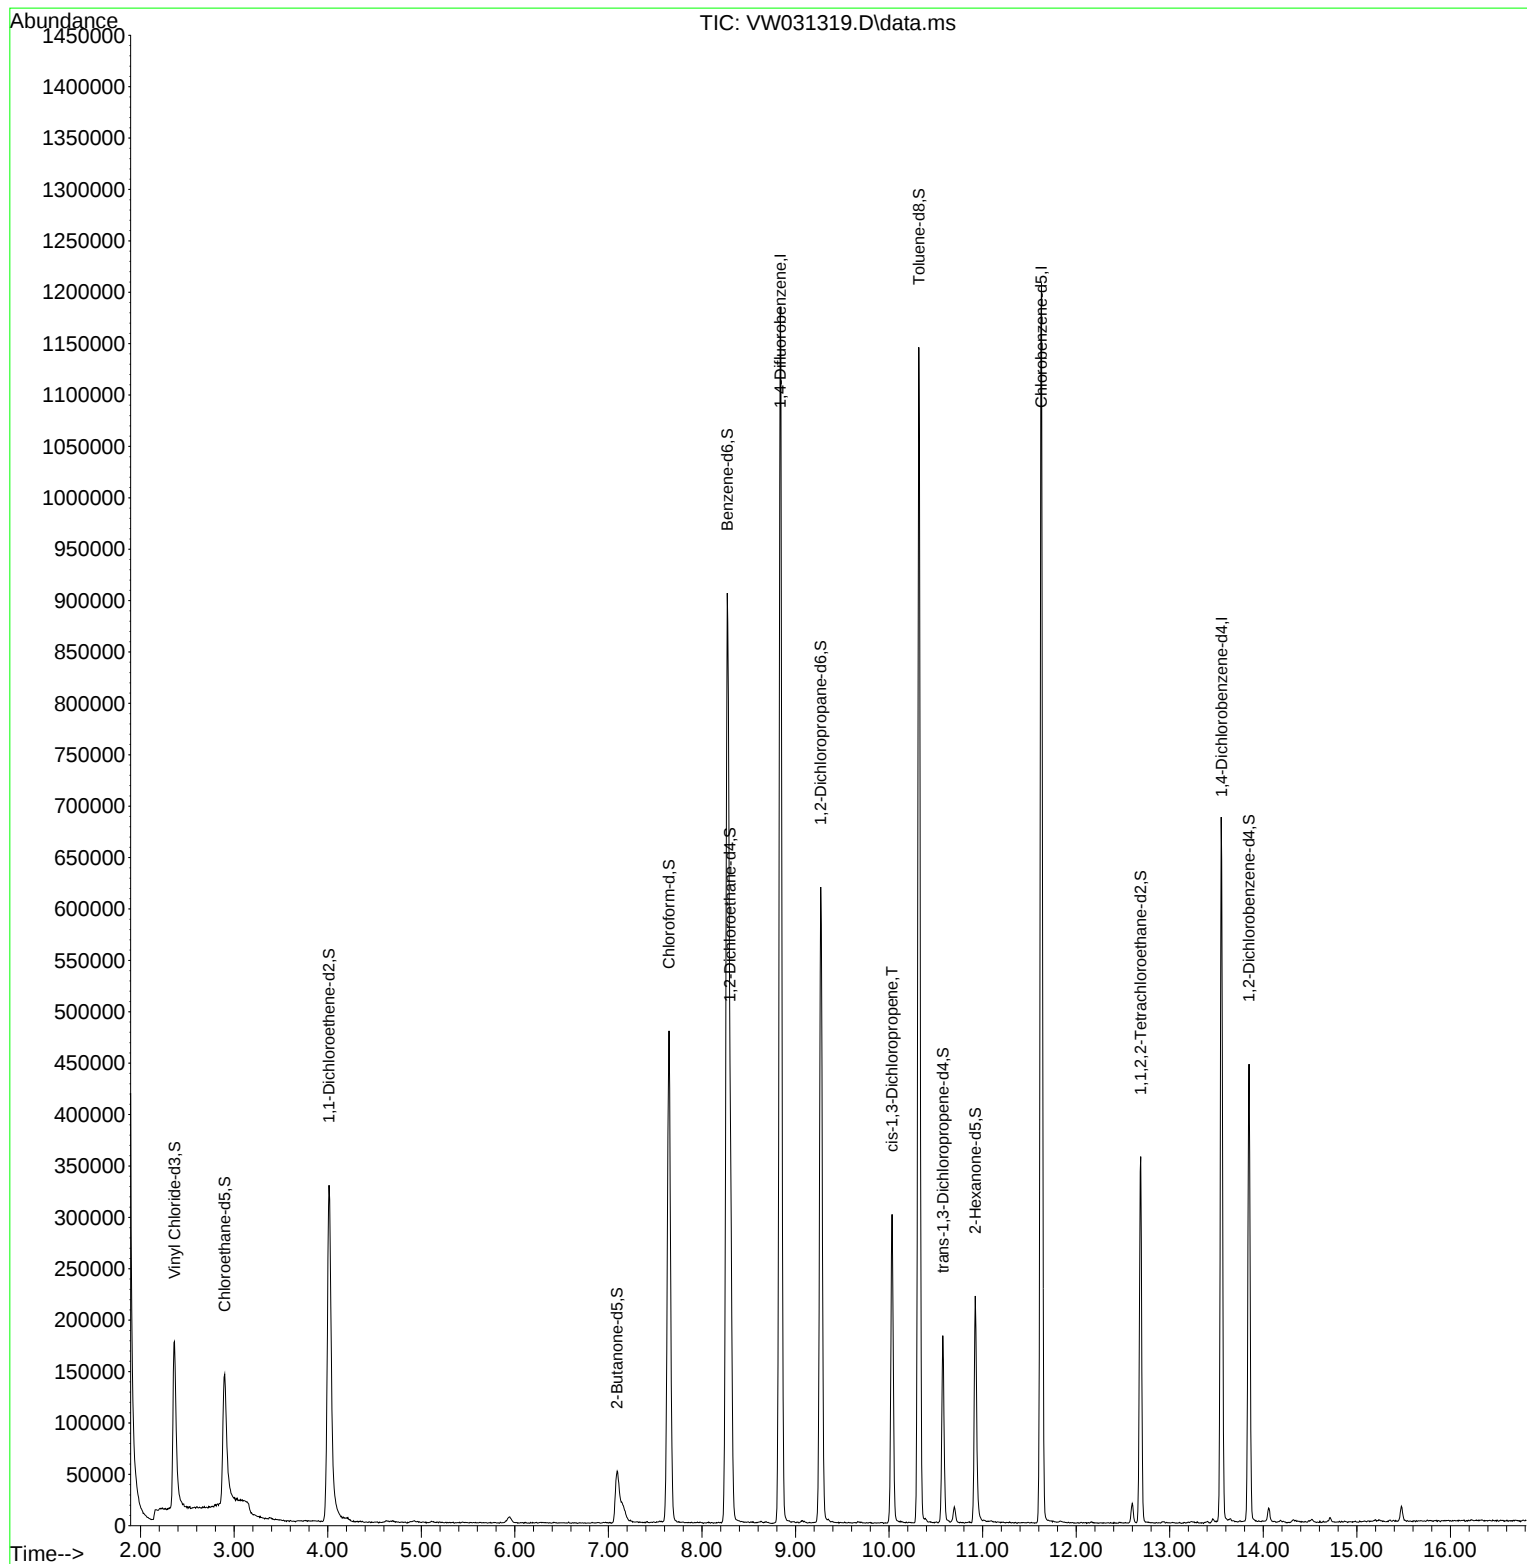

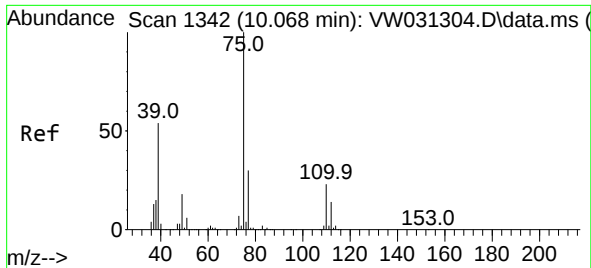

#39
 cis-1,3-Dichloropropene
 Concen: 0.460 ug/L
 RT: 10.032 min Scan# 11
 Delta R.T. -0.036 min
 Lab File: VW031319.D
 Acq: 17 Dec 2024 15:49

Instrument :
 MSVOA_W
 ClientSampleId :

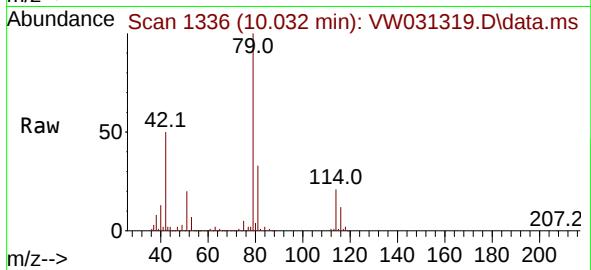

Tgt Ion: 75 Resp: 7794
 Ion Ratio Lower Upper
 75 100
 77 49.6 21.8 40.4#

