




Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121724\
Data File : VW031322.D
Acq On : 17 Dec 2024 17:01
Operator : SY/MD
Sample : P5258-21
Misc : 4.27g/10mL/MSVOA_W/SOIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Y4

Manual IntegrationsAPPROVED

Quant Time: Dec 18 00:20:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 18 00:14:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2024
Supervised By :Semsettin Yesilyurt 12/18/2024

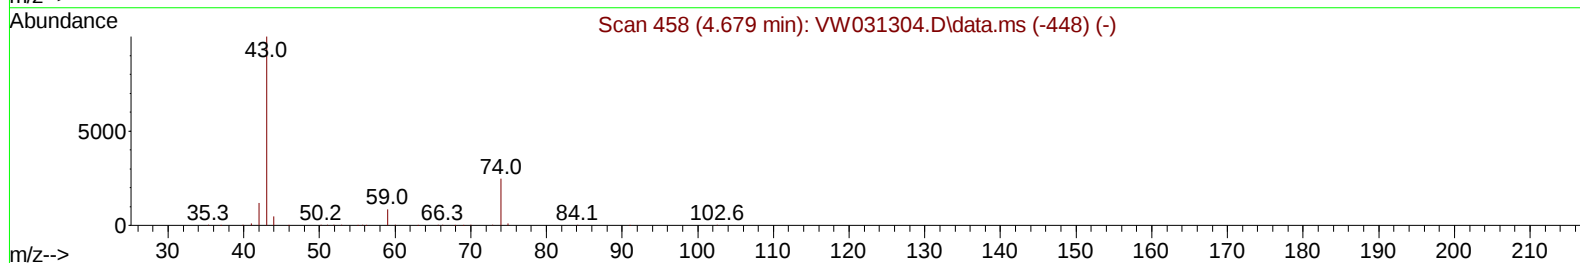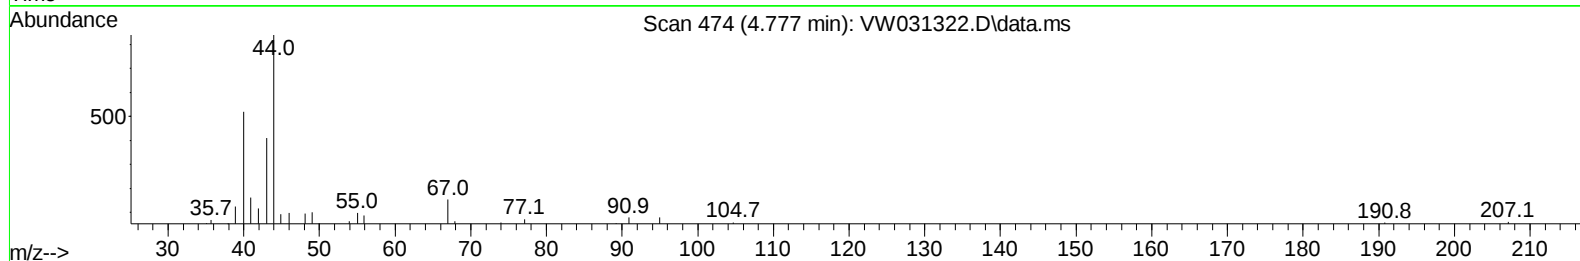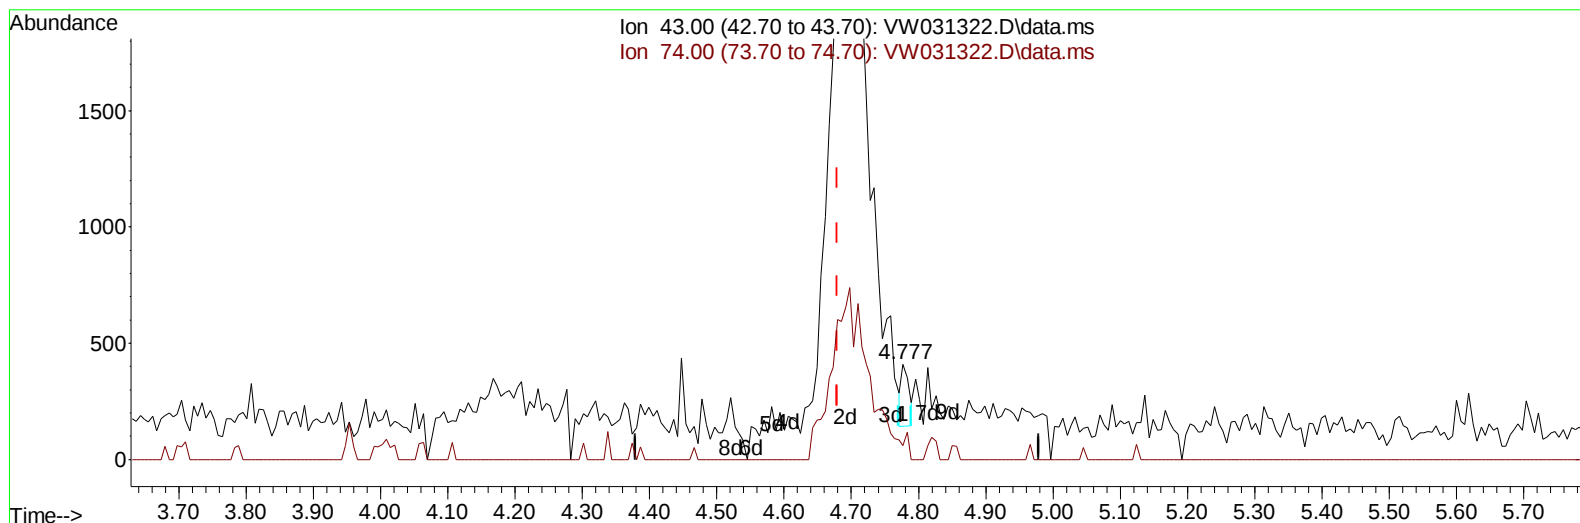

TIC: VW031322.D\data.ms

(15) Methyl Acetate (T)

4.777min (+ 0.098) 0.09 ug/L

response 210

Ion	Exp%	Act%
43.00	100.00	100.00
74.00	23.60	20.48
0.00	0.00	0.00
0.00	0.00	0.00

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\Vw121724\
 Data File : VW031322.D
 Acq On : 17 Dec 2024 17:01
 Operator : SY/MD
 Sample : P5258-21
 Misc : 4.27g/10mL/MSVOA_W/SOIL/A
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_W
 ClientSampleId :
 E28Y4

Manual IntegrationsAPPROVED

Quant Time: Dec 18 00:20:14 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
 Quant Title : SFAM01.0
 QLast Update : Wed Dec 18 00:14:15 2024
 Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2024
 Supervised By :Semsettin Yesilyurt 12/18/2024

Compound	R.T.	Q	Ion	Response	Conc	Units	Dev(Min)

Internal Standards							
1) 1,4-Difluorobenzene	8.837	114		551163	25.000	ug/L	0.00
28) Chlorobenzene-d5	11.629	117		213573	25.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	13.550	152		32700	25.000	ug/L	0.00
System Monitoring Compounds							
4) Vinyl Chloride-d3	2.363	65		235772	28.431	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	113.720%	
7) Chloroethane-d5	2.899	69		178619	29.117	ug/L	0.00
Spiked Amount 25.000	Range 30	- 150		Recovery	=	116.480%	
11) 1,1-Dichloroethene-d2	4.015	65		89805	22.830	ug/L	0.00
Spiked Amount 25.000	Range 45	- 110		Recovery	=	91.320%	
21) 2-Butanone-d5	7.094	46		68478	43.847	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	87.700%	
24) Chloroform-d	7.648	84		312092	20.666	ug/L	0.00
Spiked Amount 25.000	Range 40	- 150		Recovery	=	82.680%	
26) 1,2-Dichloroethane-d4	8.307	65		179803	23.708	ug/L	0.00
Spiked Amount 25.000	Range 70	- 130		Recovery	=	94.840%	
32) Benzene-d6	8.270	84		578659	42.272	ug/L	0.00
Spiked Amount 25.000	Range 20	- 135		Recovery	=	169.080%#	
36) 1,2-Dichloropropane-d6	9.270	67		167362	41.950	ug/L	0.00
Spiked Amount 25.000	Range 70	- 120		Recovery	=	167.800%#	
41) Toluene-d8	10.319	98		316202	24.830	ug/L	0.00
Spiked Amount 25.000	Range 30	- 130		Recovery	=	99.320%	
43) trans-1,3-Dichloroprop...	10.575	79		41804	22.725	ug/L	0.00
Spiked Amount 25.000	Range 30	- 135		Recovery	=	90.920%	
47) 2-Hexanone-d5	10.922	63		43410	80.910	ug/L	0.00
Spiked Amount 50.000	Range 20	- 135		Recovery	=	161.820%#	
56) 1,1,2,2-Tetrachloroeth...	12.684	84		85316	34.059	ug/L	0.00
Spiked Amount 25.000	Range 45	- 120		Recovery	=	136.240%#	
66) 1,2-Dichlorobenzene-d4	13.848	152		23940	19.721	ug/L	0.00
Spiked Amount 25.000	Range 75	- 120		Recovery	=	78.880%	
Target Compounds							Qvalue
15) Methyl Acetate	4.692	43		11242m	4.551	ug/L	

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_W\Data\VW121724\
Data File : VW031322.D
Acq On : 17 Dec 2024 17:01
Operator : SY/MD
Sample : P5258-21
Misc : 4.27g/10mL/MSVOA_W/SoIL/A
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
E28Y4

Manual IntegrationsAPPROVED

Quant Time: Dec 18 00:20:14 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_W\Method\SFAMWLM121324SMA.M
Quant Title : SFAM01.0
QLast Update : Wed Dec 18 00:14:15 2024
Response via : Initial Calibration

Reviewed By :Mahesh Dadoda 12/18/2024
Supervised By :Semsettin Yesilyurt 12/18/2024

