

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121819\
Quantitation Report (Qedit)




Data File : VW014438.D
Acq On : 18 Dec 2019 17:37
Operator : SY/VA
Sample : K6257-20
Misc : 4.84G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFEW8

Manual Integrations
APPROVED

MMDadoda
12/19/2019 2:01:55 PM

Quant Time: Dec 19 01:11:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 19 01:06:45 2019
Response via : Initial Calibration

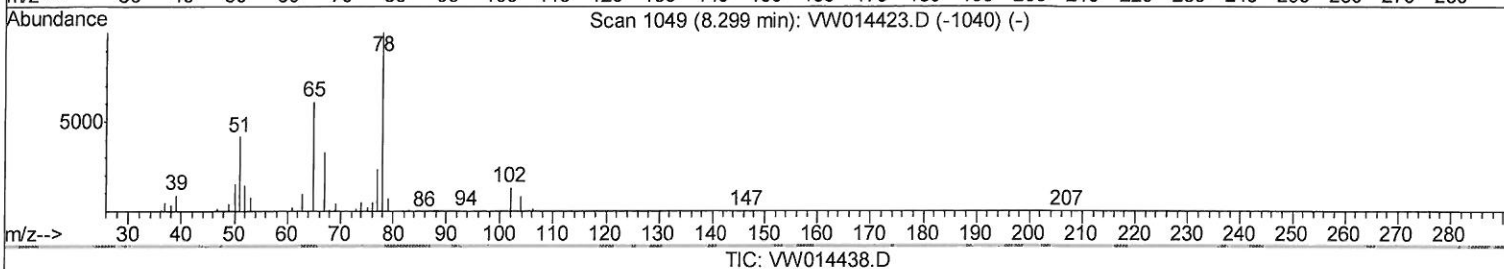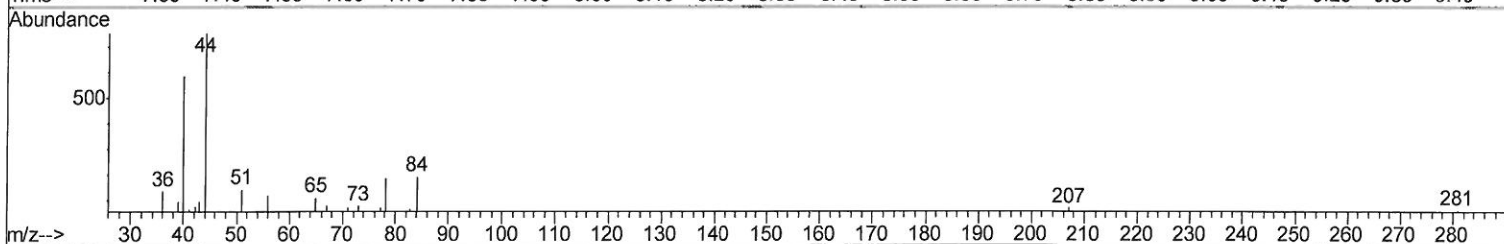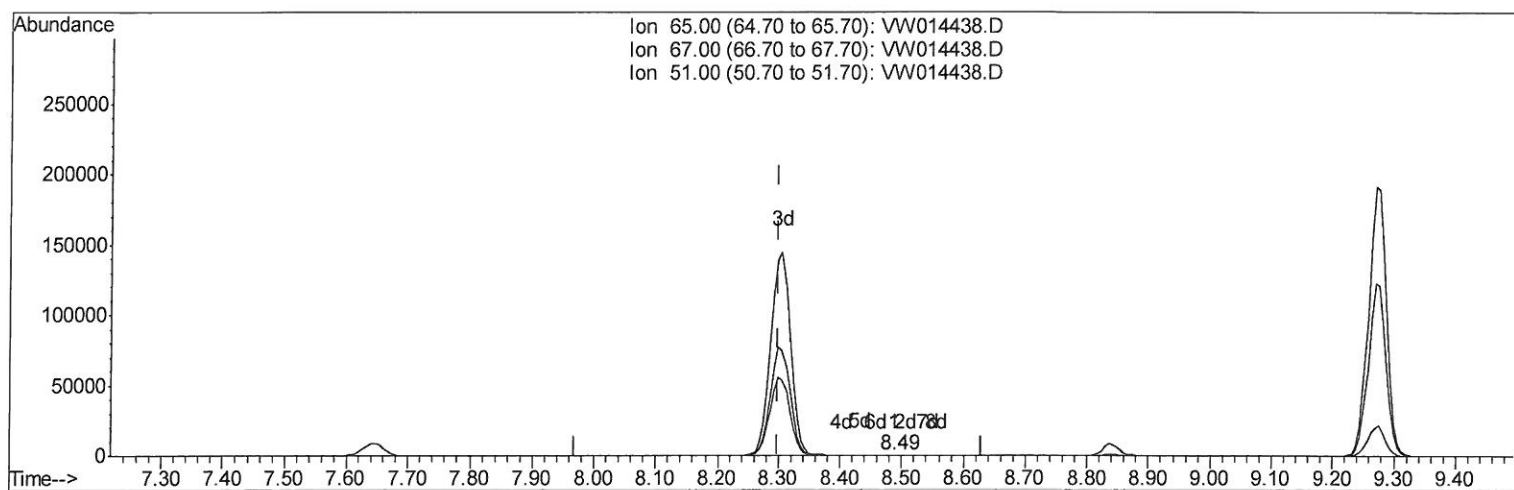

TIC: VW014438.D

(26) 1,2-Dichloroethane-d4 (S)

8.488min (+0.189) 0.01ug/L

response 118

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	64.41
51.00	107.20	109.32
0.00	0.00	0.00

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121819\
Quantitation Report (Qedit)




Data File : VW014438.D
Acq On : 18 Dec 2019 17:37
Operator : SY/VA
Sample : K6257-20
Misc : 4.84G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFEW8

Manual Integrations
APPROVED

MMDadoda
12/19/2019 2:01:55 PM

Quant Time: Dec 19 01:11:08 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 19 01:06:45 2019
Response via : Initial Calibration

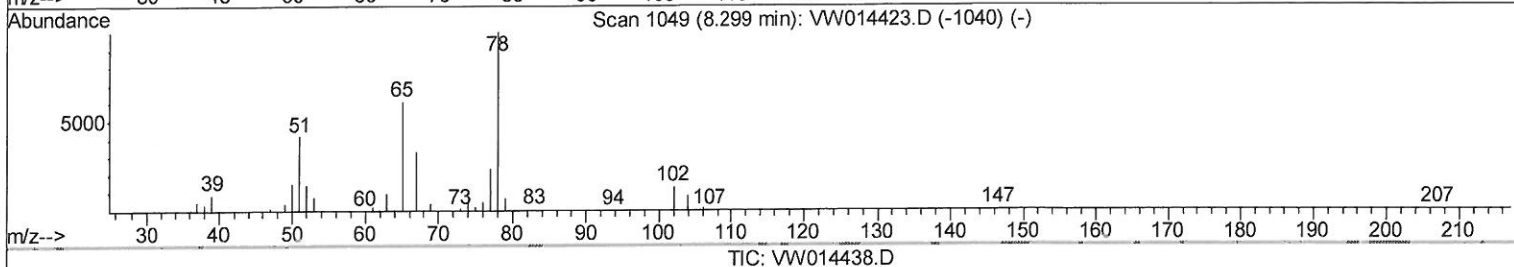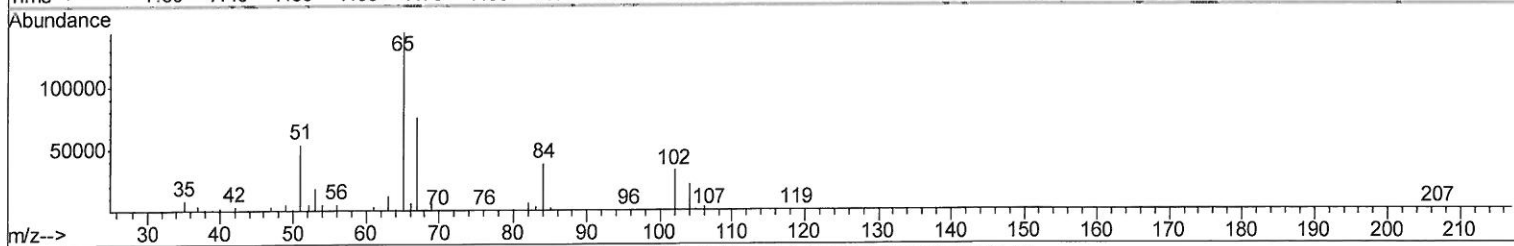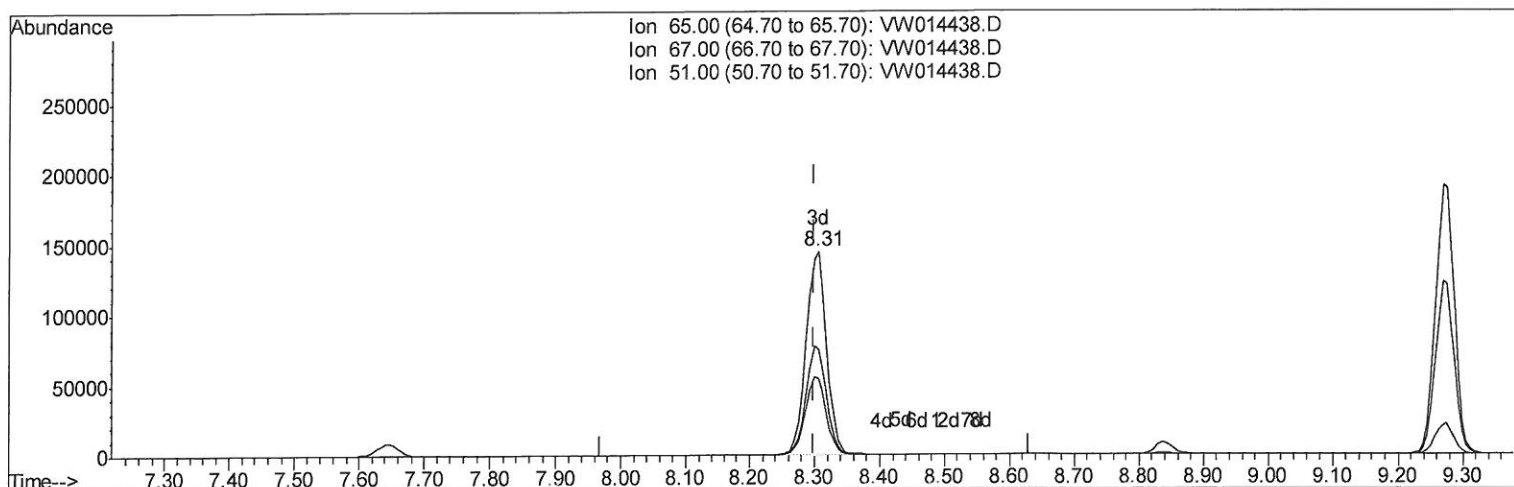

TIC: VW014438.D

(26) 1,2-Dichloroethane-d4 (S)

8.305min (+0.006) 25.29ug/L m

response 315996

Ion	Exp%	Act%
65.00	100	100
67.00	54.40	0.02#
51.00	107.20	0.04#
0.00	0.00	0.00

212/19/19 Sy

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121819\
Quantitation Report (QT Reviewed)

Data File : VW014438.D
Acq On : 18 Dec 2019 17:37
Operator : SY/VA
Sample : K6257-20
Misc : 4.84G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFEW8

Manual Integrations
APPROVED

MMDadoda
12/19/2019 2:01:55 PM

Quant Time: Dec 19 02:58:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 19 01:06:45 2019
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Difluorobenzene	8.84	114	936104	25.00	ug/L	0.00
28) Chlorobenzene-d5	11.63	117	843493	25.00	ug/L	0.00
60) 1,4-Dichlorobenzene-d4	13.55	152	327907	25.00	ug/L	0.00

System Monitoring Compounds

4) Vinyl Chloride-d3	2.35	65	267938	18.90	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	75.60%
7) Chloroethane-d5	2.89	69	235120	22.31	ug/L	0.00
Spiked Amount	25.000	Range	30 - 150	Recovery	=	89.24%
10) 1,1-Dichloroethene-d2	4.01	63	400002	15.98	ug/L	0.00
Spiked Amount	25.000	Range	45 - 110	Recovery	=	63.92%
20) 2-Butanone-d5	7.07	46	133988	36.27	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	72.54%
24) Chloroform-d	7.65	84	593013	24.88	ug/L	0.00
Spiked Amount	25.000	Range	40 - 150	Recovery	=	99.52%
26) 1,2-Dichloroethane-d4	8.31	65	315996m	25.29	ug/L	0.00
Spiked Amount	25.000	Range	70 - 130	Recovery	=	101.16%
29) Benzene-d6	8.27	84	1165185	23.57	ug/L	0.00
Spiked Amount	25.000	Range	20 - 135	Recovery	=	94.28%
33) 1,2-Dichloropropane-d6	9.27	67	385918	25.37	ug/L	0.00
Spiked Amount	25.000	Range	70 - 120	Recovery	=	101.48%
37) Toluene-d8	10.32	98	1012165	22.64	ug/L	0.00
Spiked Amount	25.000	Range	30 - 130	Recovery	=	90.56%
38) trans-1,3-Dichloropropene-	10.57	79	128495	20.14	ug/L	0.00
Spiked Amount	25.000	Range	30 - 135	Recovery	=	80.56%
39) 2-Hexanone-d5	10.92	63	106033	35.06	ug/L	0.00
Spiked Amount	50.000	Range	20 - 135	Recovery	=	70.12%
48) 1,1,2,2-Tetrachloroethane-	12.69	84	280408	22.62	ug/L	0.00
Spiked Amount	25.000	Range	45 - 120	Recovery	=	90.48%
61) 1,2-Dichlorobenzene-d4	13.85	152	307564	24.55	ug/L	0.00
Spiked Amount	25.000	Range	75 - 120	Recovery	=	98.20%

Target Compounds Qvalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

12/19/19 99

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_W\DATA\VW121819\
Quantitation Report (QT Reviewed)

Data File : VW014438.D
Acq On : 18 Dec 2019 17:37
Operator : SY/VA
Sample : K6257-20
Misc : 4.84G/10ML/MSVOA_W/SOIL
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_W
ClientSampleId :
BFEW8

Manual Integrations
APPROVED

MMDadoda
12/19/2019 2:01:55 PM

Quant Time: Dec 19 02:58:35 2019
Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_W\METHOD\SOM2WLM120519S.M
Quant Title : VOC Analysis
QLast Update : Thu Dec 19 01:06:45 2019
Response via : Initial Calibration

